


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080918\
 Data File : BF108039.D
 Acq On : 9 Aug 2018 9:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

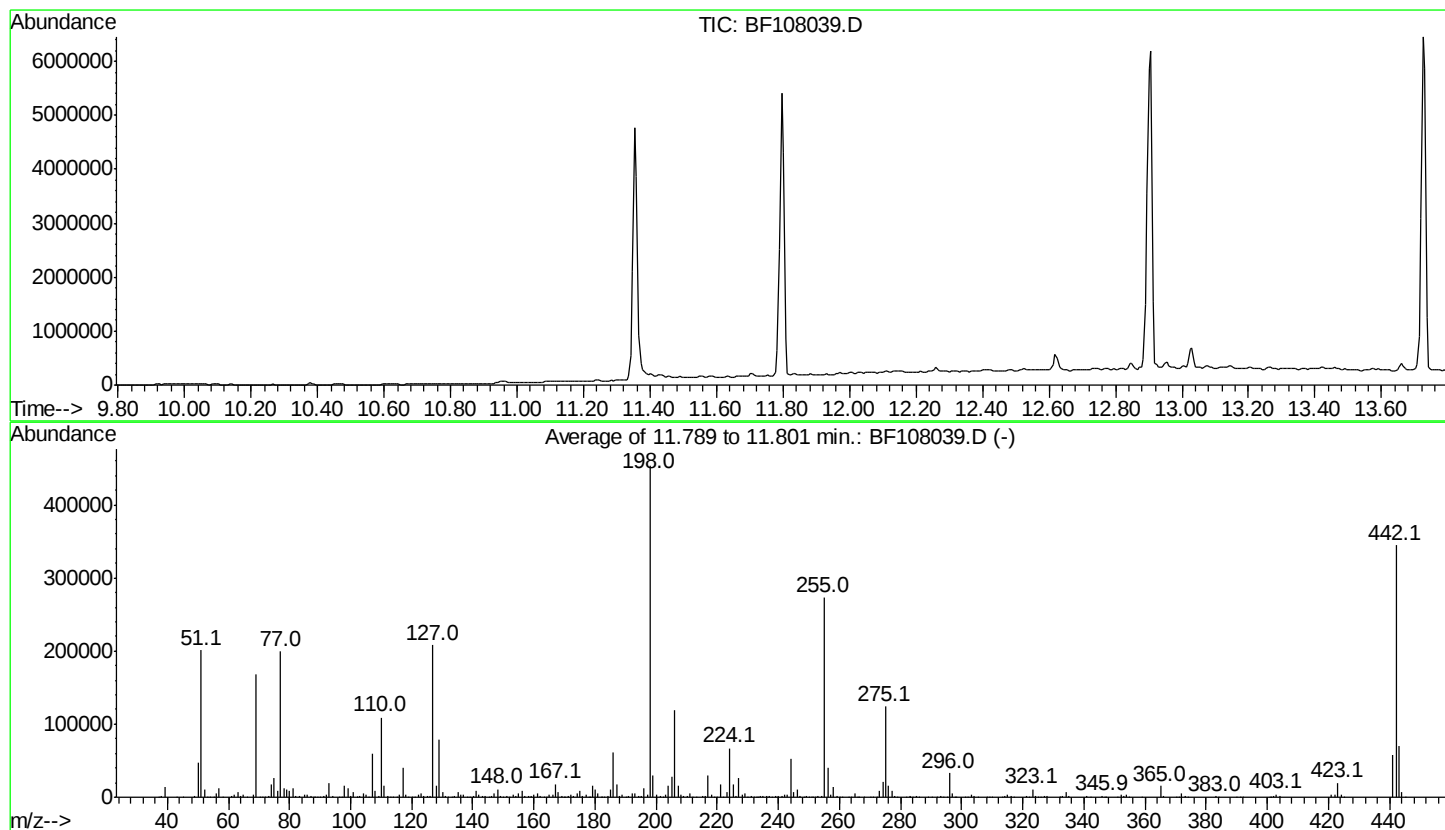

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	200826	PASS
68	69	0.00	2	1.7	2851	PASS
69	198	0.00	100	37.1	168451	PASS
70	69	0.00	2	0.4	724	PASS
127	198	10	80	45.9	208244	PASS
197	198	0.00	2	0.8	3439	PASS
198	198	100	100	100.0	453589	PASS
199	198	5	9	6.7	30347	PASS
275	198	10	60	27.3	123658	PASS
365	198	1	100	3.4	15259	PASS
441	198	0.01	100	12.7	57624	PASS
442	198	50	100	76.0	344560	PASS
443	442	15	24	20.4	70322	PASS