


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080918\
 Data File : BF108066.D
 Acq On : 9 Aug 2018 22:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

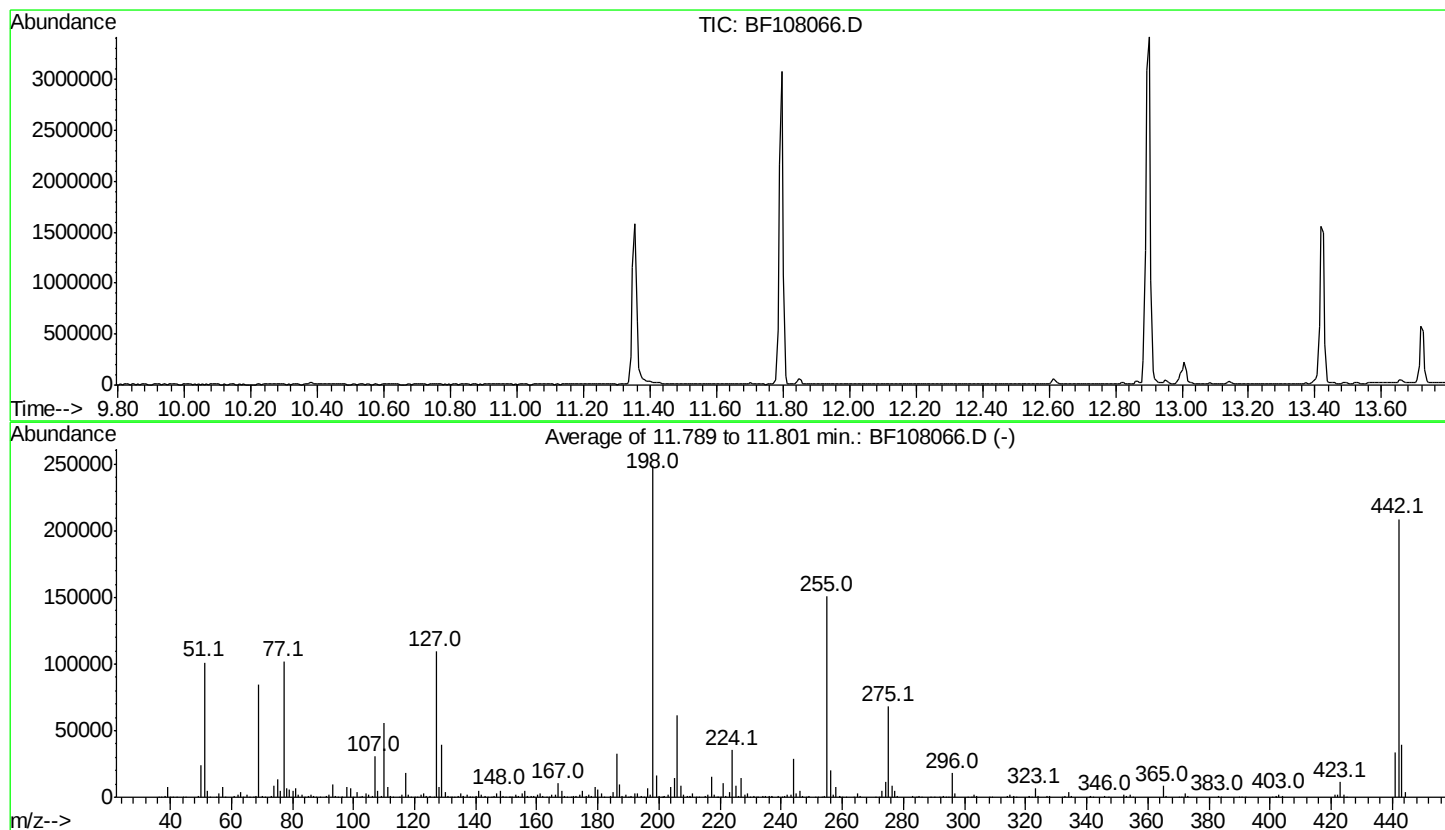

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	101170	PASS
68	69	0.00	2	1.6	1398	PASS
69	198	0.00	100	34.1	84989	PASS
70	69	0.00	2	0.6	522	PASS
127	198	10	80	43.9	109325	PASS
197	198	0.00	2	0.6	1617	PASS
198	198	100	100	100.0	248941	PASS
199	198	5	9	6.8	16816	PASS
275	198	10	60	27.3	67896	PASS
365	198	1	100	3.4	8570	PASS
441	198	0.01	100	13.7	34069	PASS
442	198	50	100	83.9	208776	PASS
443	442	15	24	19.0	39605	PASS