
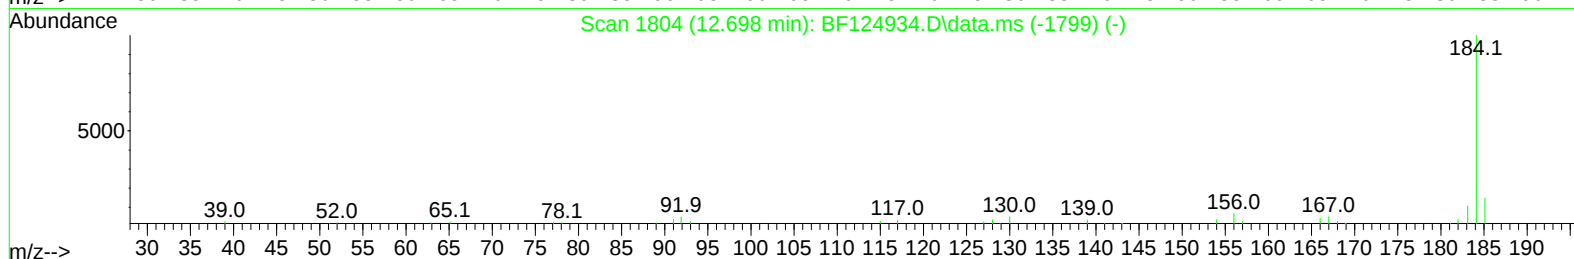
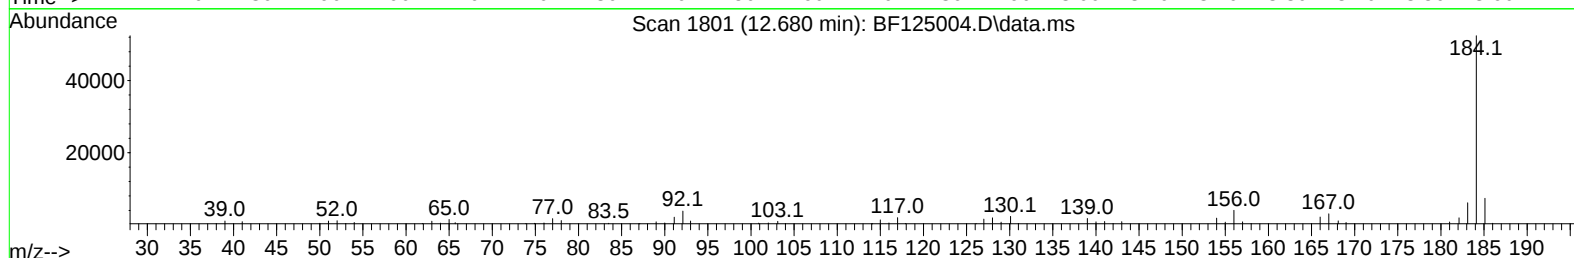


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
 Data File : BF125004.D
 Acq On : 9 Aug 2021 16:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 17:33:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 11:03:44 2021
 Response via : Initial Calibration

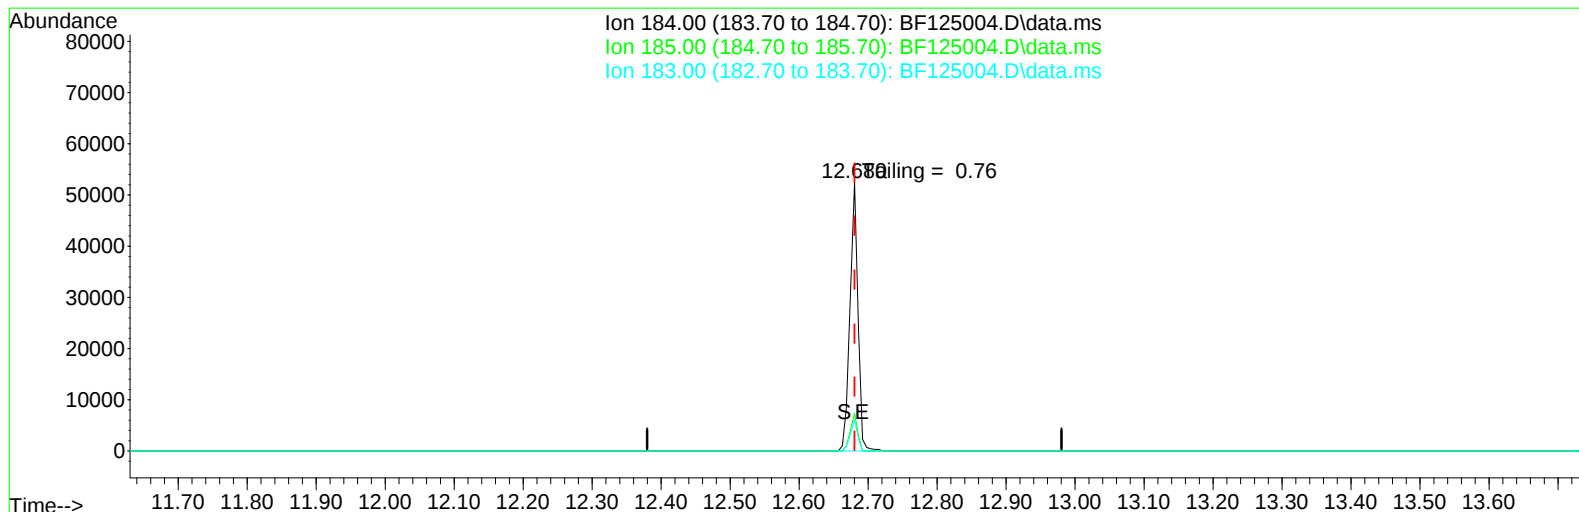

TIC: BF125004.D\data.ms

(77) Benzidine




12.680min (+ 0.000) 0.00 ng

response 42360

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.06
183.00	10.10	11.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
Data File : BF125004.D
Acq On : 9 Aug 2021 16:23
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 17:33:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 11:03:44 2021
Response via : Initial Calibration

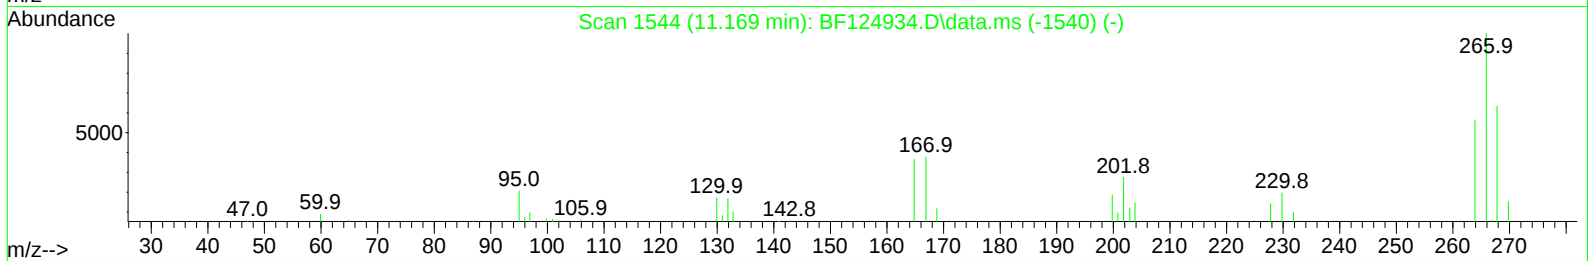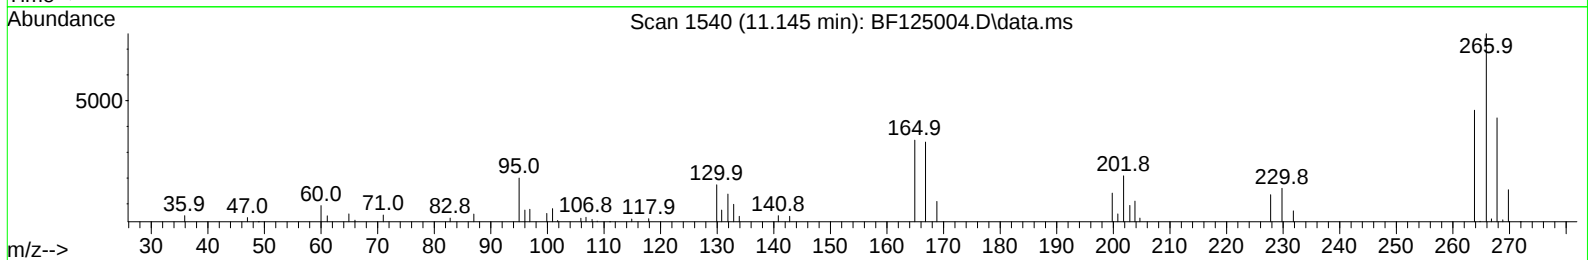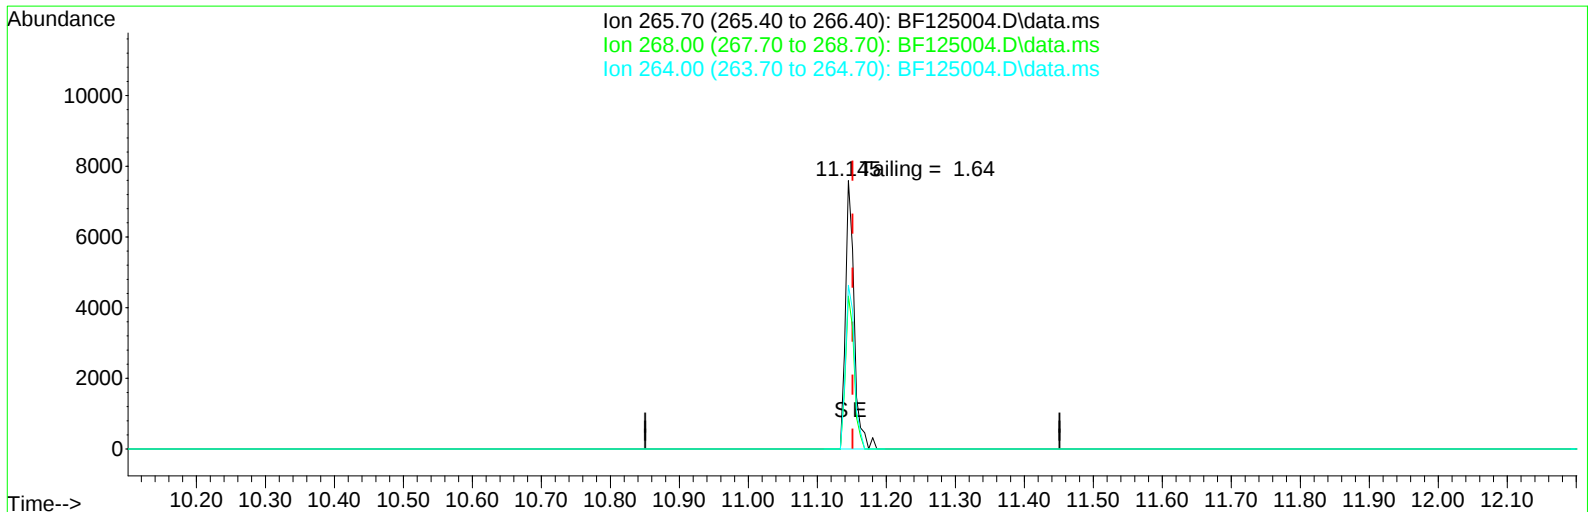

TIC: BF125004.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.006) 0.00 ng

response 6620

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	57.00
264.00	69.90	60.98
0.00	0.00	0.00