

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
 Data File : BF125006.D
 Acq On : 9 Aug 2021 17:29
 Operator : JU/CG
 Sample : PB138266BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138266BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	567	572	575	rBV	236105	219414	69.01%	12.741%
2	6.457	737	743	745	rBV	212767	225866	71.04%	13.116%
3	6.816	801	804	807	rBB	55535	43568	13.70%	2.530%
4	7.381	895	900	903	rBV	134892	147431	46.37%	8.561%
5	8.098	1018	1022	1026	rBB	63422	59117	18.59%	3.433%
6	9.175	1200	1205	1208	rBV	273828	288432	90.71%	16.749%
7	9.857	1316	1321	1324	rBB	77991	70094	22.04%	4.070%
8	10.645	1450	1455	1458	rBV	190176	166886	52.49%	9.691%
9	11.339	1570	1573	1577	rBV	84524	72476	22.79%	4.209%
10	12.927	1839	1843	1846	rBV	316176	317962	100.00%	18.464%
11	13.845	1996	1999	2001	rBB	3826	3457	1.09%	0.201%
12	13.980	2018	2022	2025	rBV	67524	57478	18.08%	3.338%
13	15.433	2264	2269	2274	rBB	39941	46386	14.59%	2.694%
14	15.868	2339	2343	2347	rBB2	2739	3498	1.10%	0.203%




Sum of corrected areas: 1722065

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
Data File : BF125006.D
Acq On : 9 Aug 2021 17:29
Operator : JU/CG
Sample : PB138266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138266BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

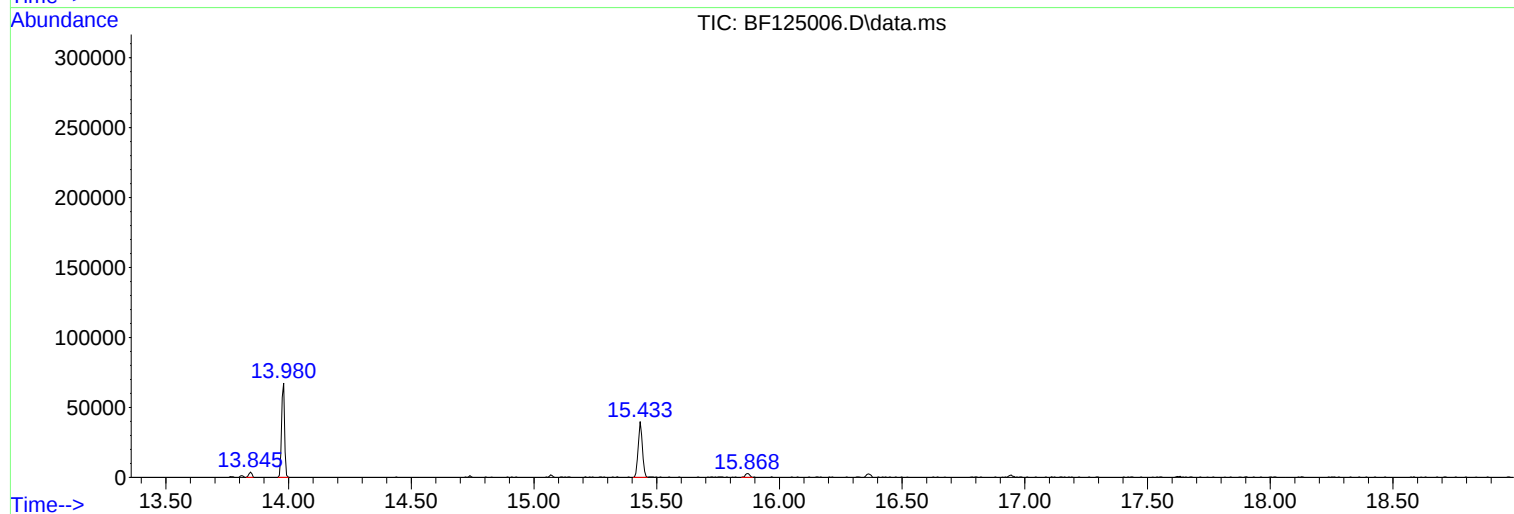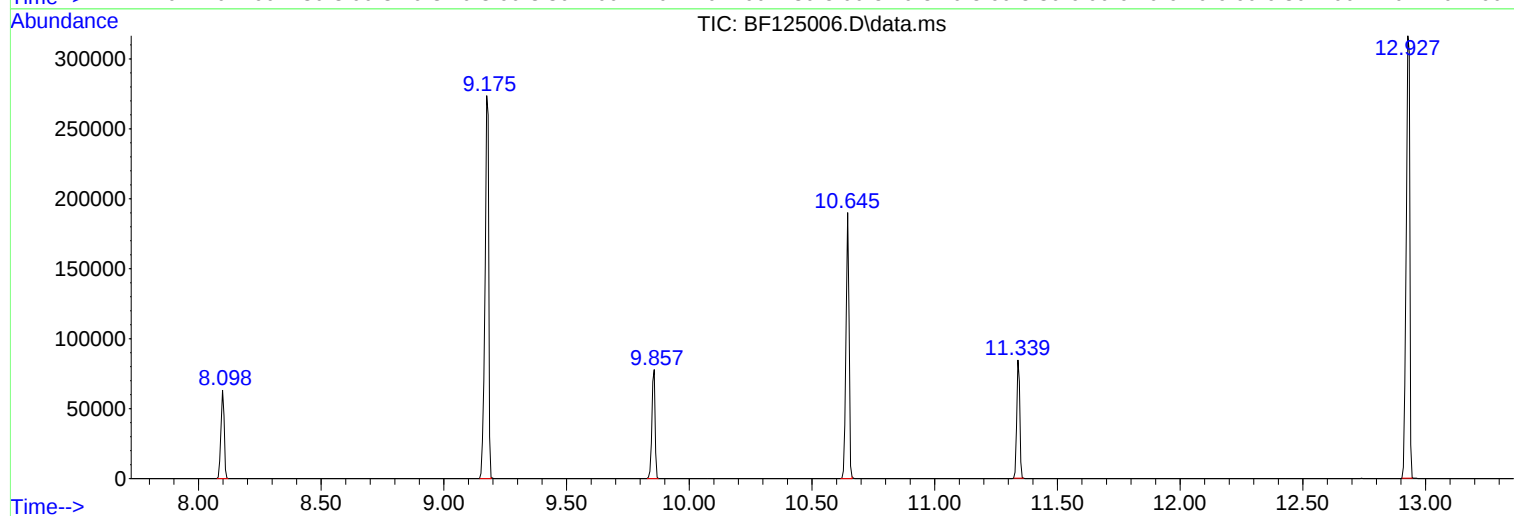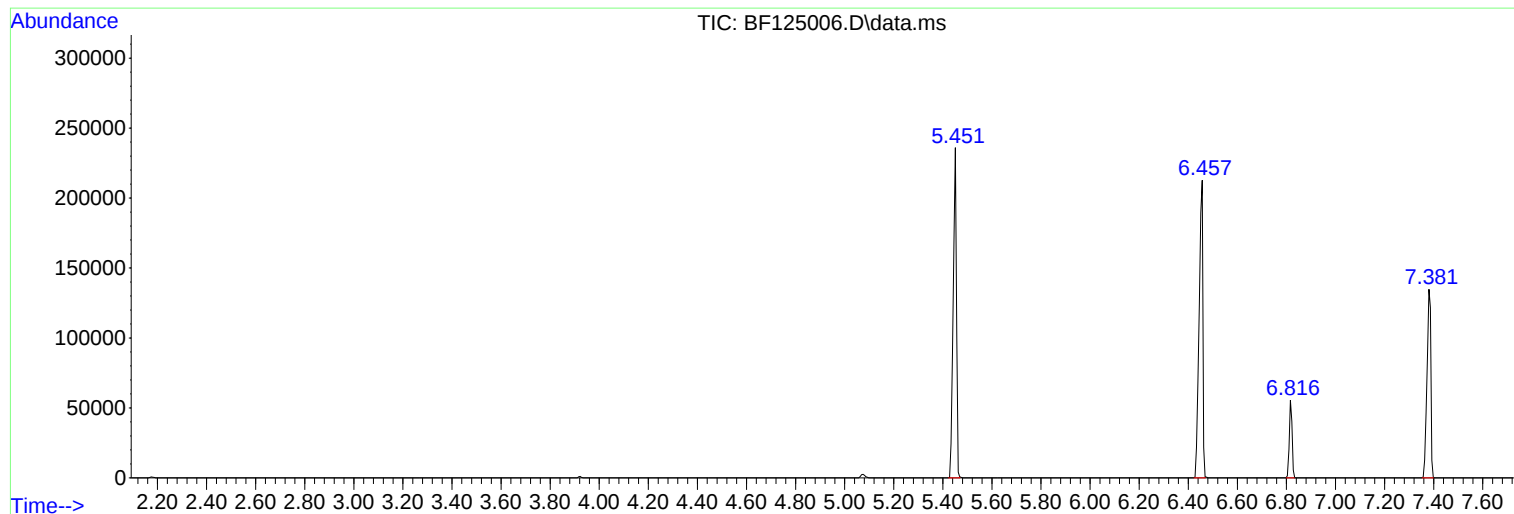

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
Data File : BF125006.D
Acq On : 9 Aug 2021 17:29
Operator : JU/CG
Sample : PB138266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138266BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080921\
Data File : BF125006.D
Acq On : 9 Aug 2021 17:29
Operator : JU/CG
Sample : PB138266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138266BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------