
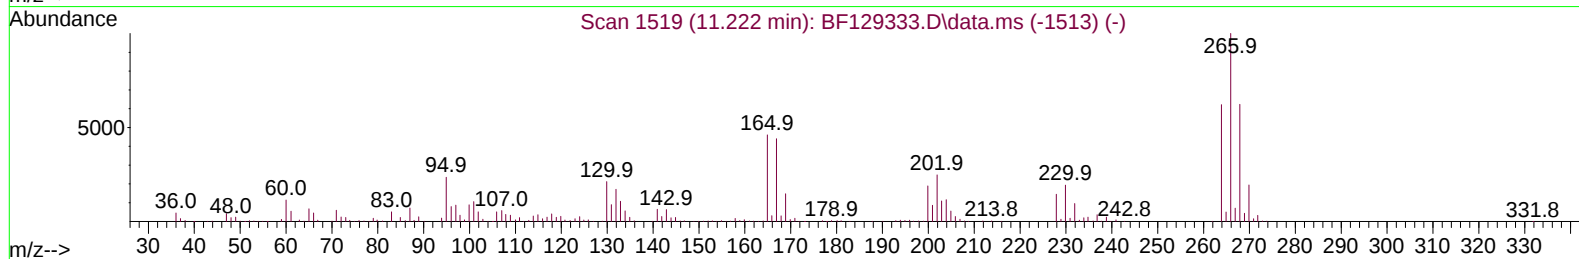
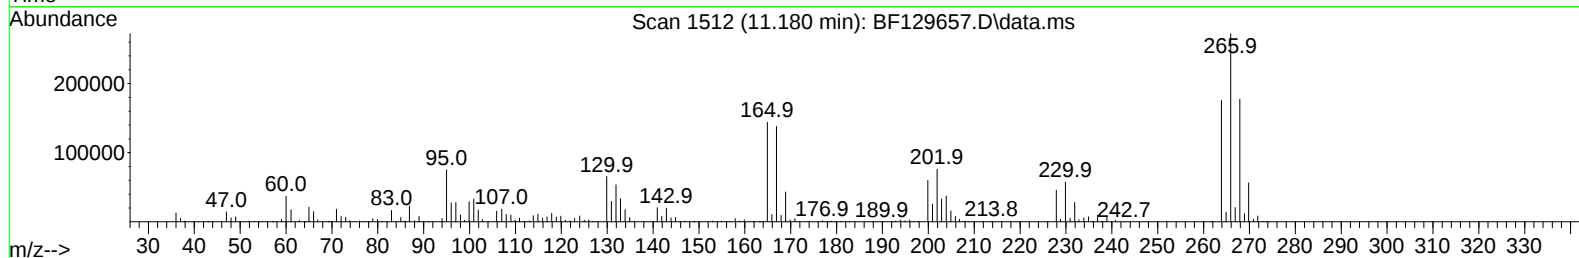


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
Data File : BF129657.D
Acq On : 09 Aug 2022 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 16:32:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

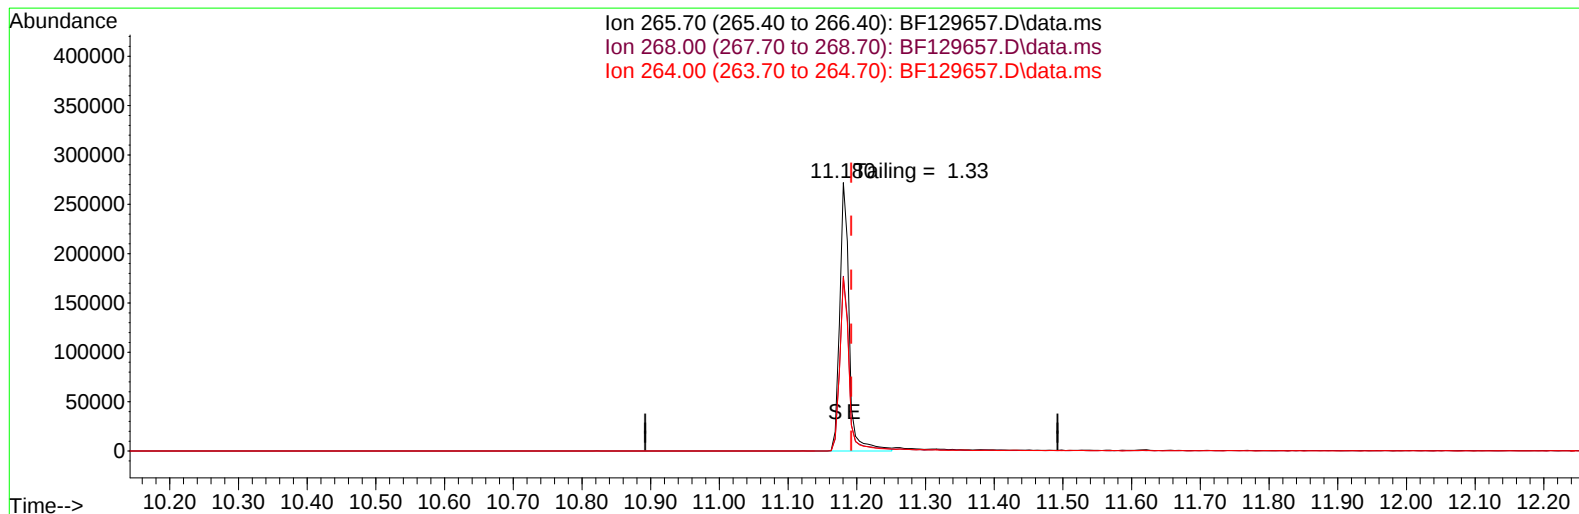

TIC: BF129657.D\data.ms

(70) Pentachlorophenol (C)




11.180min (-0.012) 202493.75 ng

response 261224

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.12
264.00	61.80	64.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129657.D
 Acq On : 09 Aug 2022 09:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 16:32:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 16:27:34 2022
 Response via : Initial Calibration

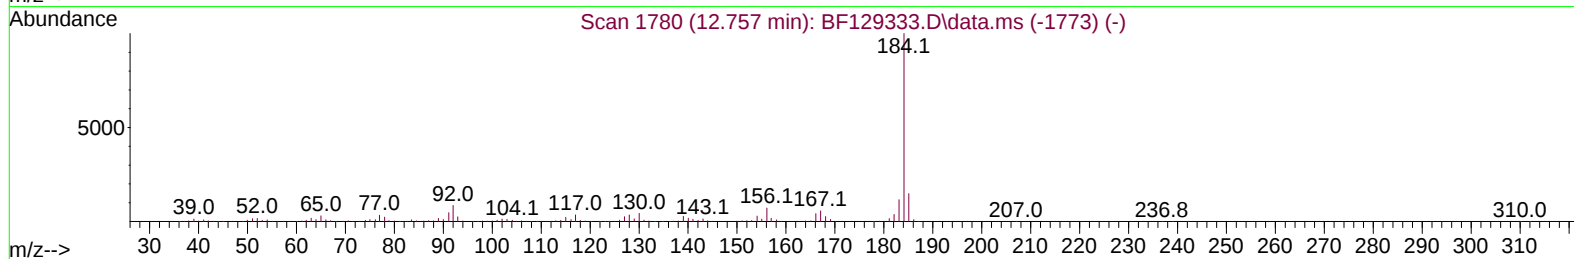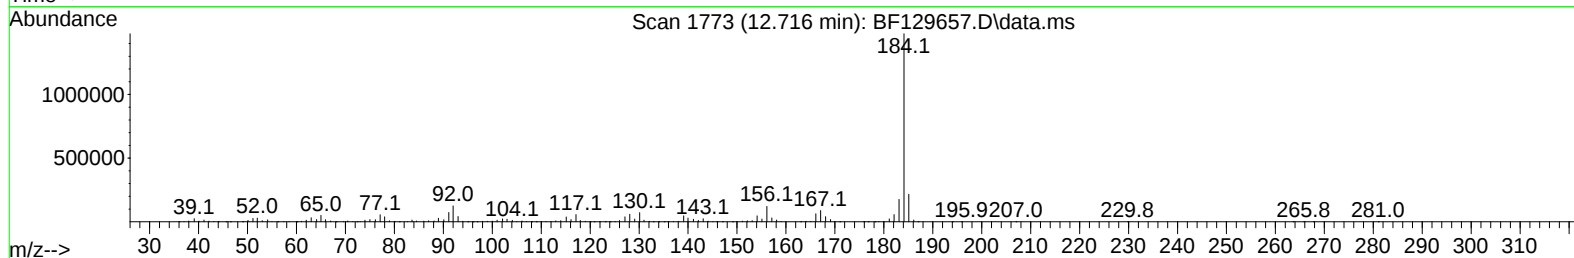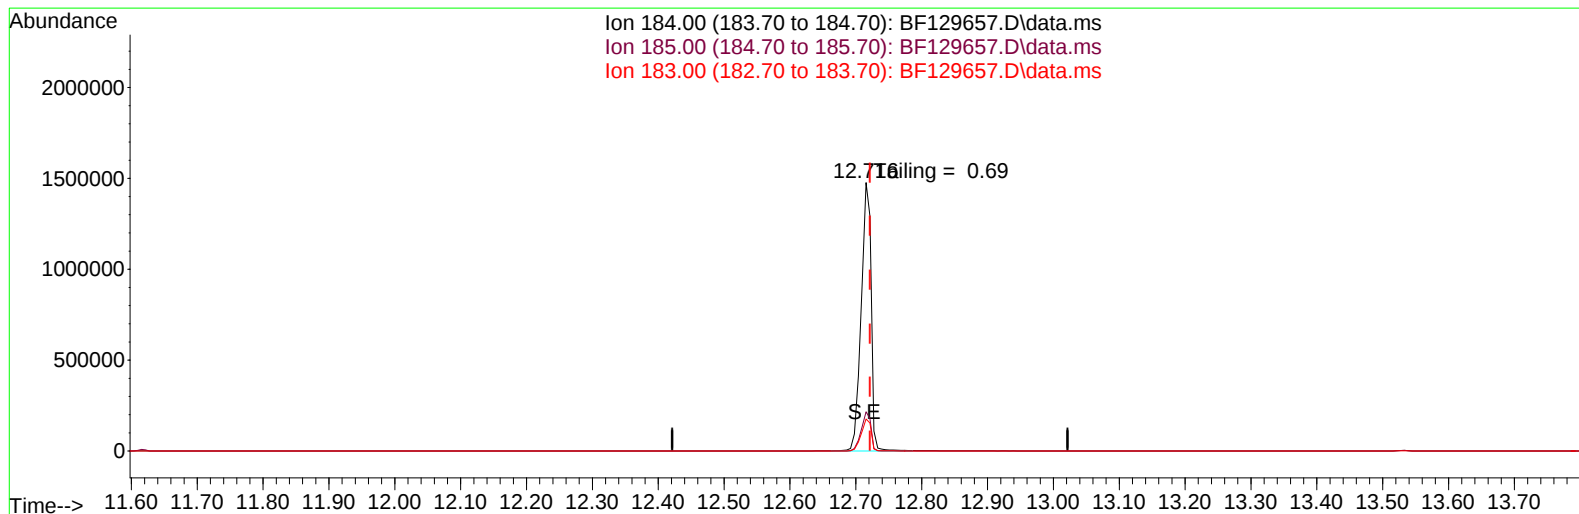

TIC: BF129657.D\data.ms

(77) Benzidine**12.716min (-0.006) 94484.03 ng****response 1558793**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.63
183.00	11.60	11.96
0.00	0.00	0.00