

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129687.D
 Acq On : 10 Aug 2022 02:45
 Operator : CG\JU
 Sample : N4088-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	539	544	556	rBV	3514994	3496137	56.29%	4.117%
2	6.498	711	716	719	rBV	3679773	3368549	54.23%	3.967%
3	6.840	770	774	778	rBV	1359857	1053898	16.97%	1.241%
4	7.410	866	871	874	rBV	2186878	2128797	34.27%	2.507%
5	8.122	988	992	995	rBV	1545090	1275612	20.54%	1.502%
6	9.198	1170	1175	1178	rBV	4485635	3607531	58.08%	4.248%
7	9.457	1216	1219	1224	rVB2	95789	105848	1.70%	0.125%
8	9.534	1229	1232	1235	rVV	95731	96886	1.56%	0.114%
9	9.739	1264	1267	1272	rVV	251765	218089	3.51%	0.257%
10	9.787	1272	1275	1280	rVB5	47083	67529	1.09%	0.080%
11	9.881	1288	1291	1294	rBV	1516666	1140153	18.36%	1.343%
12	9.910	1294	1296	1300	rVB	357443	288552	4.65%	0.340%
13	9.987	1305	1309	1312	rBV3	45766	64196	1.03%	0.076%
14	10.081	1322	1325	1329	rBV2	207881	202443	3.26%	0.238%
15	10.122	1329	1332	1336	rVB	79429	76505	1.23%	0.090%
16	10.192	1341	1344	1347	rBV2	93438	110646	1.78%	0.130%
17	10.298	1356	1362	1365	rBV4	64238	120597	1.94%	0.142%
18	10.428	1381	1384	1390	rVB	401018	359033	5.78%	0.423%
19	10.516	1397	1399	1401	rVB	89376	67733	1.09%	0.080%
20	10.586	1405	1411	1414	rVB3	108480	136370	2.20%	0.161%
21	10.675	1422	1426	1429	rBV	2117401	1783972	28.72%	2.101%
22	10.775	1439	1443	1451	rVB5	151412	316627	5.10%	0.373%
23	10.975	1473	1477	1480	rBV3	126120	152586	2.46%	0.180%
24	11.057	1489	1491	1494	rVB	74481	64432	1.04%	0.076%
25	11.104	1494	1499	1501	rBV3	109865	153491	2.47%	0.181%
26	11.128	1501	1503	1508	rVV2	126219	146960	2.37%	0.173%
27	11.175	1508	1511	1515	rVV	265536	268397	4.32%	0.316%
28	11.216	1515	1518	1521	rVV	220550	221225	3.56%	0.261%
29	11.269	1525	1527	1531	rVB	214150	184661	2.97%	0.217%
30	11.375	1541	1545	1546	rBV	1026645	961727	15.48%	1.133%
31	11.398	1546	1549	1552	rVV	3773302	3129457	50.38%	3.685%
32	11.445	1552	1557	1560	rVV	1179327	1082703	17.43%	1.275%
33	11.481	1560	1563	1566	rVB2	112786	122633	1.97%	0.144%
34	11.604	1579	1584	1588	rBV2	344277	433959	6.99%	0.511%
35	11.645	1588	1591	1592	rVV	158355	132722	2.14%	0.156%
36	11.663	1592	1594	1598	rVV	142737	161285	2.60%	0.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129687.D
 Acq On : 10 Aug 2022 02:45
 Operator : CG\JU
 Sample : N4088-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.704	1598	1601	1605	rVB3	149582	165441	2.66%	0.195%
38	11.751	1605	1609	1612	rBV	1052922	897694	14.45%	1.057%
39	11.781	1612	1614	1617	rVB	65752	63063	1.02%	0.074%
40	11.875	1626	1630	1632	rBV	640853	569814	9.17%	0.671%
41	11.898	1632	1634	1638	rVV	1066545	1009770	16.26%	1.189%
42	11.951	1640	1643	1646	rVV	334328	306286	4.93%	0.361%
43	11.986	1646	1649	1651	rVV	1071023	1084694	17.46%	1.277%
44	12.010	1651	1653	1657	rVB	462665	371058	5.97%	0.437%
45	12.051	1657	1660	1663	rBV	205557	187916	3.03%	0.221%
46	12.104	1667	1669	1673	rVV2	95991	100054	1.61%	0.118%
47	12.169	1677	1680	1682	rVV	480031	425835	6.86%	0.501%
48	12.198	1682	1685	1689	rVB	462603	400129	6.44%	0.471%
49	12.316	1700	1705	1708	rBV2	171508	230459	3.71%	0.271%
50	12.351	1708	1711	1713	rVV	171282	151843	2.44%	0.179%
51	12.375	1713	1715	1718	rVB	151798	115176	1.85%	0.136%
52	12.439	1720	1726	1728	rBV2	3054727	3254769	52.40%	3.833%
53	12.463	1728	1730	1732	rVV	3471540	2824315	45.47%	3.326%
54	12.522	1736	1740	1742	rBV2	489023	592422	9.54%	0.698%
55	12.545	1742	1744	1748	rVB	618183	487193	7.84%	0.574%
56	12.598	1748	1753	1756	rBV	5663999	6188666	99.63%	7.288%
57	12.633	1756	1759	1761	rVV	150348	165711	2.67%	0.195%
58	12.651	1761	1762	1765	rVB	183743	142808	2.30%	0.168%
59	12.686	1765	1768	1770	rBV2	160274	152493	2.46%	0.180%
60	12.739	1773	1777	1780	rVV2	196090	254226	4.09%	0.299%
61	12.769	1780	1782	1786	rVV4	79731	96450	1.55%	0.114%
62	12.833	1786	1793	1796	rVB2	4729290	6211455	100.00%	7.315%
63	12.869	1796	1799	1803	rVB2	354930	354378	5.71%	0.417%
64	12.957	1807	1814	1817	rBV2	3044139	3208535	51.66%	3.779%
65	12.980	1817	1818	1822	rVB	295780	228385	3.68%	0.269%
66	13.039	1823	1828	1832	rBV2	475099	839909	13.52%	0.989%
67	13.151	1844	1847	1849	rVB	821757	792489	12.76%	0.933%
68	13.175	1849	1851	1853	rBV2	98098	85405	1.37%	0.101%
69	13.216	1855	1858	1860	rVB	525594	407851	6.57%	0.480%
70	13.257	1860	1865	1867	rBV2	646406	785495	12.65%	0.925%
71	13.310	1872	1874	1877	rVB2	142627	110505	1.78%	0.130%
72	13.345	1877	1880	1883	rBV	361467	376491	6.06%	0.443%
73	13.380	1883	1886	1888	rBV	396645	360471	5.80%	0.425%
74	13.516	1907	1909	1912	rBV4	114502	152136	2.45%	0.179%
75	13.663	1931	1934	1938	rVB	647656	575816	9.27%	0.678%
76	13.769	1949	1952	1955	rBV	579324	592062	9.53%	0.697%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129687.D
 Acq On : 10 Aug 2022 02:45
 Operator : CG\JU
 Sample : N4088-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	13.798	1955	1957	1959	rVV	575467	431548	6.95%	0.508%
78	13.827	1959	1962	1966	rVV2	415586	660622	10.64%	0.778%
79	13.874	1966	1970	1973	rVB	656266	707405	11.39%	0.833%
80	13.939	1979	1981	1987	rVB	207540	223480	3.60%	0.263%
81	14.016	1990	1994	1998	rVV2	2867330	4176195	67.23%	4.918%
82	14.057	1998	2001	2006	rVB	2752856	2561676	41.24%	3.017%
83	14.116	2008	2011	2012	rBV2	452858	415594	6.69%	0.489%
84	14.174	2019	2021	2027	rVB4	200738	220178	3.54%	0.259%
85	14.239	2030	2032	2033	rBV	148115	99219	1.60%	0.117%
86	14.280	2037	2039	2042	rBV2	152601	171140	2.76%	0.202%
87	14.369	2052	2054	2056	rBV	238909	228924	3.69%	0.270%
88	14.410	2059	2061	2064	rVV	554472	447002	7.20%	0.526%
89	14.445	2064	2067	2069	rVV	235075	195771	3.15%	0.231%
90	14.533	2080	2082	2084	rBV	208248	178174	2.87%	0.210%
91	14.557	2084	2086	2089	rVB	287961	243995	3.93%	0.287%
92	14.904	2142	2145	2153	rVB2	271018	433716	6.98%	0.511%
93	15.080	2170	2175	2177	rBV	1899834	2874783	46.28%	3.386%
94	15.180	2189	2192	2196	rVB	488144	521022	8.39%	0.614%
95	15.380	2222	2226	2232	rVB	1092351	1452980	23.39%	1.711%
96	15.451	2233	2238	2241	rVV	1718401	2136644	34.40%	2.516%
97	15.504	2244	2247	2250	rVV	489130	677364	10.91%	0.798%
98	15.539	2250	2253	2260	rVB2	507378	699299	11.26%	0.824%
99	17.004	2497	2502	2509	rVB	750193	1515310	24.40%	1.785%
100	17.462	2575	2580	2589	rVB	485796	1020919	16.44%	1.202%




Sum of corrected areas: 84914569

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
Data File : BF129687.D
Acq On : 10 Aug 2022 02:45
Operator : CG\JU
Sample : N4088-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-02-080522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

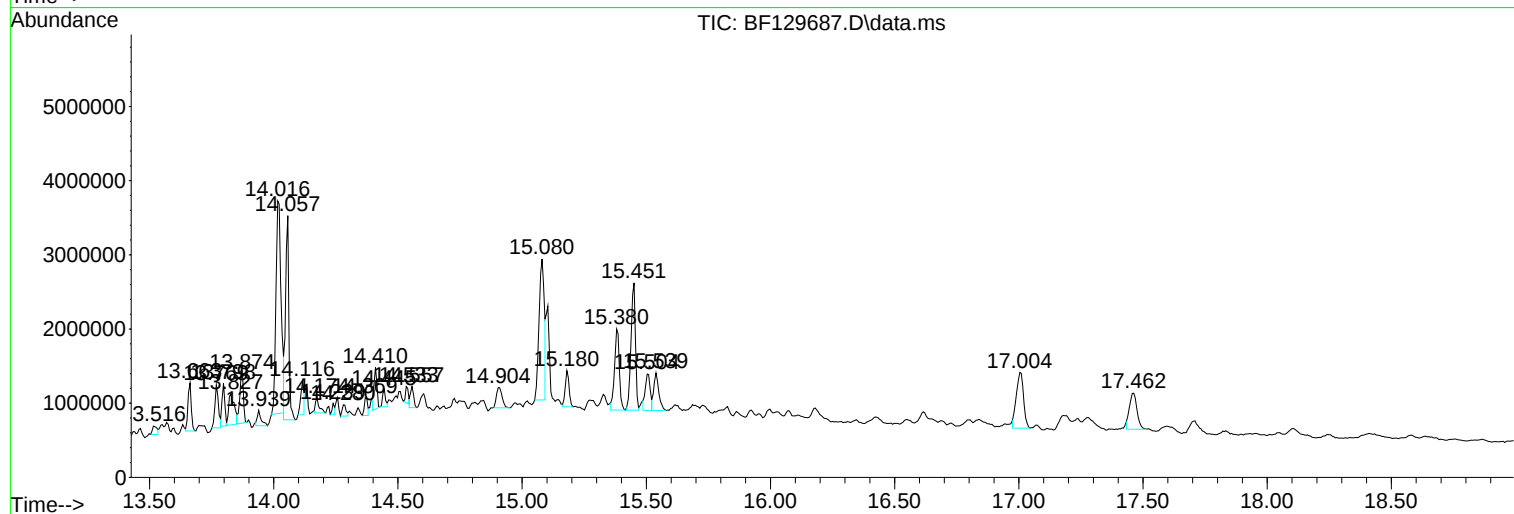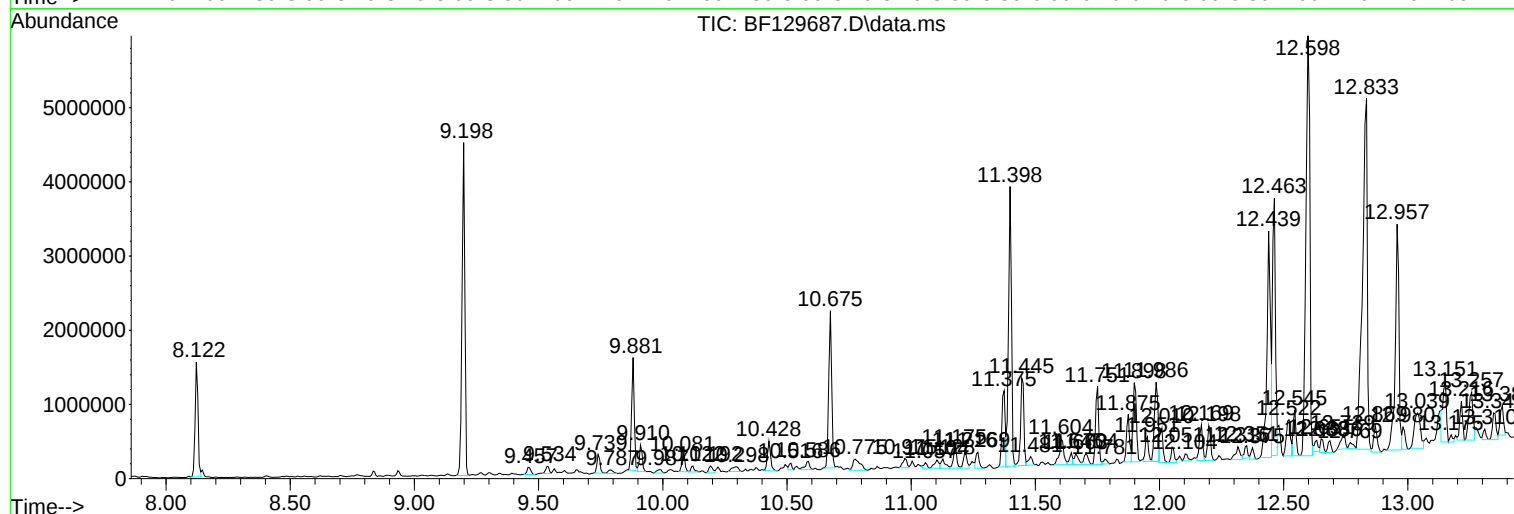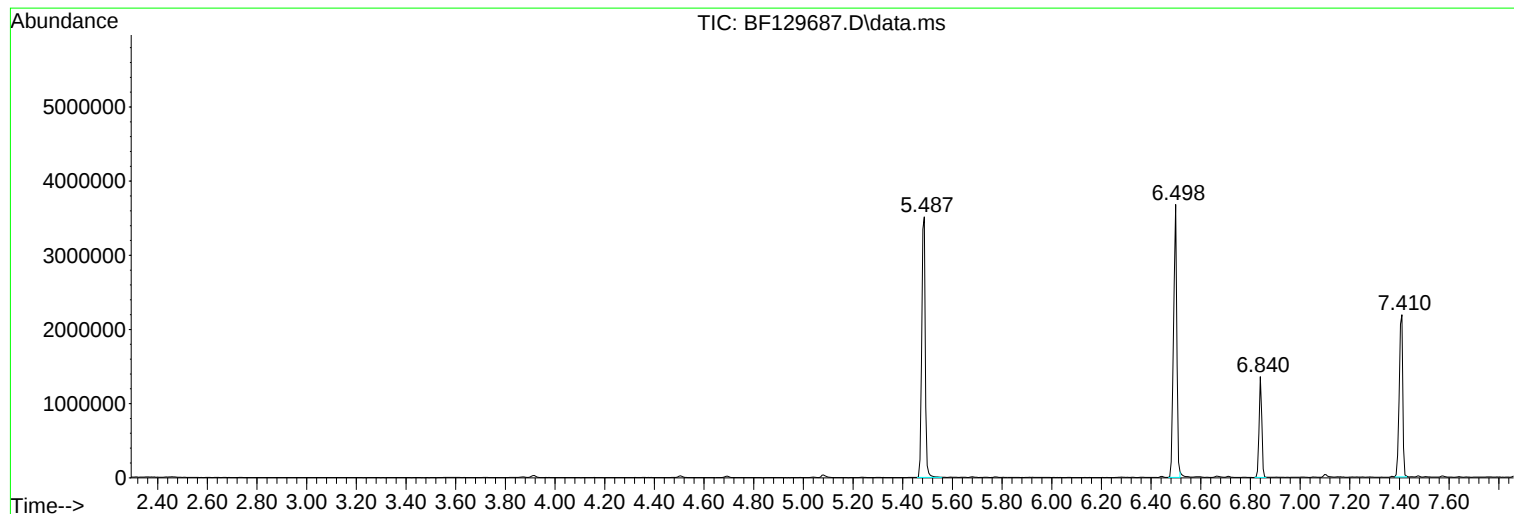

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
Data File : BF129687.D
Acq On : 10 Aug 2022 02:45
Operator : CG\JU
Sample : N4088-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-02-080522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
Data File : BF129687.D
Acq On : 10 Aug 2022 02:45
Operator : CG\JU
Sample : N4088-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-02-080522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------