
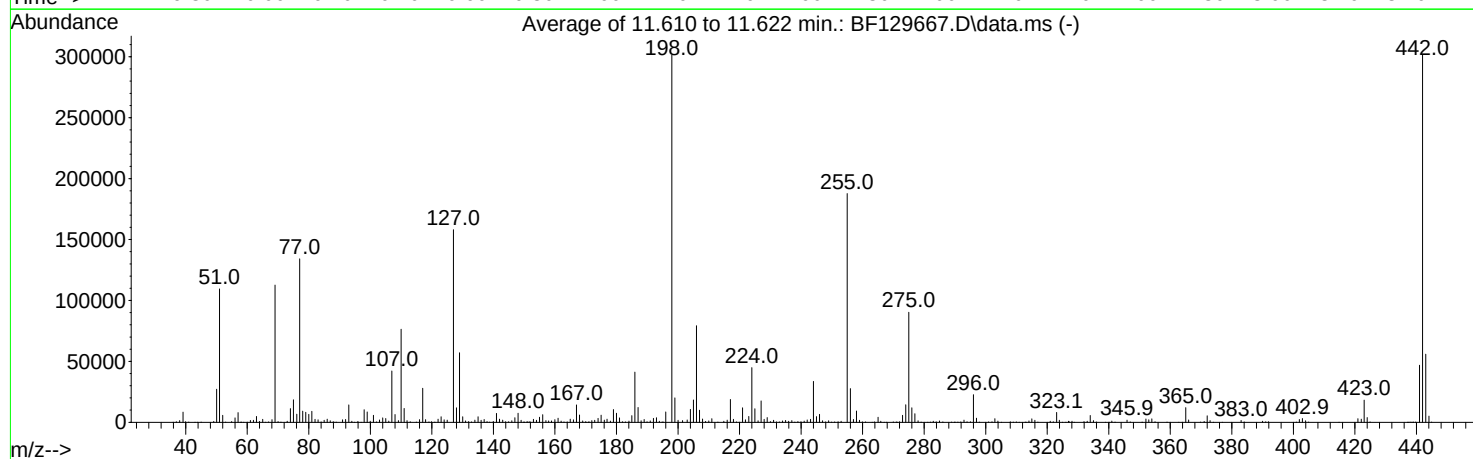


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129667.D
 Acq On : 09 Aug 2022 15:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 16:27:34 2022

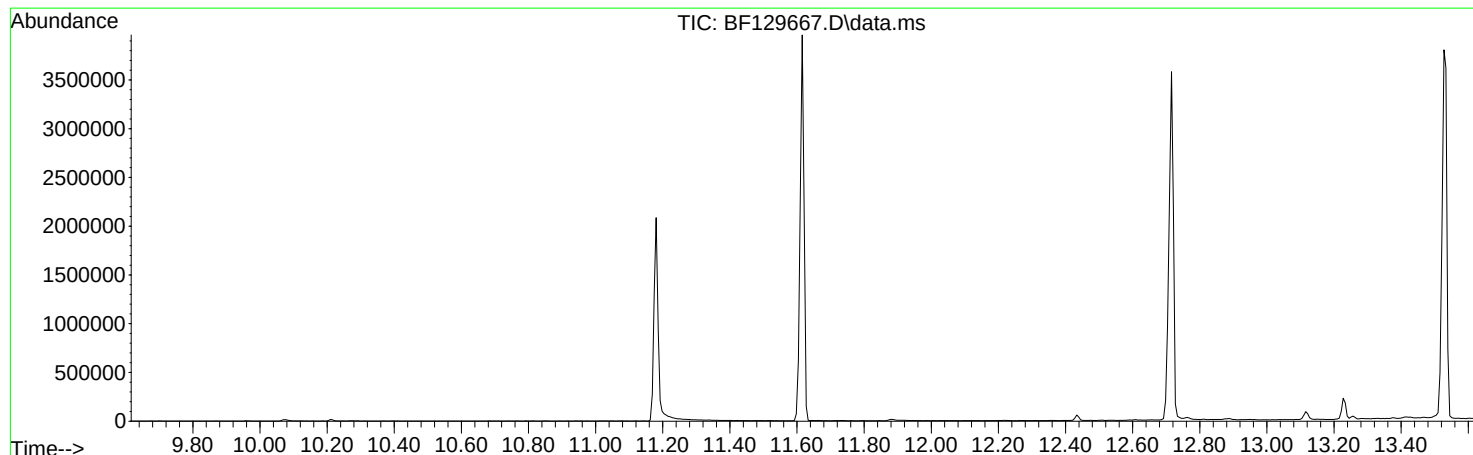




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	109493	PASS
68	69	0.00	2	1.9	2130	PASS
69	198	0.00	100	37.4	112605	PASS
70	69	0.00	2	0.5	617	PASS
127	198	10	80	52.4	158008	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	301291	PASS
199	198	5	9	6.6	19987	PASS
275	198	10	60	30.0	90301	PASS
365	198	1	100	4.0	12055	PASS
441	198	0.01	100	15.5	46840	PASS
442	442	50	100	100.0	301931	PASS
443	442	15	24	18.5	55880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
 Data File : BF129667.D
 Acq On : 09 Aug 2022 15:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 09 16:29:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 16:27:34 2022
 Response via : Initial Calibration

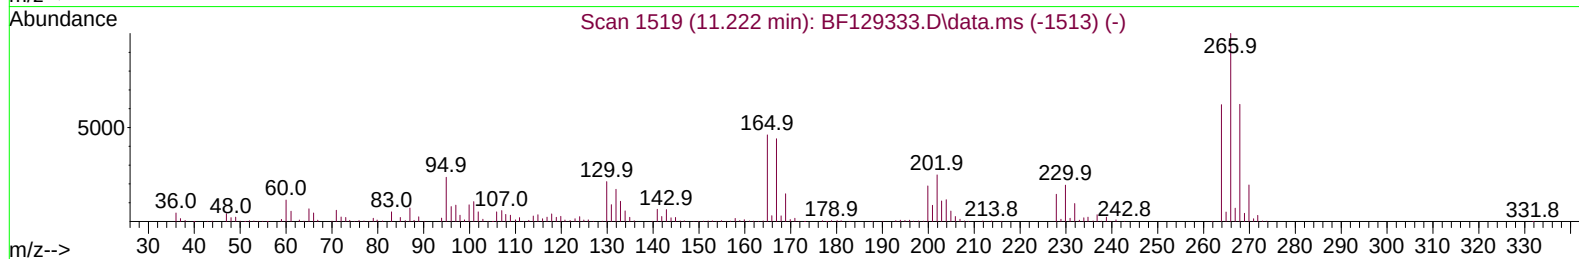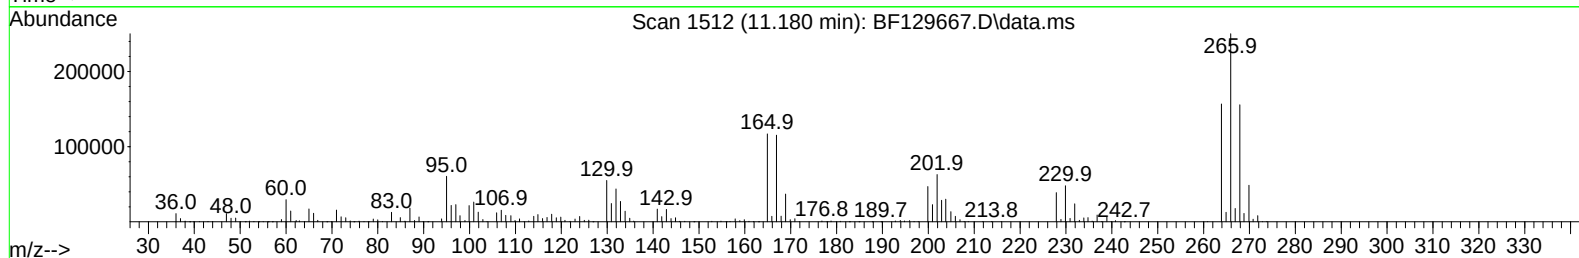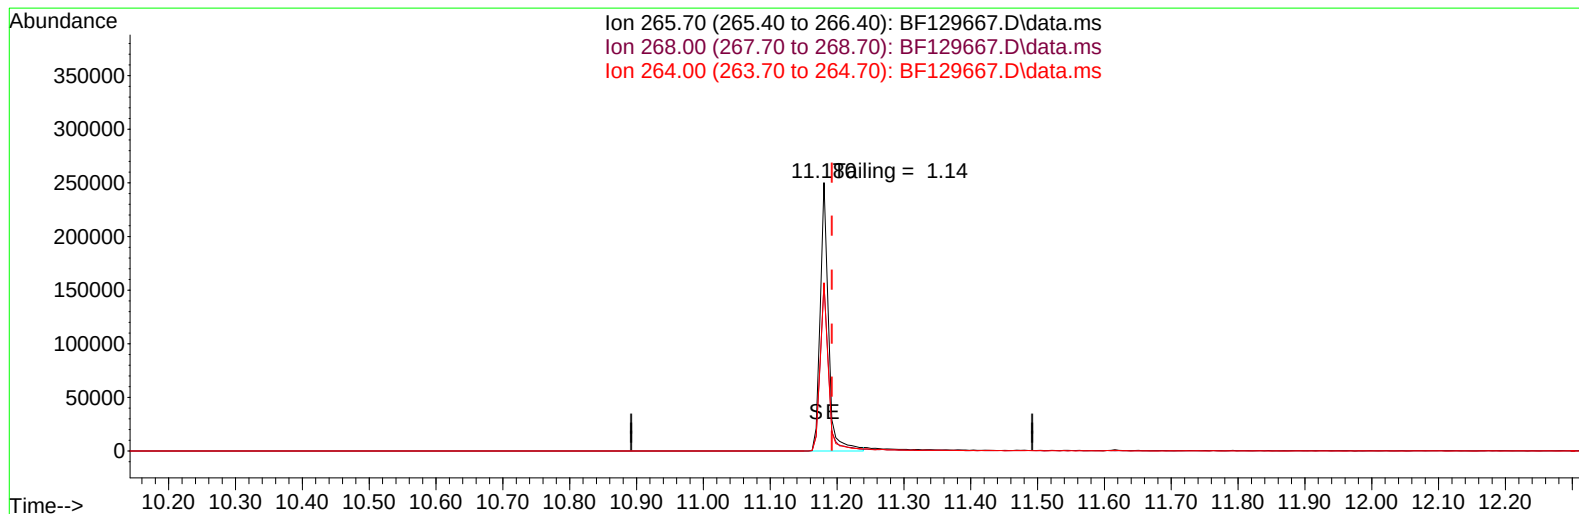

TIC: BF129667.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.012) 125304.05 ng




response 225497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.28
264.00	61.80	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080922\
Data File : BF129667.D
Acq On : 09 Aug 2022 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 16:29:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

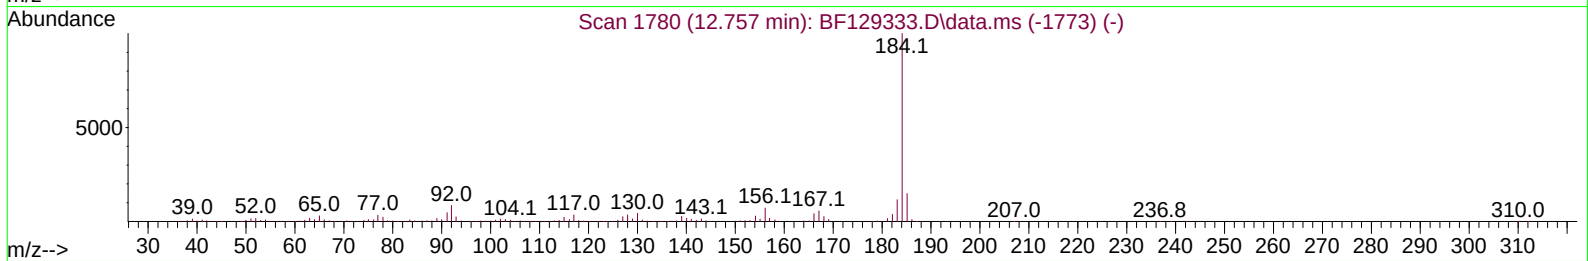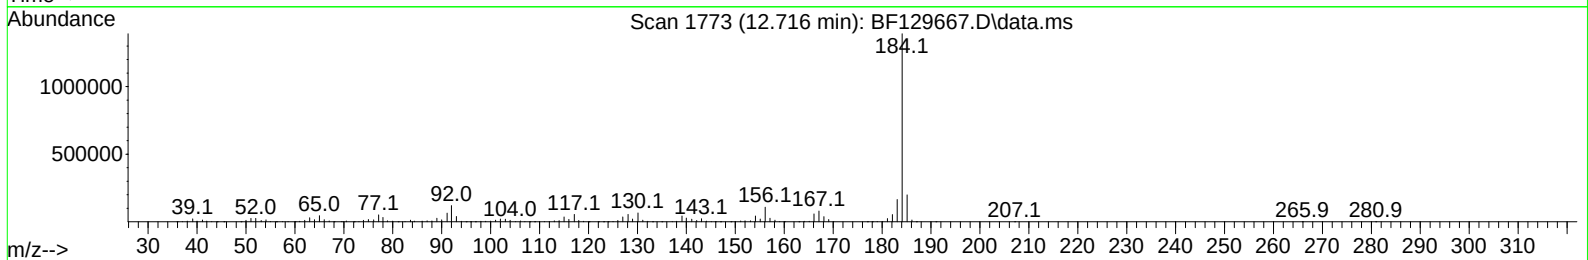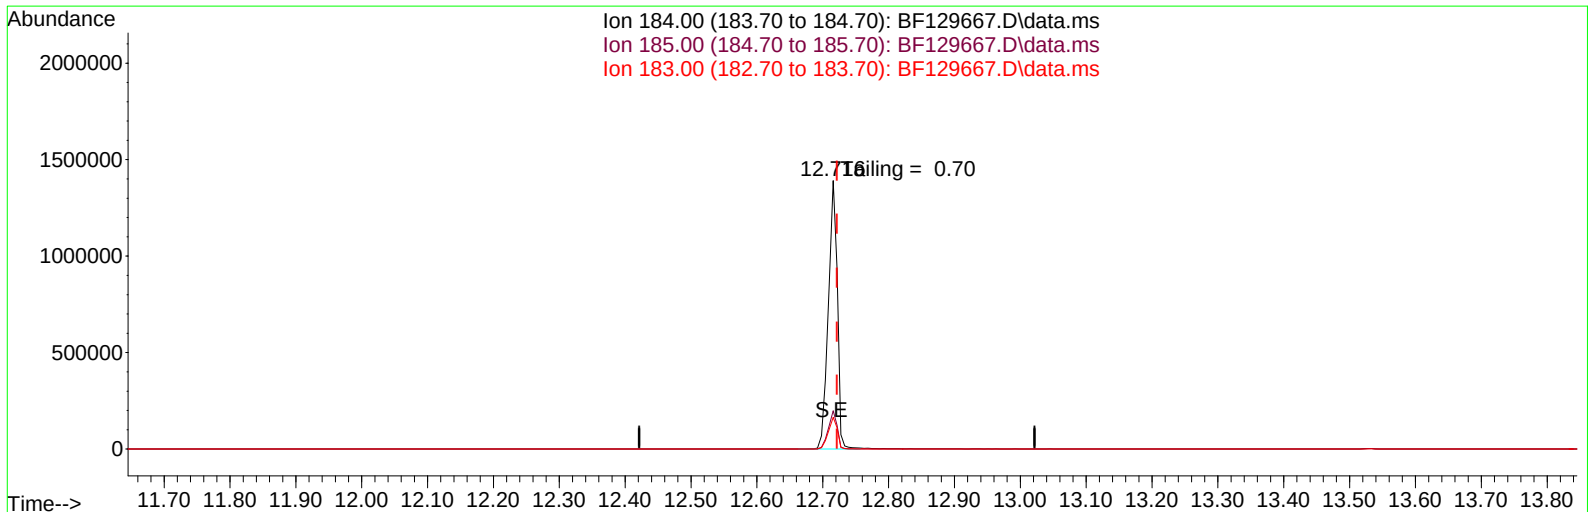

TIC: BF129667.D\data.ms

(77) Benzidine

12.716min (-0.006) 59173.76 ng

response 1325353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	11.60	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2022	BNA_F	<u>BF129667.D</u>
Compound Name	Response	Retention Time
DDT	714250	13.53
DDD	34469	13.22
DDE	1445	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35914	750164	4.79

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP