
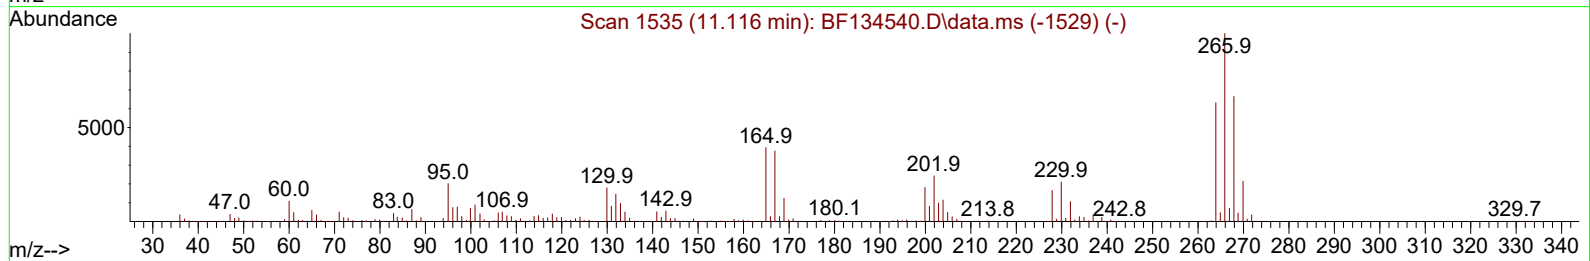
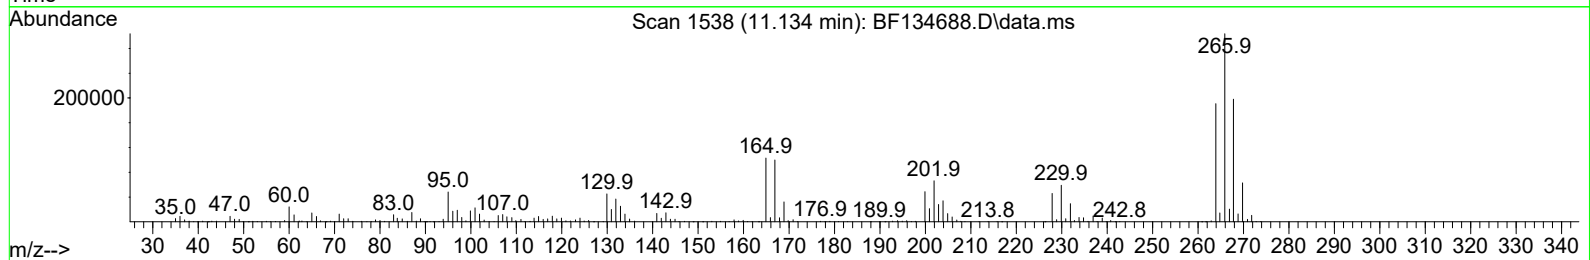


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134688.D
Acq On : 09 Aug 2023 13:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 03:19:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

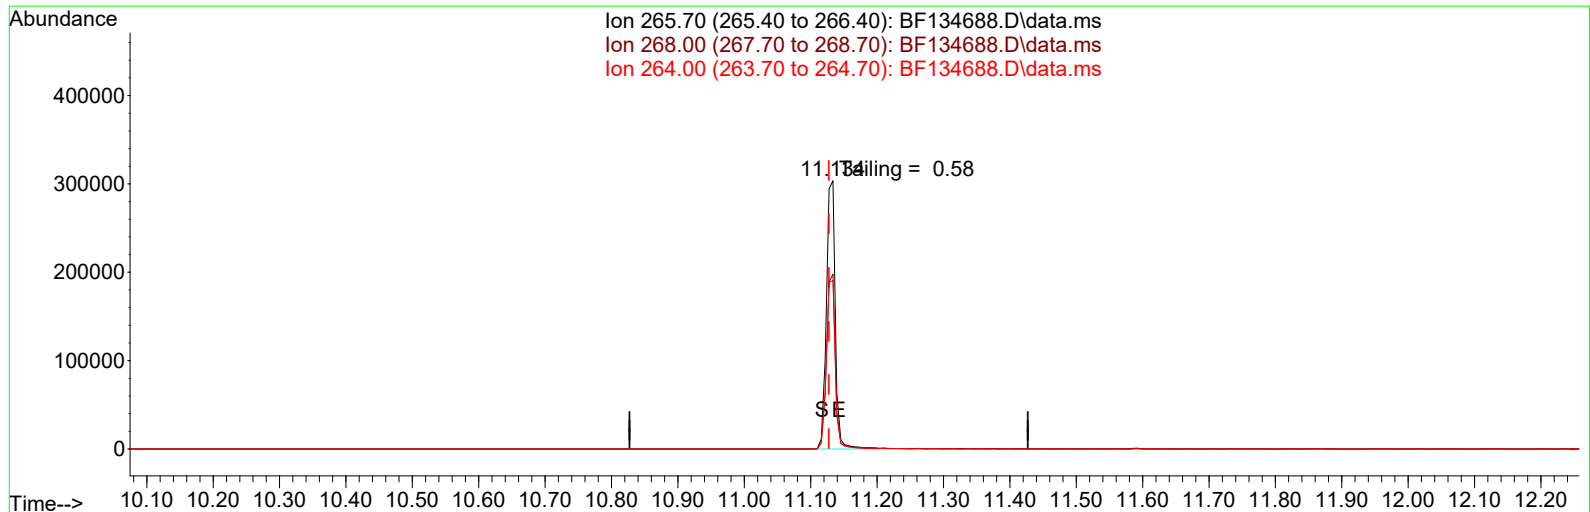

TIC: BF134688.D\data.ms

(70) Pentachlorophenol (C)




11.134min (+ 0.006) 158312.01 ng

response 286673

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	65.18
264.00	59.70	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134688.D
Acq On : 09 Aug 2023 13:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 03:19:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

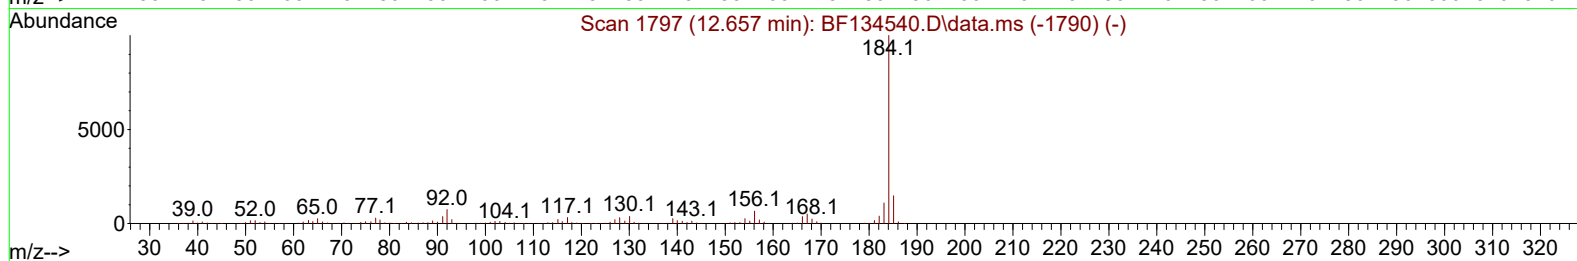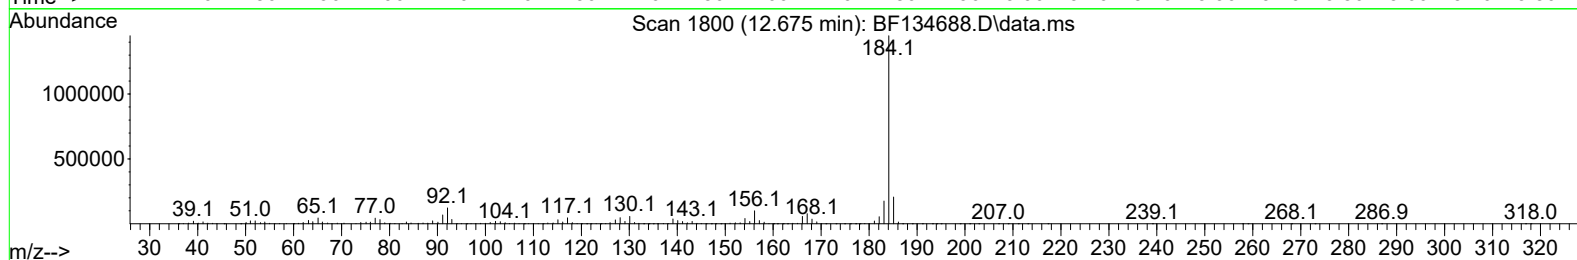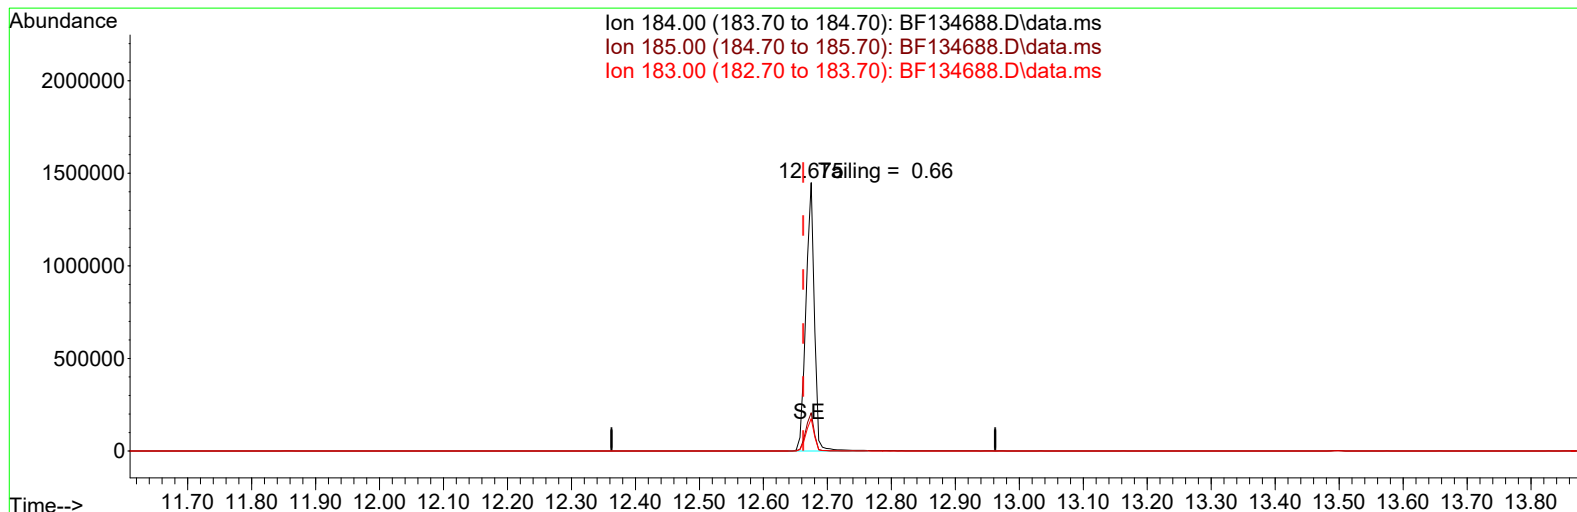

TIC: BF134688.D\data.ms

(77) Benzidine**12.675min (+ 0.012) 244351.13 ng****response 1352608**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.26
183.00	10.80	12.08
0.00	0.00	0.00