

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
 Data File : BF134687.D
 Acq On : 09 Aug 2023 13:09
 Operator : CG\JU
 Sample : 03903-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-08

Quant Time: Aug 10 01:39:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 09:29:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.804	152	258576	20.000	ng	0.00
21) Naphthalene-d8	8.081	136	1006944	20.000	ng	# 0.00
39) Acenaphthene-d10	9.833	164	493456	20.000	ng	0.00
64) Phenanthrene-d10	11.327	188	768418	20.000	ng	# 0.00
76) Chrysene-d12	13.980	240	565266	20.000	ng	# 0.00
86) Perylene-d12	15.456	264	481099	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	883115	51.916	ng	0.00
7) Phenol-d6	6.439	99	1119053	51.463	ng	0.00
23) Nitrobenzene-d5	7.363	82	671392	41.668	ng	0.00
42) 2,4,6-Tribromophenol	10.627	330	264030	52.488	ng	0.00
45) 2-Fluorobiphenyl	9.157	172	1204187	40.575	ng	0.00
79) Terphenyl-d14	12.921	244	1001848	31.244	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	13.968	149	79825	4.101	ng	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134687.D
Acq On : 09 Aug 2023 13:09
Operator : CG\JU
Sample : 03903-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-08

Quant Time: Aug 10 01:39:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration




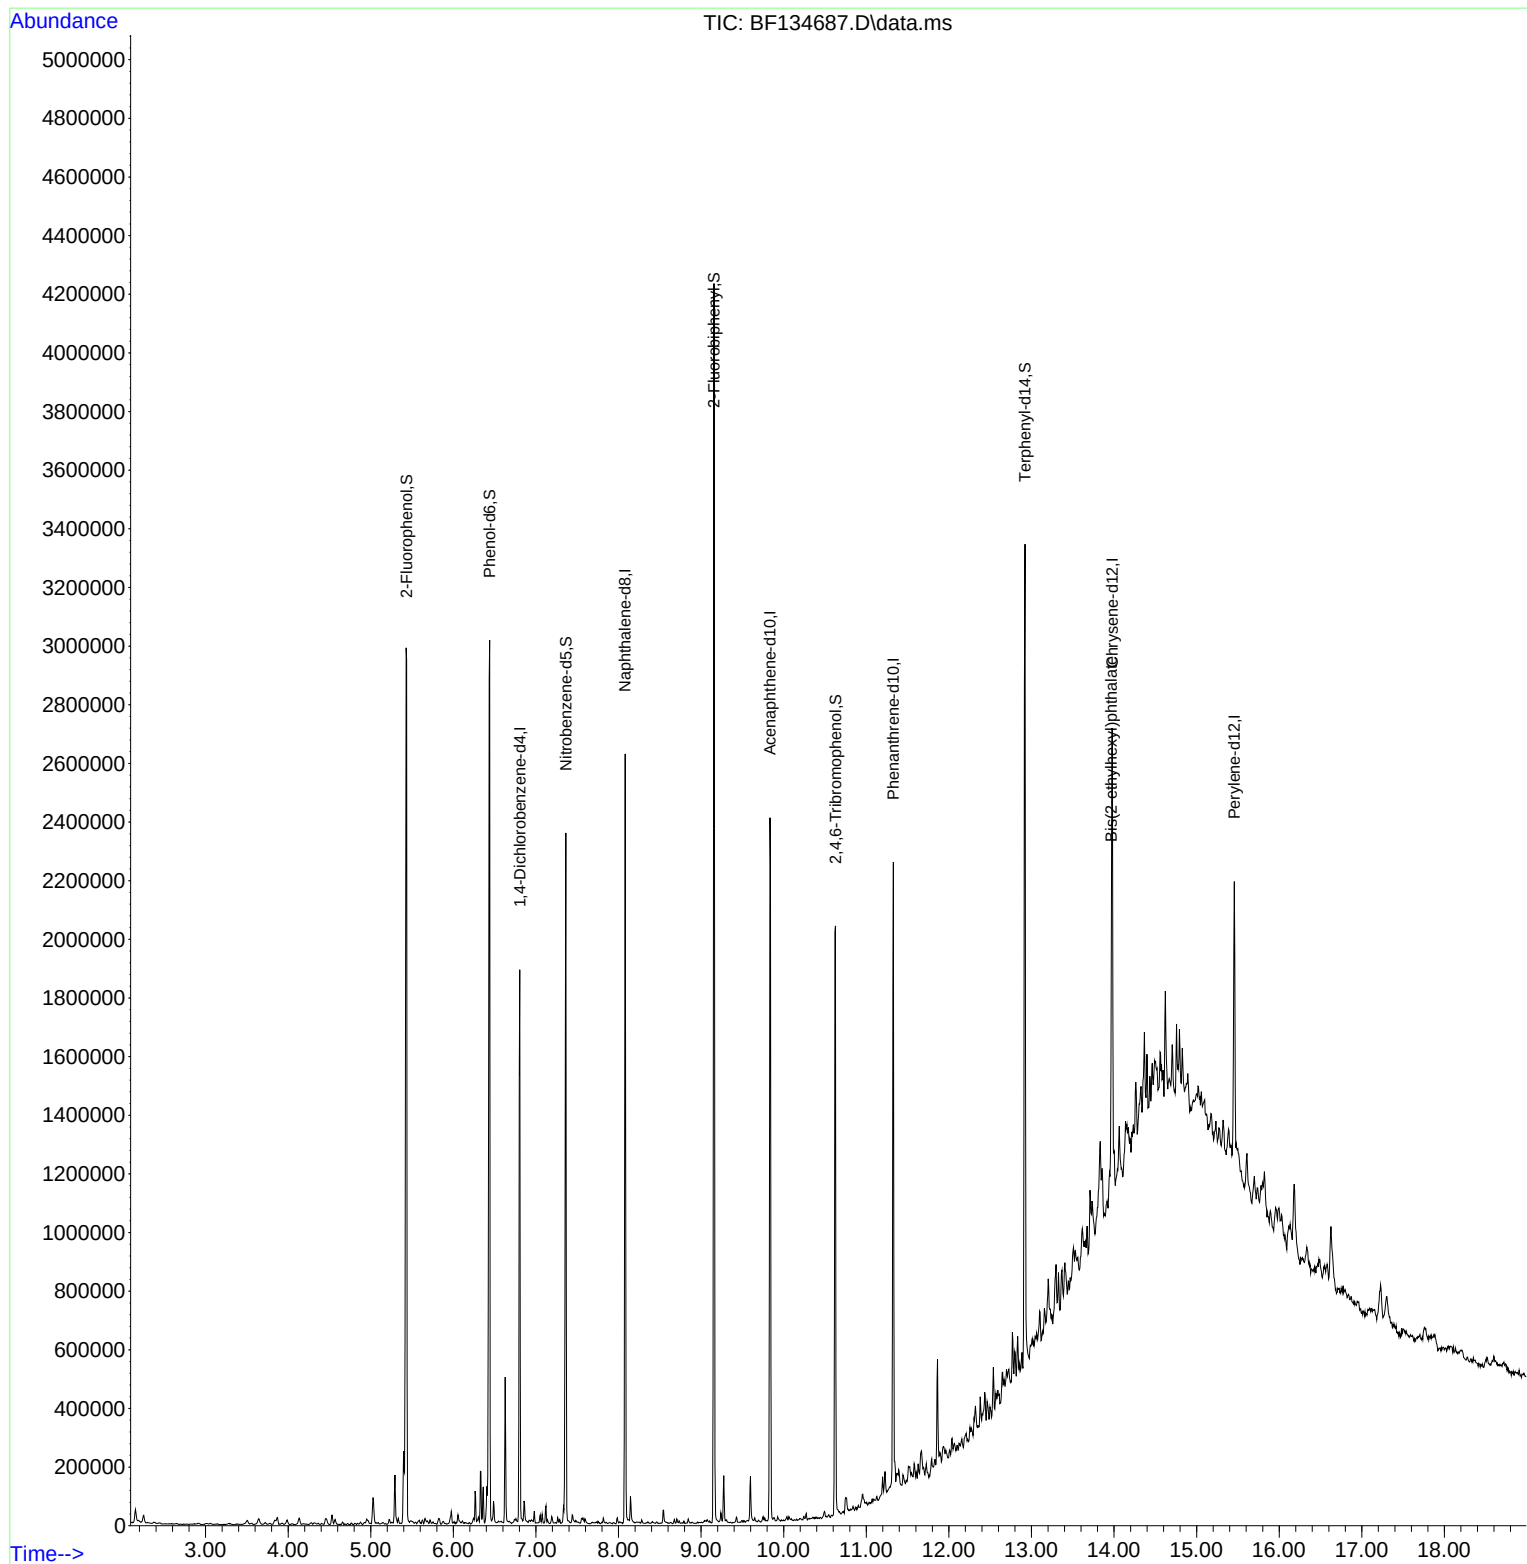


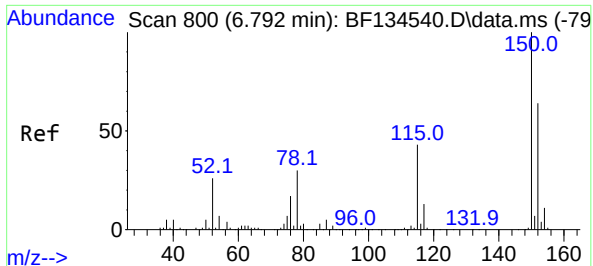

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.804 min Scan# 800
Delta R.T. 0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09




Instrument :
BNA_F
ClientSampleId :
MW-08


Tgt Ion:152 Resp: 258576
Ion Ratio Lower Upper
152 100
150 154.9 128.3 192.5
115 61.5 52.4 78.6

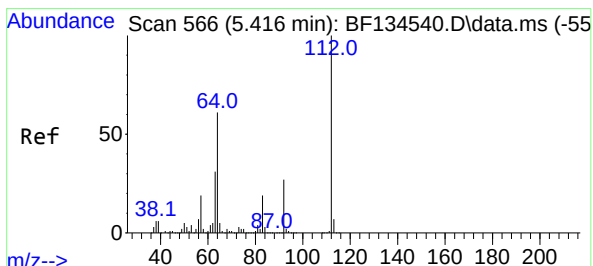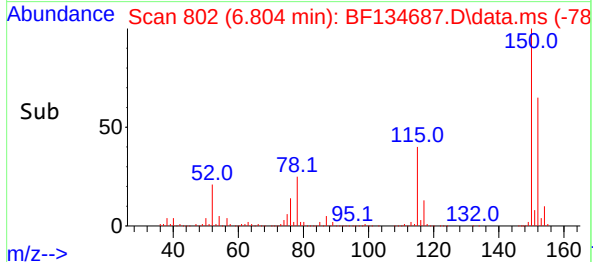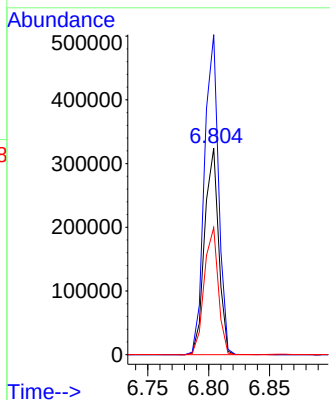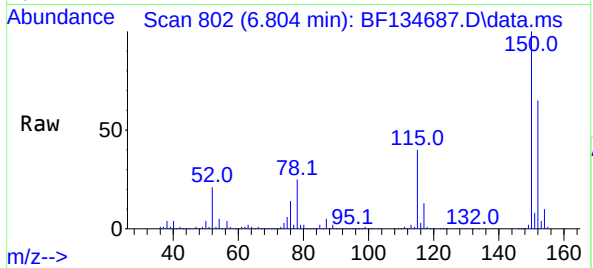

#5
2-Fluorophenol
Concen: 51.916 ng
RT: 5.434 min Scan# 569
Delta R.T. 0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Tgt Ion:112 Resp: 883115
Ion Ratio Lower Upper
112 100
64 57.2 44.9 67.3
63 29.3 25.4 38.0


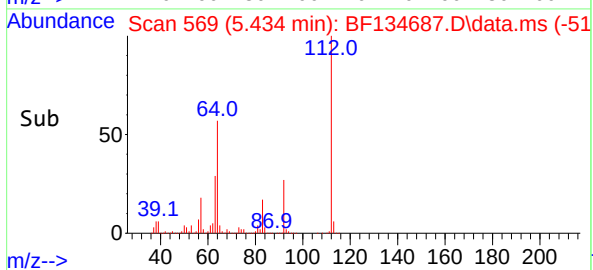
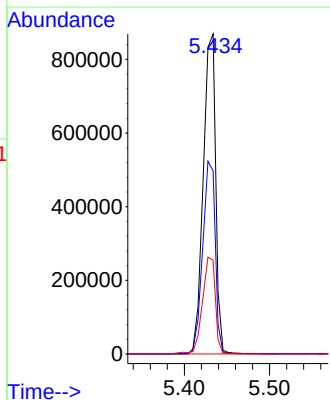
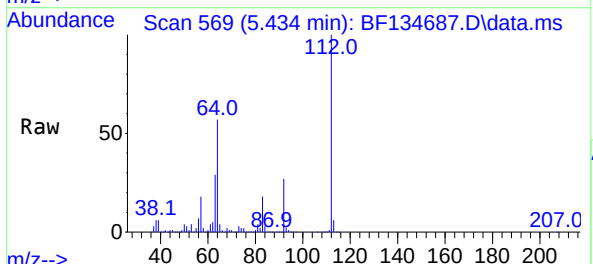


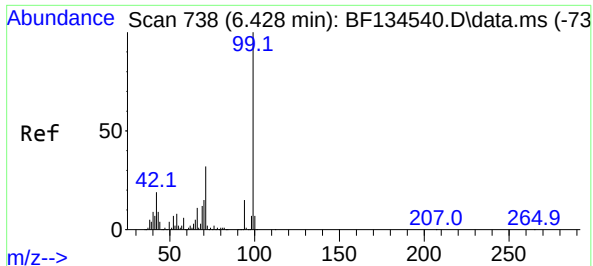

#7
Phenol-d6
Concen: 51.463 ng
RT: 6.439 min Scan# 74
Delta R.T. -0.000 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09




Instrument :
BNA_F
ClientSampleId :
MW-08


Tgt Ion: 99 Resp: 1119053
Ion Ratio Lower Upper
99 100
42 17.7 18.7 28.1#
71 31.5 36.4 54.6#

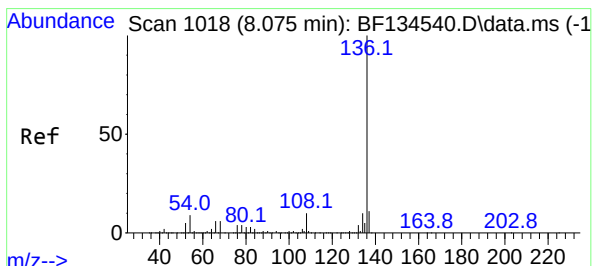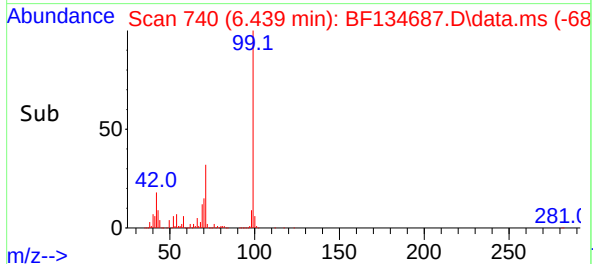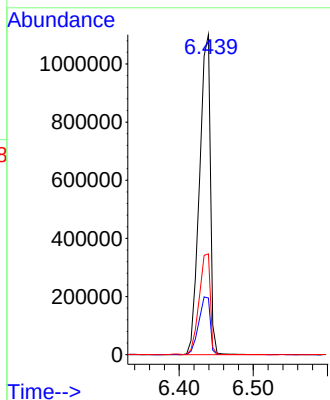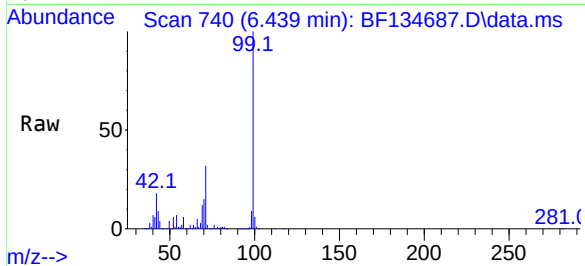

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1019
Delta R.T. -0.000 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Tgt Ion: 136 Resp: 1006944
Ion Ratio Lower Upper
136 100
137 11.5 8.4 12.6
54 8.3 5.2 7.8#
68 6.6 2.9 4.3#


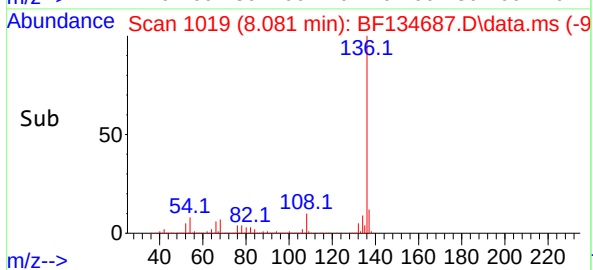
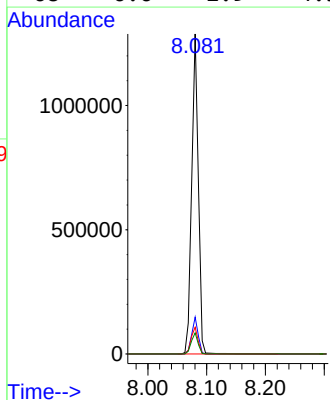
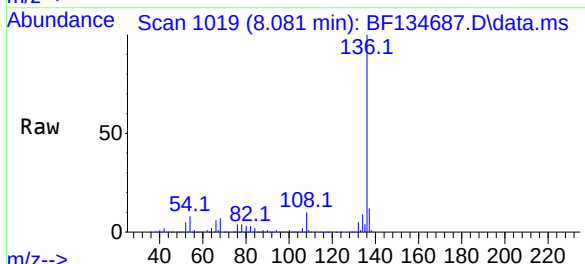


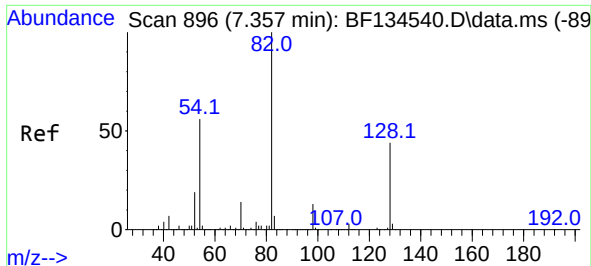

#23
Nitrobenzene-d5
Concen: 41.668 ng
RT: 7.363 min Scan# 896
Delta R.T. -0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09




Instrument :
BNA_F
ClientSampleId :
MW-08


Tgt Ion: 82 Resp: 671392
Ion Ratio Lower Upper
82 100
128 47.2 34.3 51.5
54 52.3 43.8 65.6

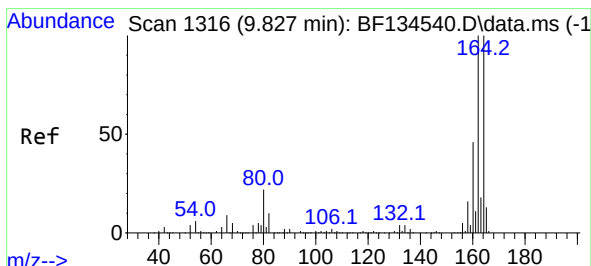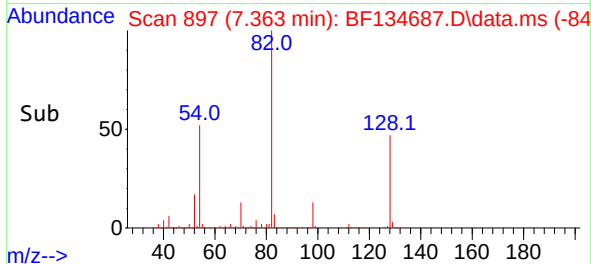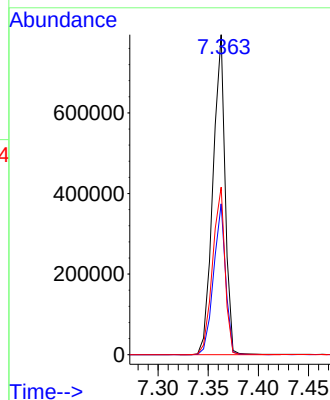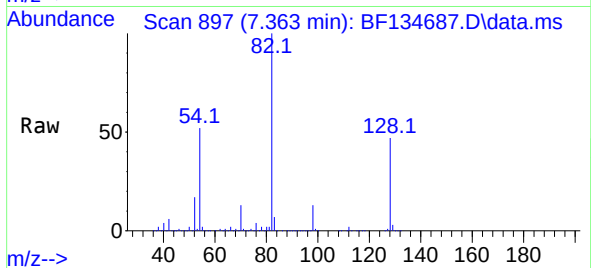

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.833 min Scan# 1317
Delta R.T. -0.000 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09


Tgt Ion:164 Resp: 493456
Ion Ratio Lower Upper
164 100
162 102.0 82.6 123.8
160 46.0 37.2 55.8

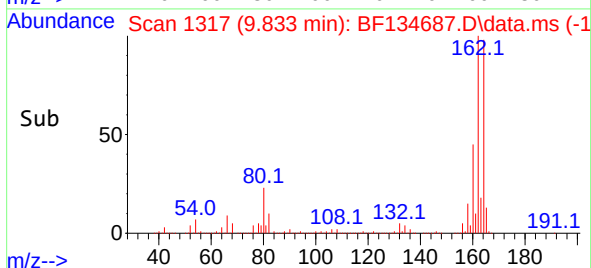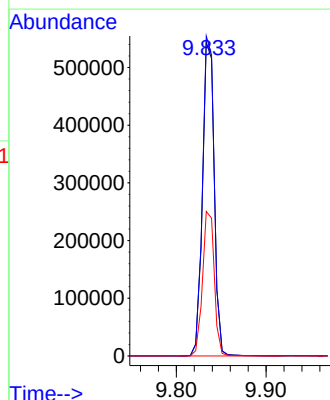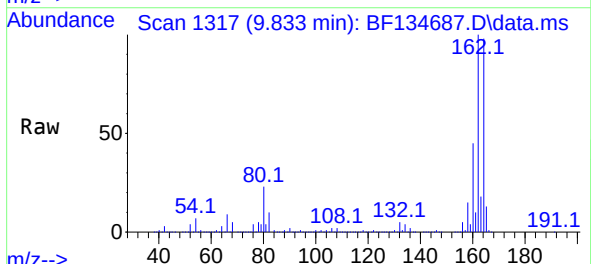



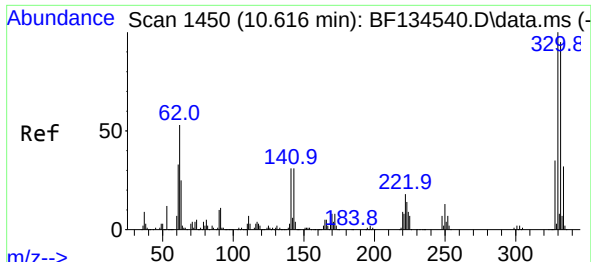


#42
2,4,6-Tribromophenol
Concen: 52.488 ng
RT: 10.627 min Scan# 1452
Delta R.T. -0.000 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Instrument :
BNA_F
ClientSampleId :
MW-08



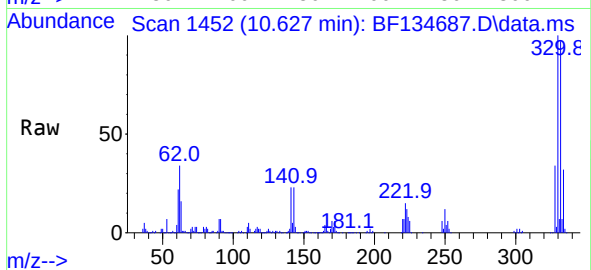



Tgt Ion:330 Resp: 264030
Ion Ratio Lower Upper
330 100
332 96.5 78.8 118.2
141 29.3 25.4 38.2

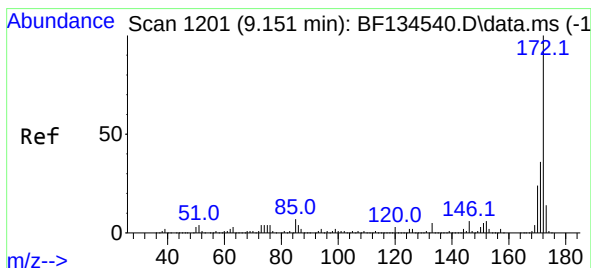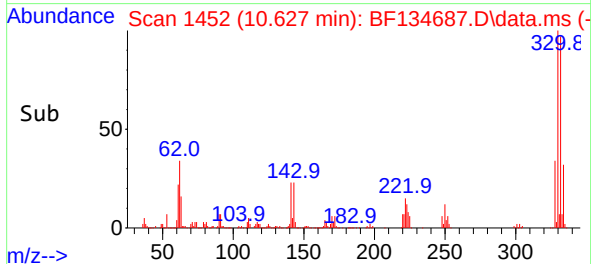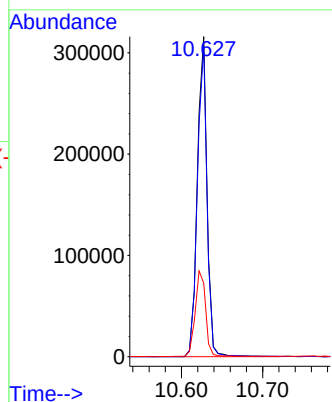

#45
2-Fluorobiphenyl
Concen: 40.575 ng
RT: 9.157 min Scan# 1202
Delta R.T. -0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Tgt Ion:172 Resp: 1204187
Ion Ratio Lower Upper
172 100
171 35.5 28.8 43.2
170 23.6 18.7 28.1


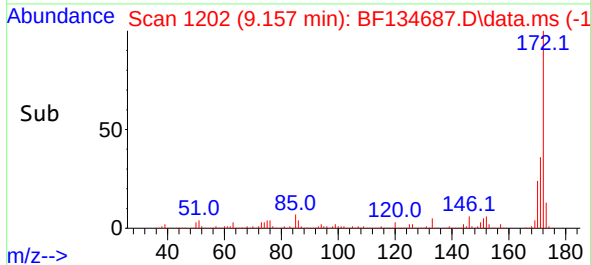
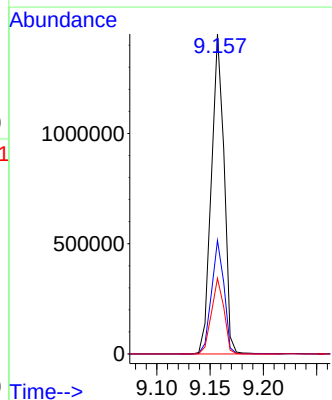
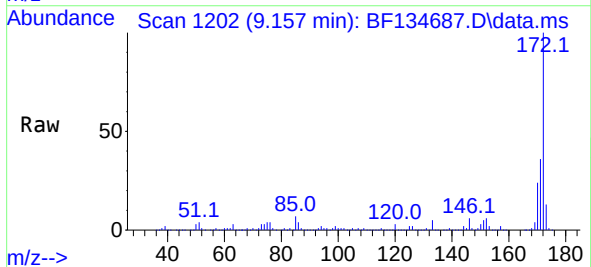


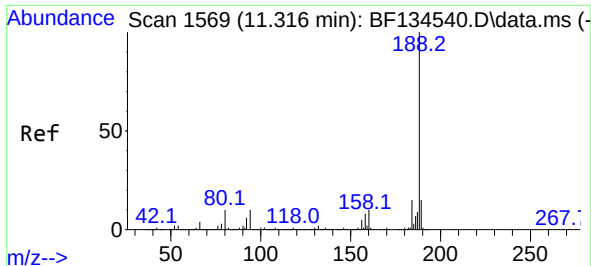

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.327 min Scan# 11
Delta R.T. 0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09




Instrument :
BNA_F
ClientSampleId :
MW-08


Tgt Ion:188 Resp: 768418
Ion Ratio Lower Upper
188 100
94 10.3 5.1 7.7#
80 10.3 6.6 9.8#

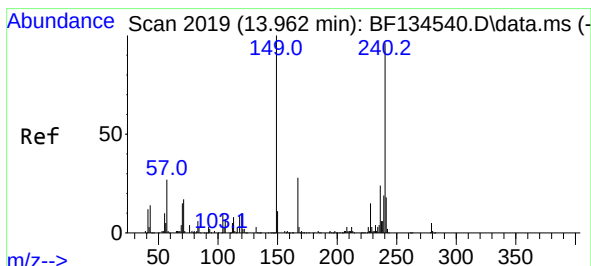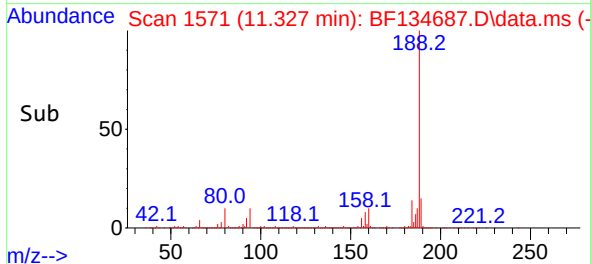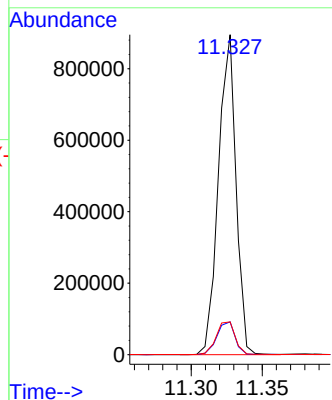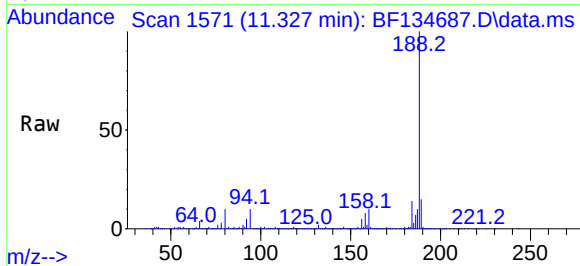

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.980 min Scan# 2022
Delta R.T. 0.006 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Tgt Ion:240 Resp: 565266
Ion Ratio Lower Upper
240 100
120 10.9 6.6 10.0#
236 25.7 20.2 30.2


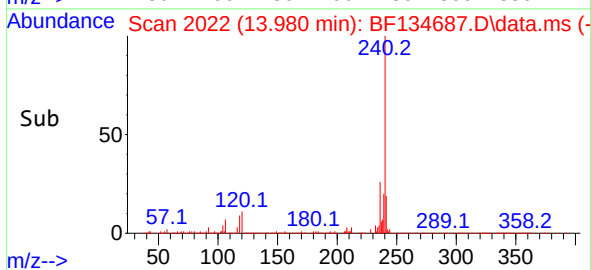
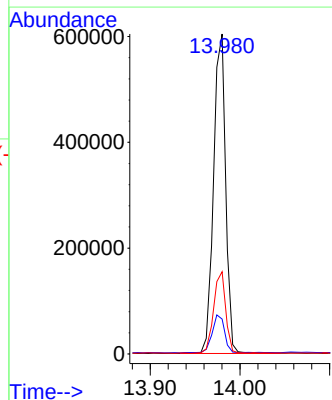
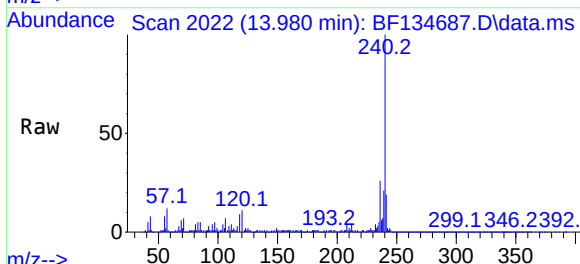


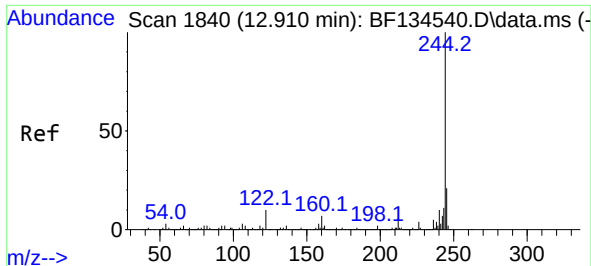

#79
 Terphenyl-d14
 Concen: 31.244 ng
 RT: 12.921 min Scan# 1842
 Delta R.T. -0.000 min
 Lab File: BF134687.D
 Acq: 09 Aug 2023 13:09




Instrument :
 BNA_F
 ClientSampleId :
 MW-08


Tgt Ion:244 Resp: 1001848
 Ion Ratio Lower Upper
 244 100
 212 6.0 5.6 8.4
 122 10.1 8.0 12.0

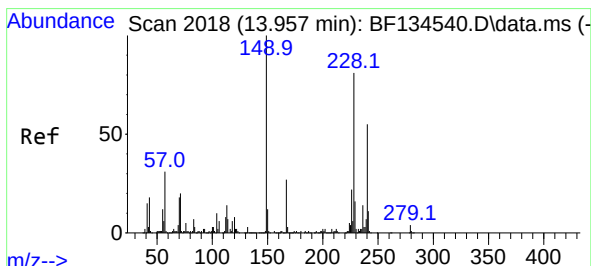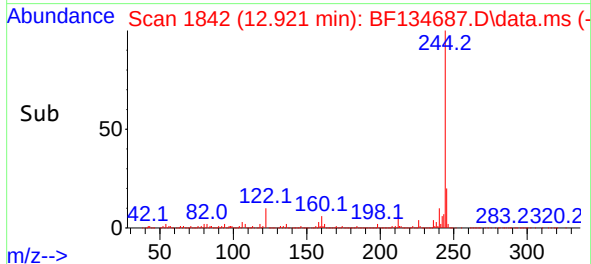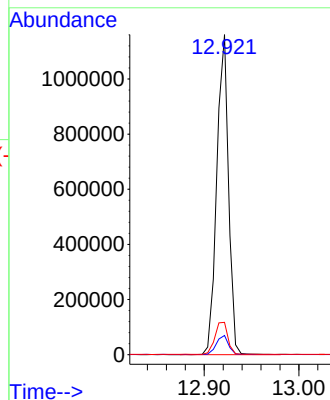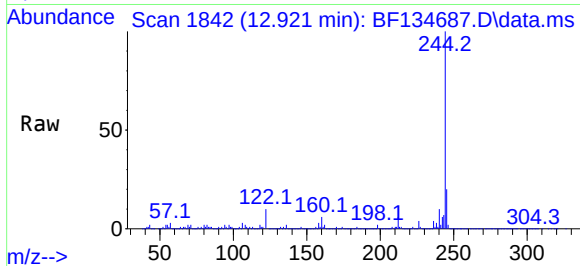

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 4.101 ng
 RT: 13.968 min Scan# 2020
 Delta R.T. 0.006 min
 Lab File: BF134687.D
 Acq: 09 Aug 2023 13:09

Tgt Ion:149 Resp: 79825
 Ion Ratio Lower Upper
 149 100
 167 30.0 21.6 32.4
 279 5.0 3.5 5.3

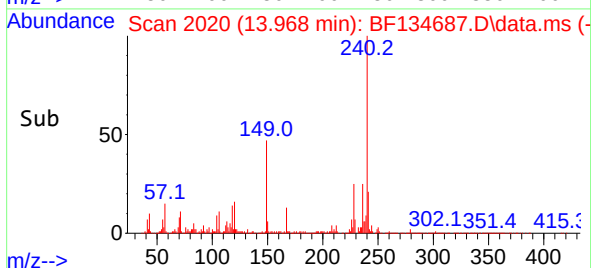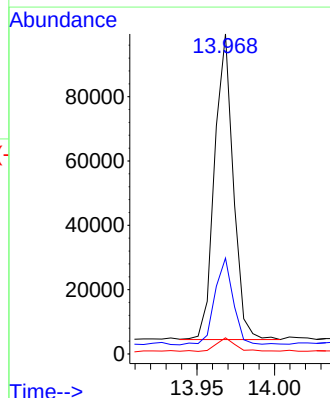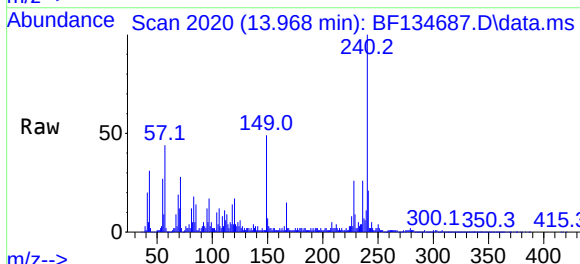

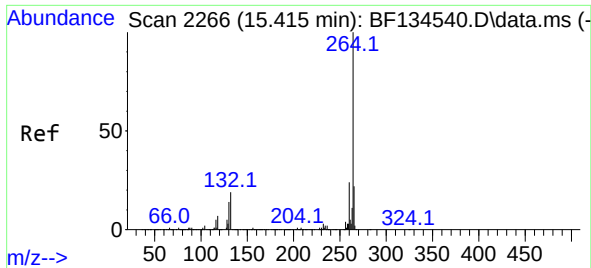

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.456 min Scan# 21
Delta R.T. 0.018 min
Lab File: BF134687.D
Acq: 09 Aug 2023 13:09

Instrument :
BNA_F
ClientSampleId :
MW-08

Tgt Ion:264 Resp: 481099
Ion Ratio Lower Upper
264 100
260 23.6 18.4 27.6
265 22.3 15.8 23.8

