


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134678.D
Acq On : 09 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 09:29:15 2023

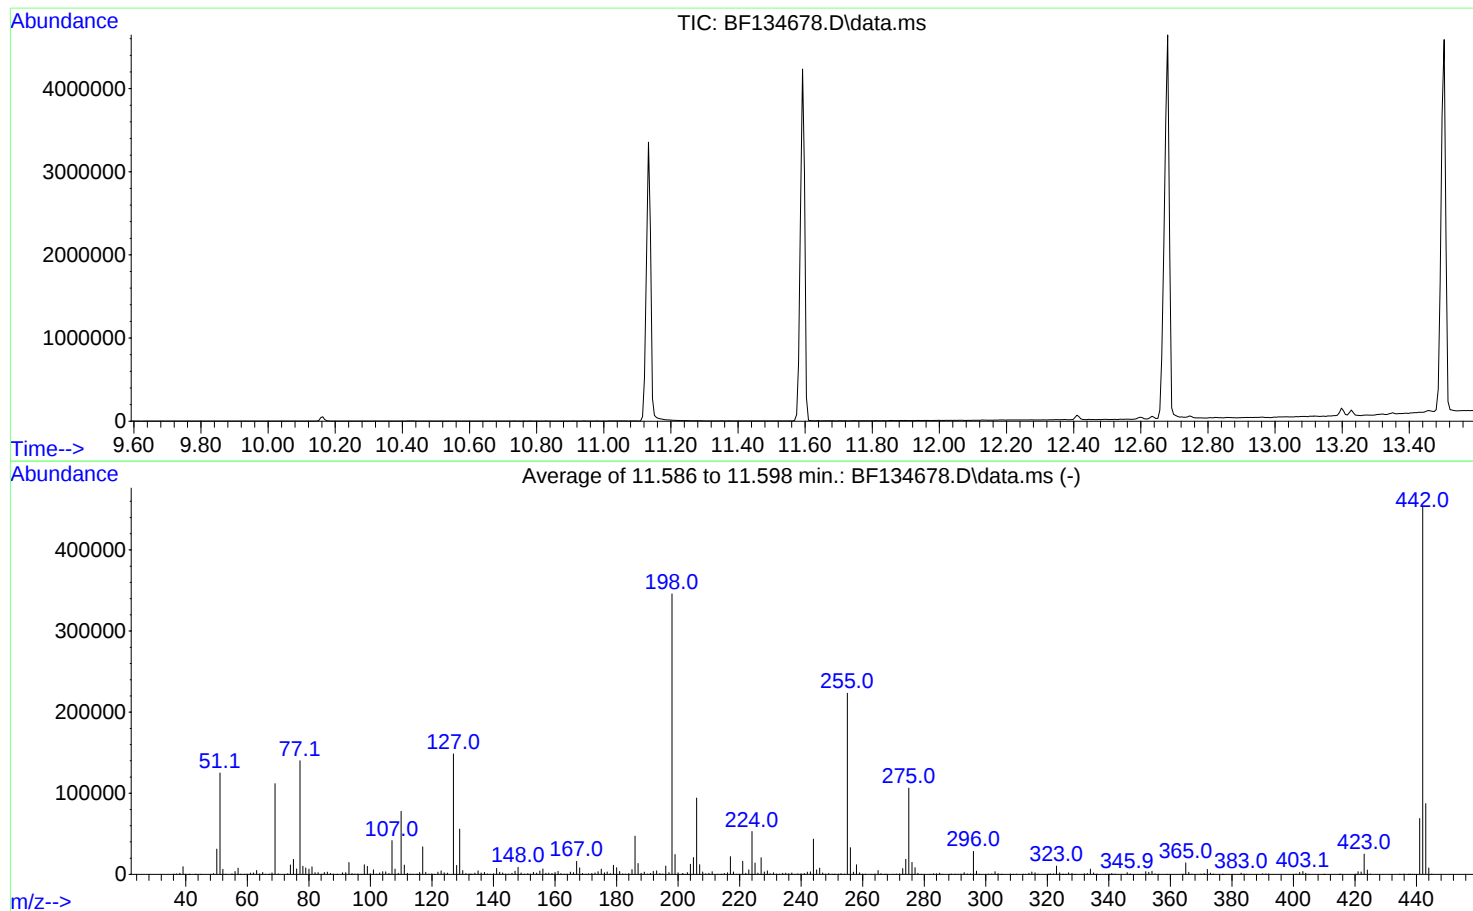




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	124995	PASS
68	69	0.00	2	1.7	1857	PASS
69	198	0.00	100	32.4	111924	PASS
70	69	0.00	2	0.5	578	PASS
127	198	10	80	42.9	148517	PASS
197	198	0.00	2	0.6	2096	PASS
198	198	100	100	100.0	345899	PASS
199	198	5	9	7.1	24395	PASS
275	198	10	60	30.8	106381	PASS
365	198	1	100	4.1	14258	PASS
441	198	0.01	100	19.9	68779	PASS
442	442	50	100	100.0	453568	PASS
443	442	15	24	19.2	87136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134678.D
Acq On : 09 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:44:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

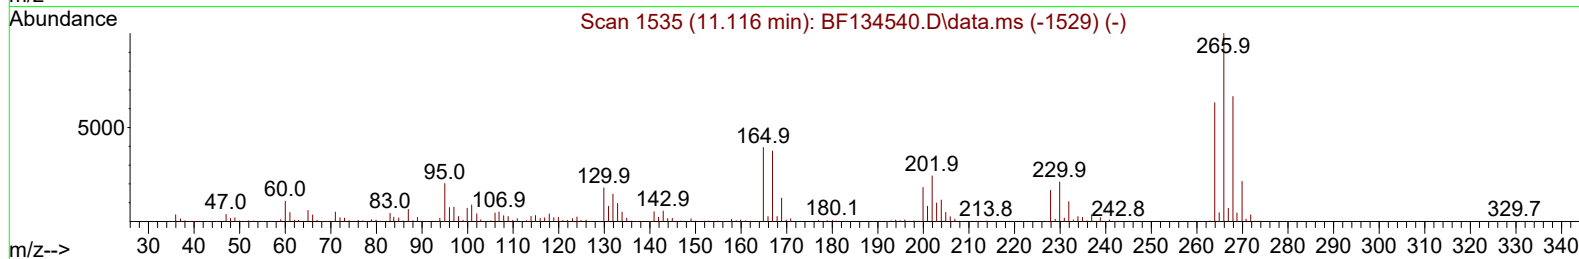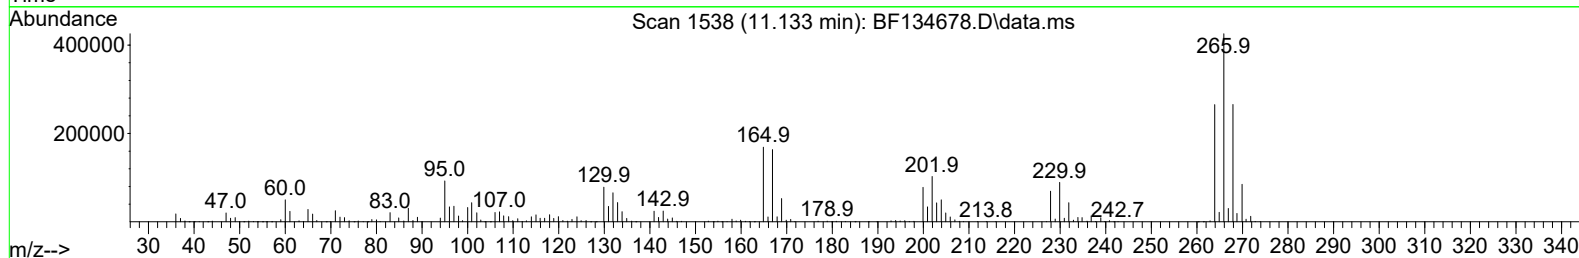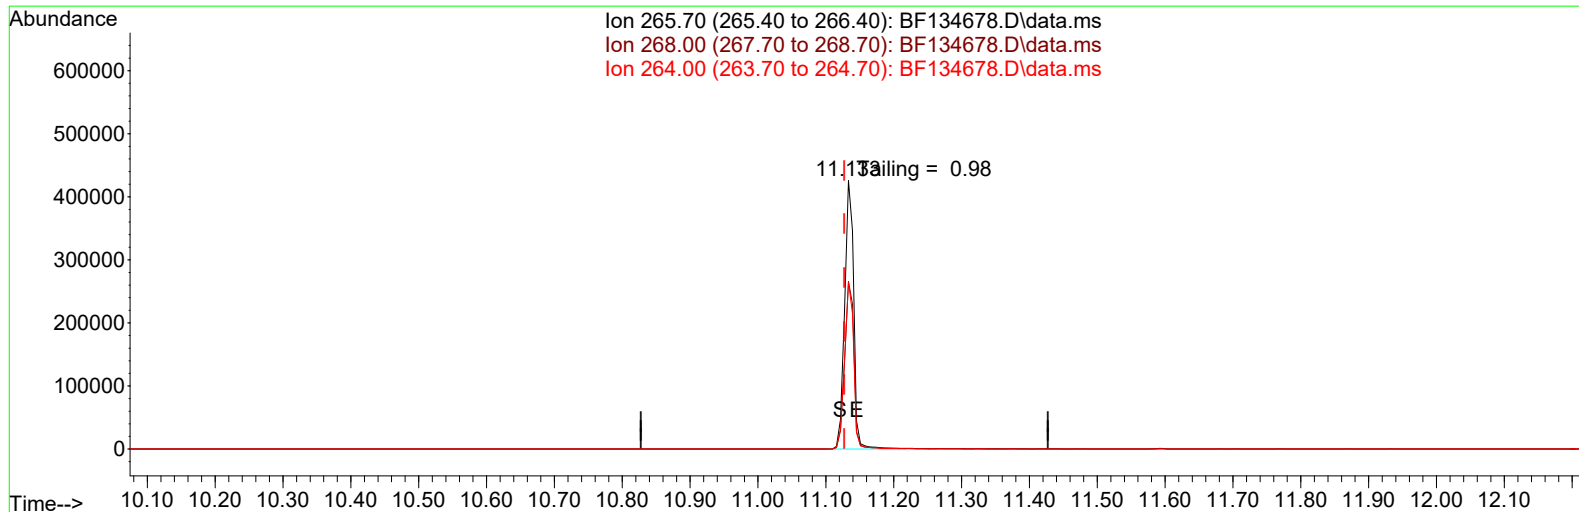

TIC: BF134678.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 734957.06 ng




response 394526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	62.37
264.00	59.70	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134678.D
Acq On : 09 Aug 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:44:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

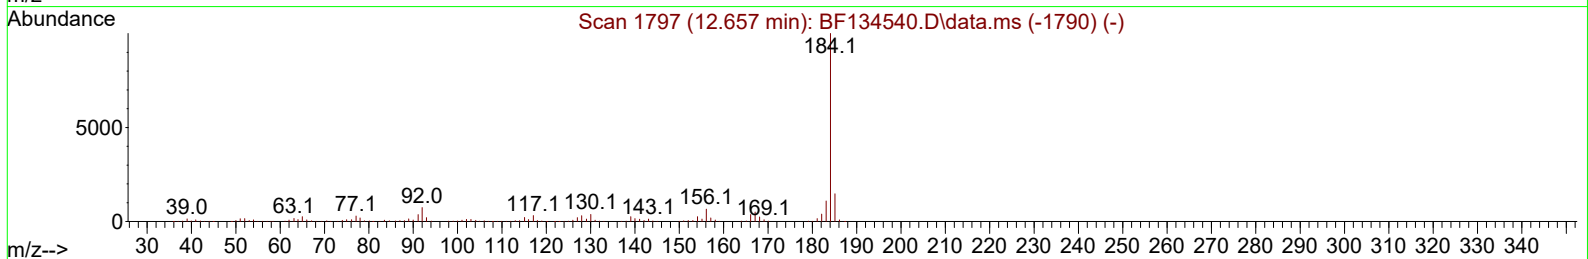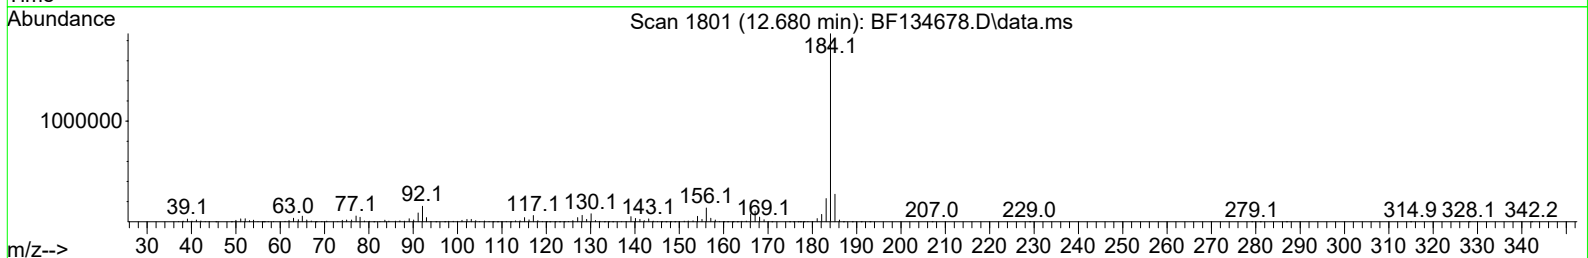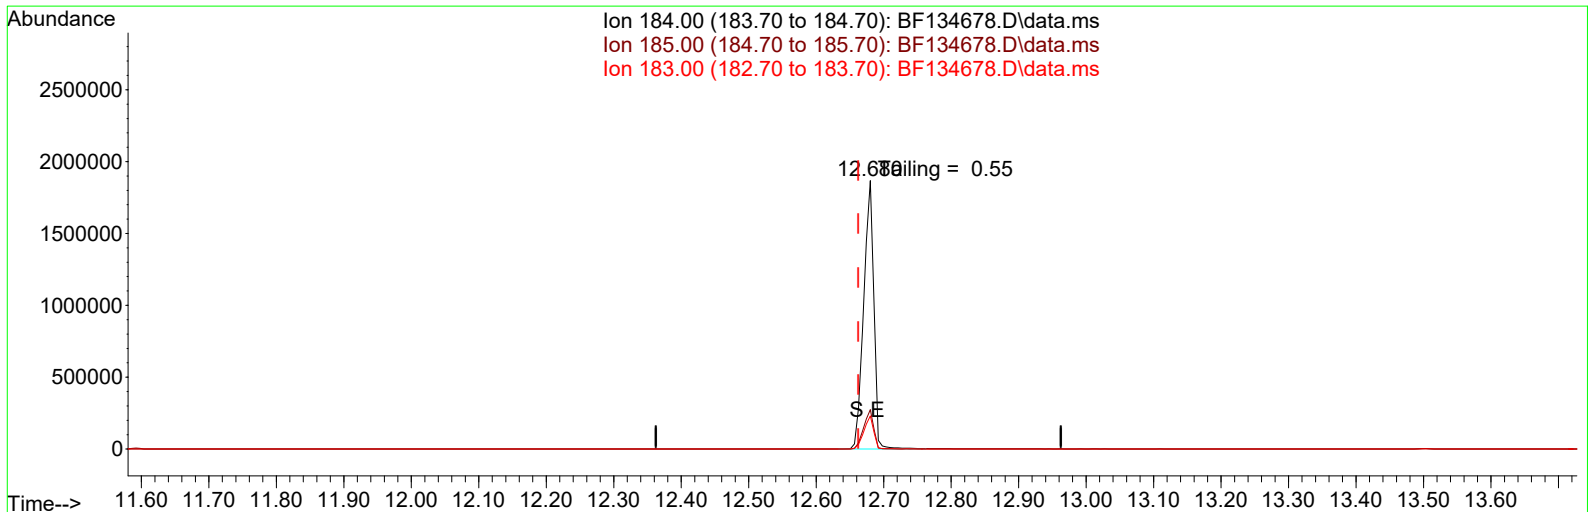

TIC: BF134678.D\data.ms

(77) Benzidine

12.680min (+ 0.018) 191992.12 ng

response 1954671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.69
183.00	10.80	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_F	<u>BF134678.D</u>
Compound Name	Response	Retention Time
DDT	872389	13.504
DDD	25228	13.198
DDE	799	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26027	898416	2.90

Instrument :
BNA_F
ClientSampleId :
DFTPP