
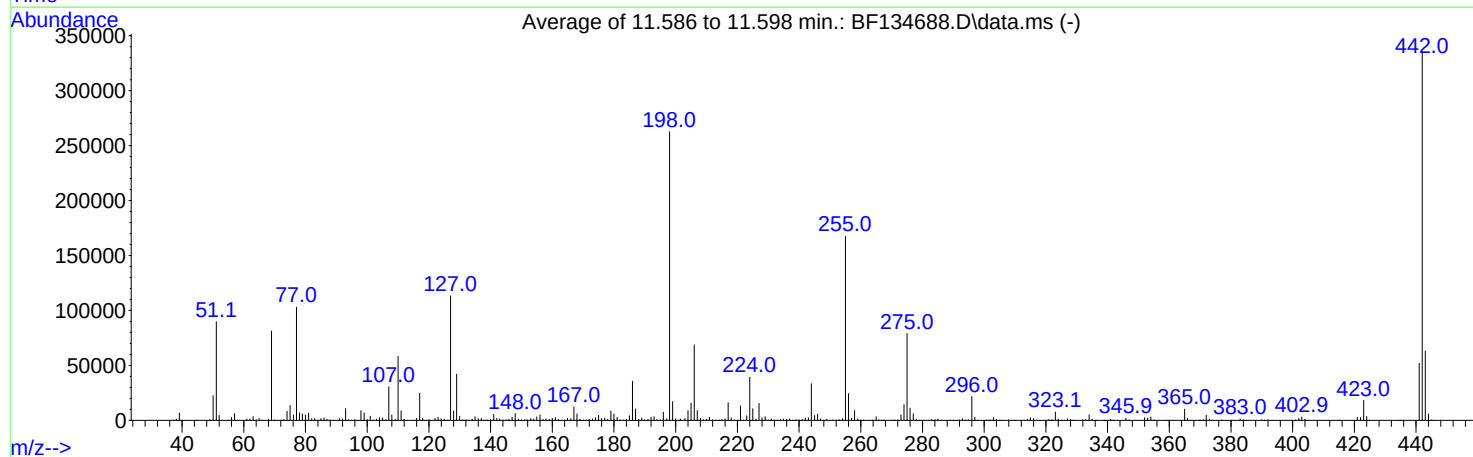


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
 Data File : BF134688.D
 Acq On : 09 Aug 2023 13:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 09:29:15 2023

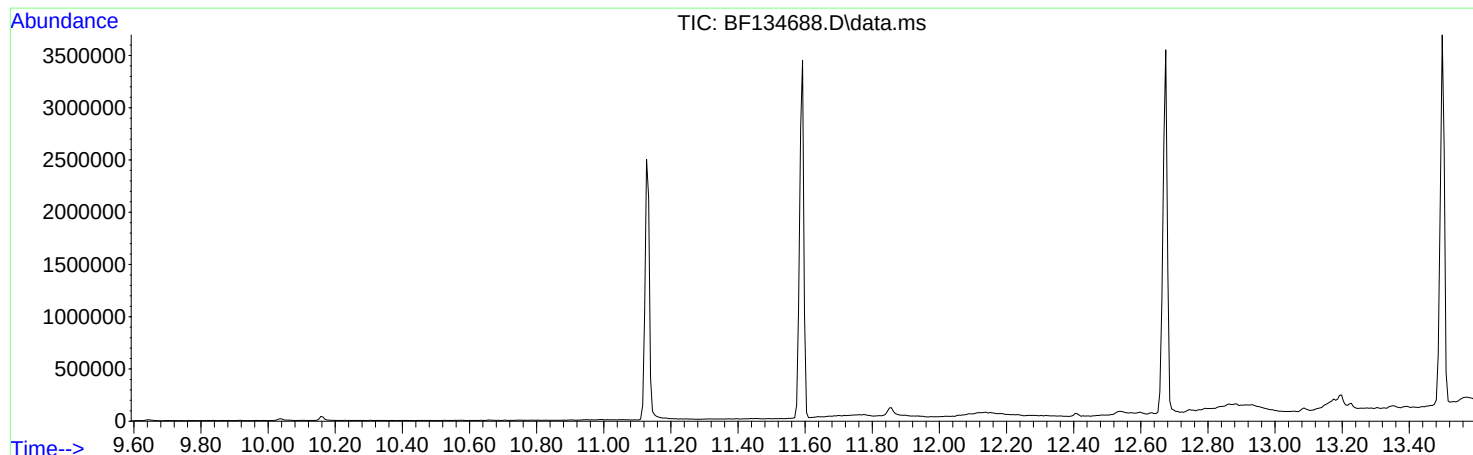




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	89821	PASS
68	69	0.00	2	1.7	1345	PASS
69	198	0.00	100	30.9	81233	PASS
70	69	0.00	2	0.6	450	PASS
127	198	10	80	43.1	113339	PASS
197	198	0.00	2	0.6	1468	PASS
198	198	100	100	100.0	262664	PASS
199	198	5	9	6.5	17106	PASS
275	198	10	60	30.1	79024	PASS
365	198	1	100	3.9	10150	PASS
441	198	0.01	100	19.8	51896	PASS
442	442	50	100	100.0	334699	PASS
443	442	15	24	18.9	63117	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080923\
Data File : BF134688.D
Acq On : 09 Aug 2023 13:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 10 03:19:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 09:29:15 2023
Response via : Initial Calibration

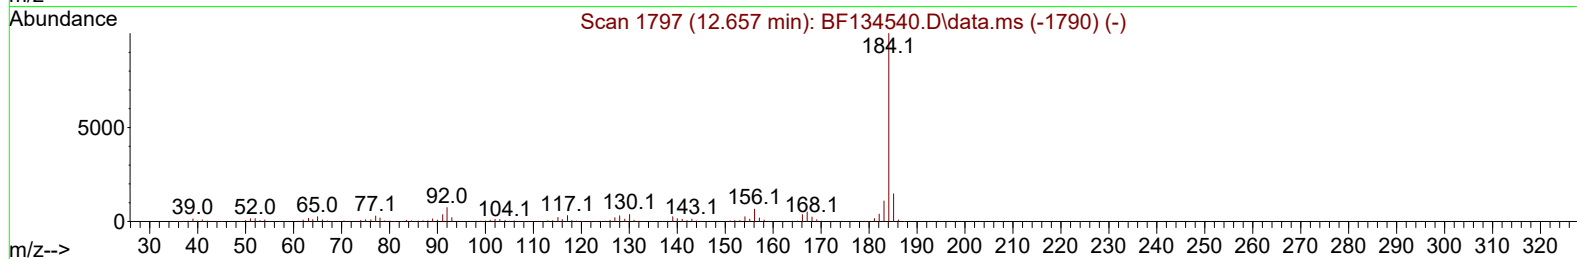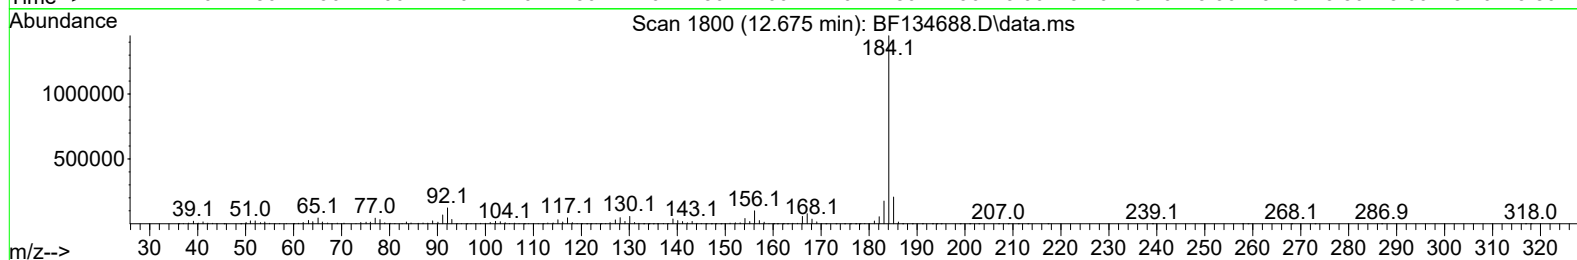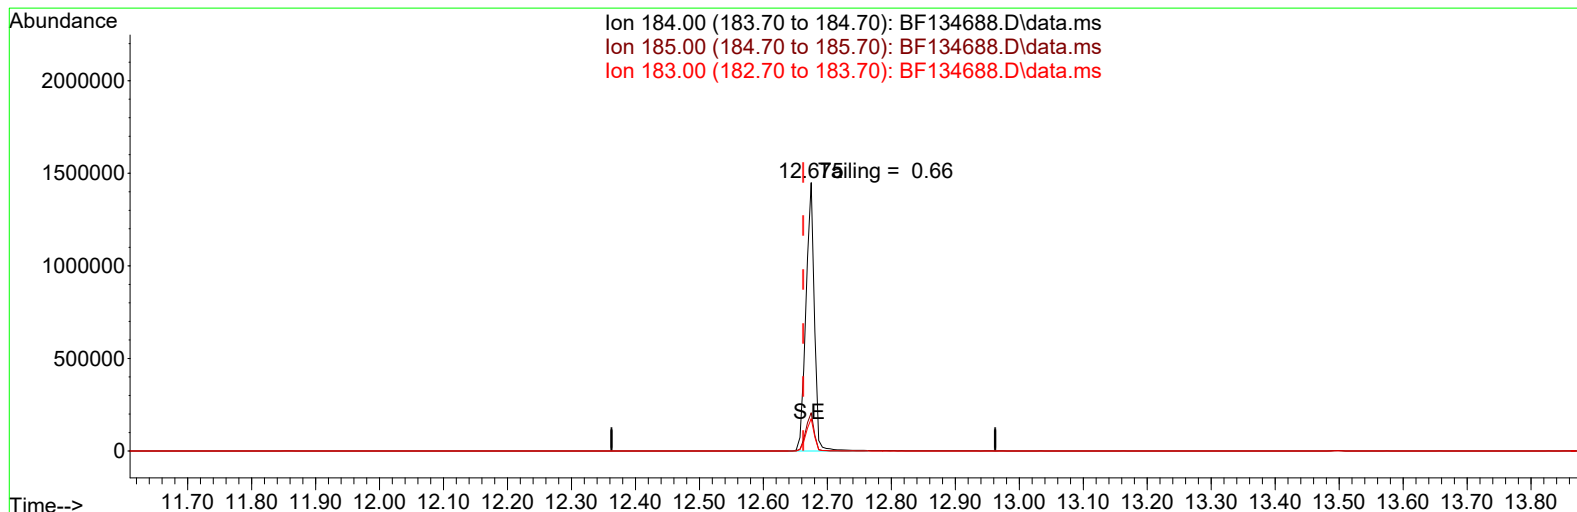

TIC: BF134688.D\data.ms

(77) Benzidine

12.675min (+ 0.012) 244351.13 ng

response 1352608

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.26
183.00	10.80	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_F	<u>BF134688.D</u>
Compound Name	Response	Retention Time
DDT	647549	13.498
DDD	22438	13.198
DDE	1710	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24148	671697	3.60

Instrument :
BNA_F
ClientSampleId :
DFTPP