


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081015\
 Data File : BF080950.D
 Acq On : 10 Aug 2015 11:08
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 08 01:33:05 2015

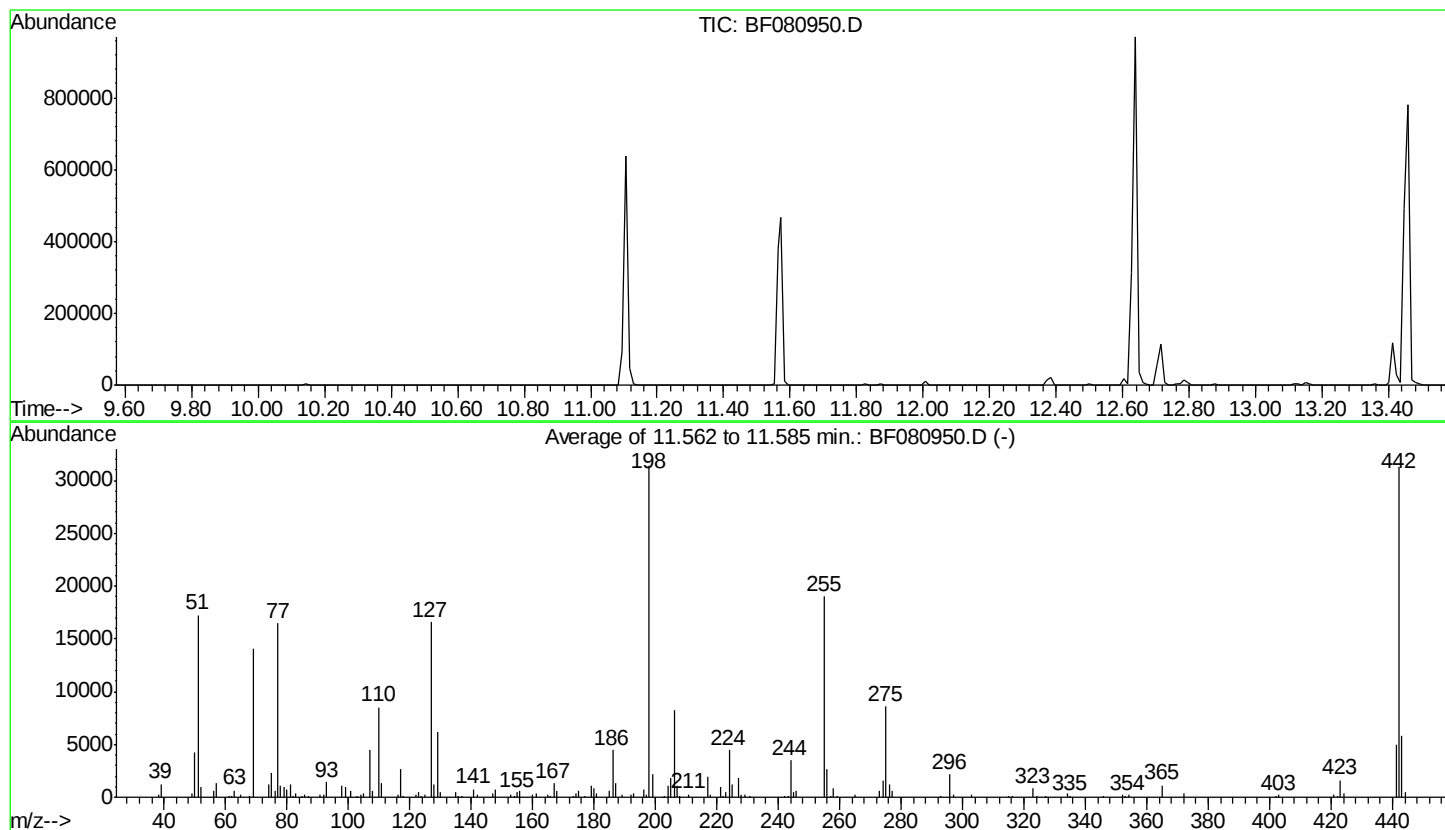

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	17254	PASS
68	69	0.00	2	1.0	147	PASS
69	198	0.00	100	44.8	14052	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	16552	PASS
197	198	0.00	2	0.6	188	PASS
198	198	100	100	100.0	31397	PASS
199	198	5	9	6.8	2134	PASS
275	198	10	60	27.3	8581	PASS
365	198	1	100	3.5	1095	PASS
441	442	0.01	24	15.8	4963	PASS
442	198	50	100	99.7	31317	PASS
443	442	15	24	18.6	5822	PASS