
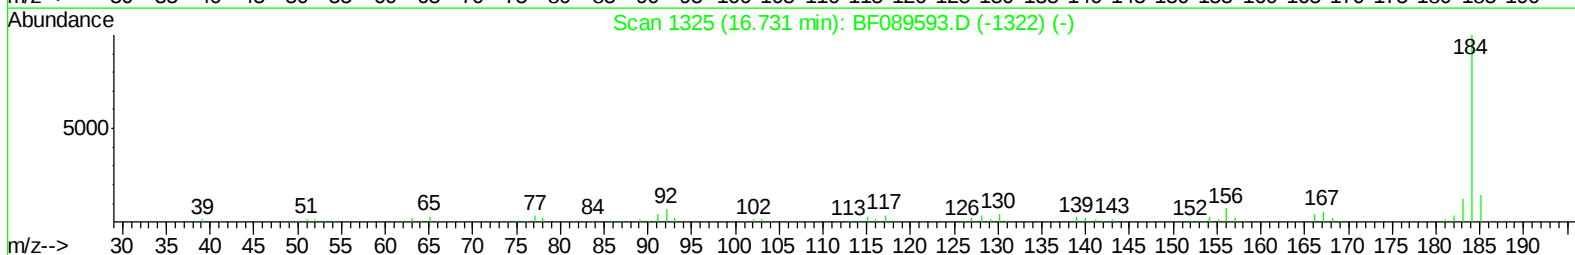
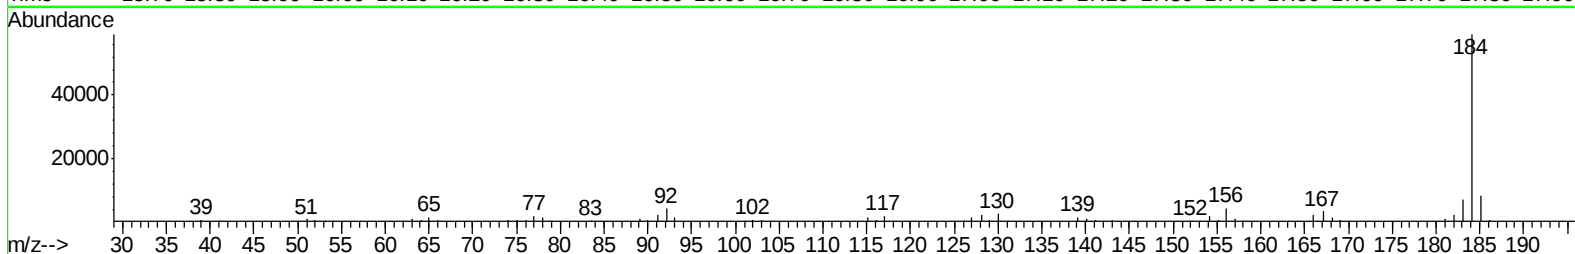


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081016\
Data File : BF089700.D
Acq On : 10 Aug 2016 15:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 07:36:30 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 11 01:52:35 2016
Response via : Initial Calibration

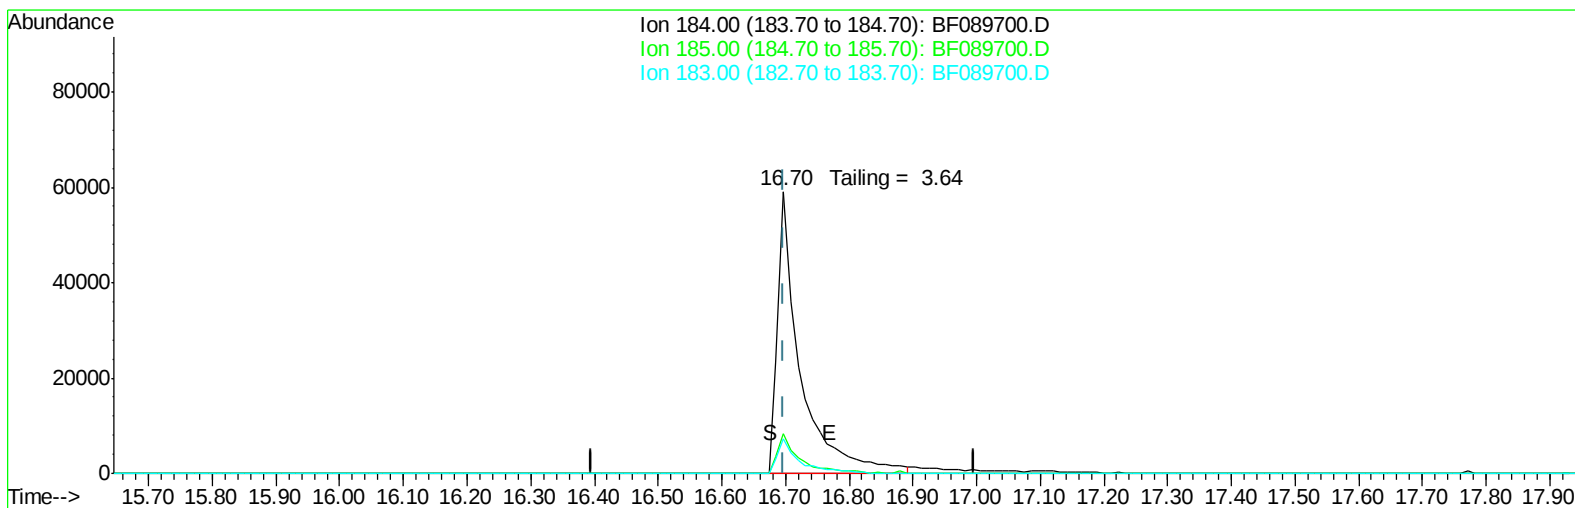

TIC: BF089700.D

(76) Benzidine




16.697min (-0.000) 0.00ng

response 149271

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.02
183.00	12.30	12.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081016\
Data File : BF089700.D
Acq On : 10 Aug 2016 15:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 07:36:30 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 11 01:52:35 2016
Response via : Initial Calibration

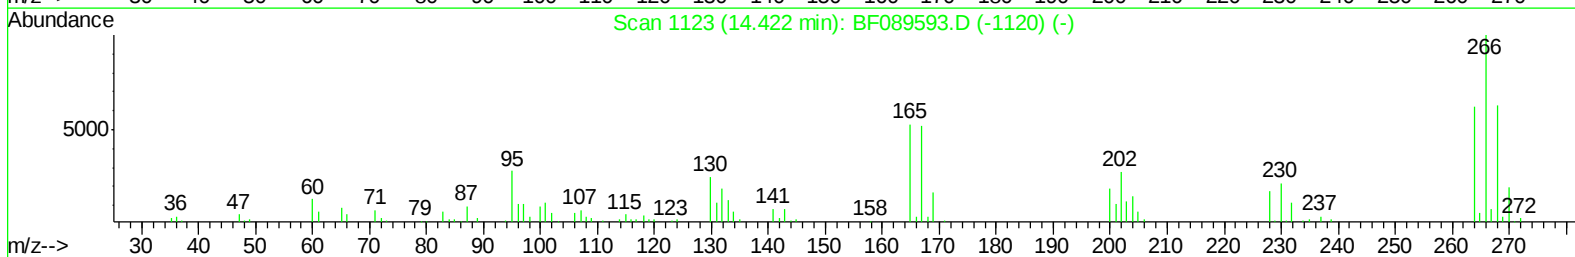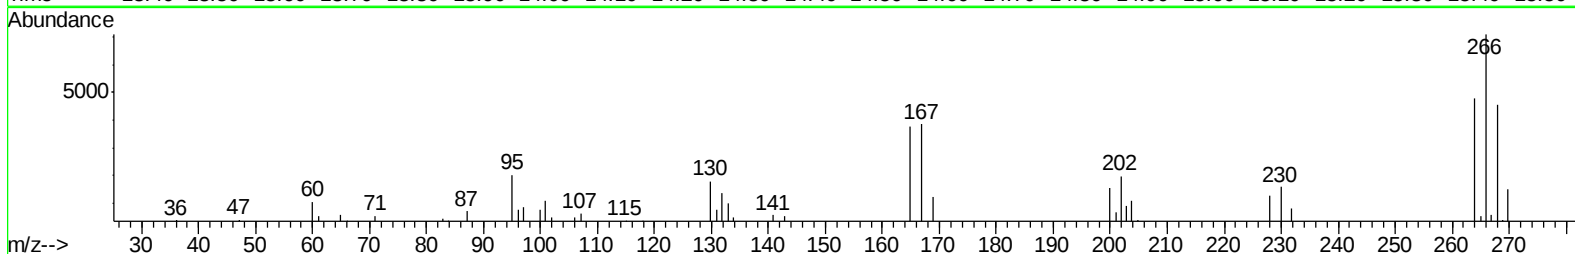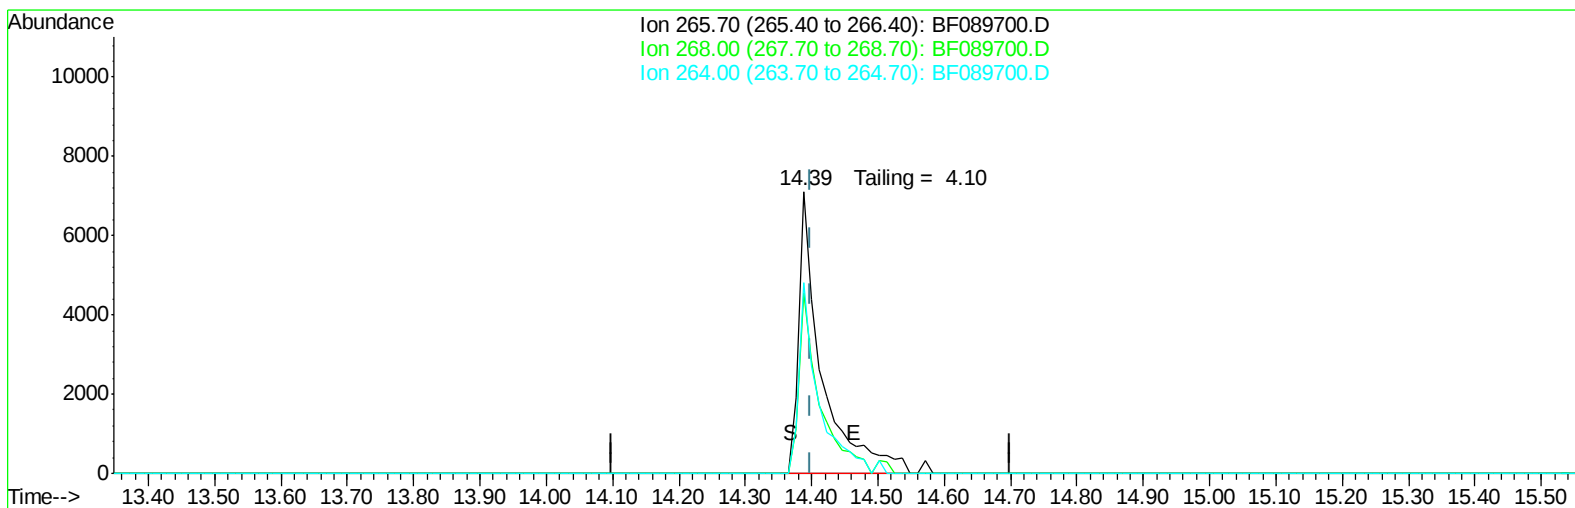

TIC: BF089700.D

(69) Pentachlorophenol (C)

14.388min (-0.012) 0.00ng

response 16904

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.98
264.00	61.90	67.65
0.00	0.00	0.00