
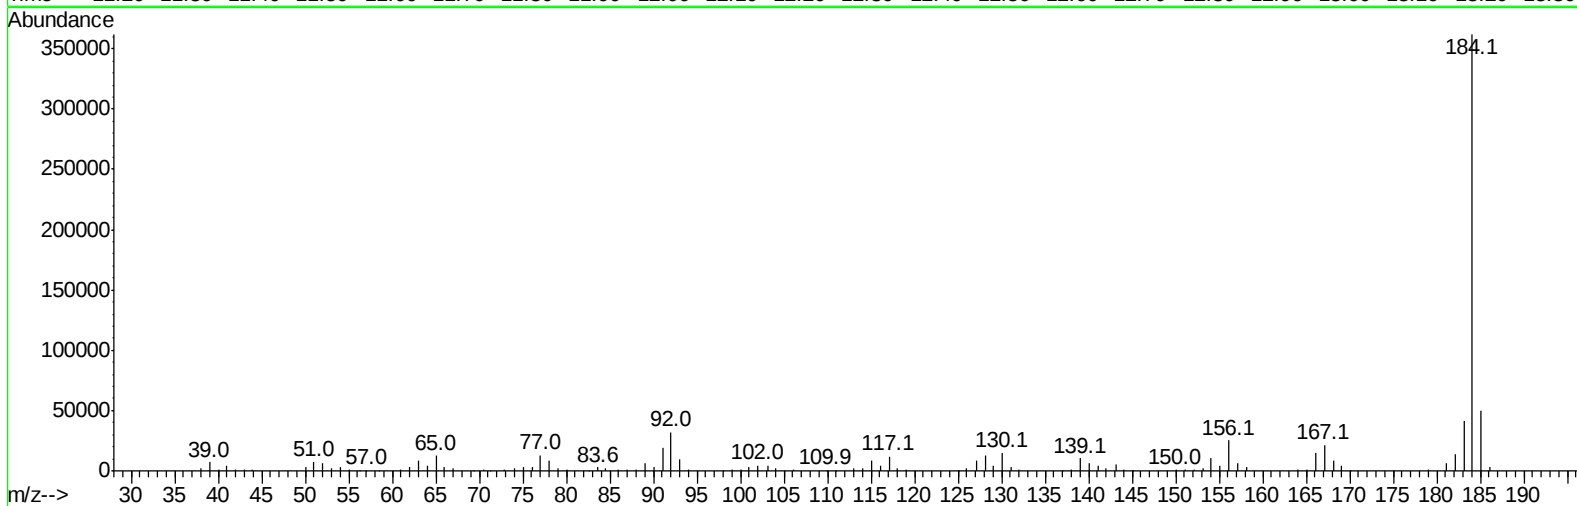


Data Path : Z:\HPCHEM1\BNA F\Data\BF081017\
Data File : BF097559.D
Acq On : 10 Aug 2017 15:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 08:17:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

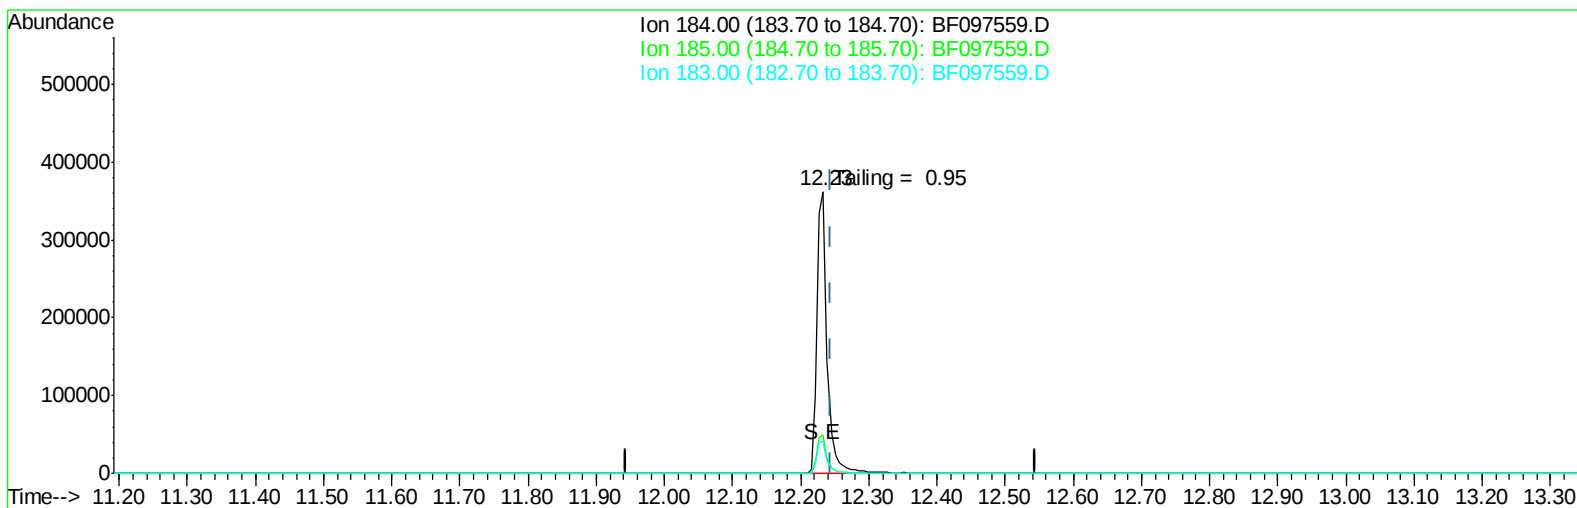

TIC: BF097559.D

(76) Benzidine



12.233min (-0.012) 0.00ng

response 380614

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.79#
183.00	12.20	11.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF081017\
Data File : BF097559.D
Acq On : 10 Aug 2017 15:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 08:17:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

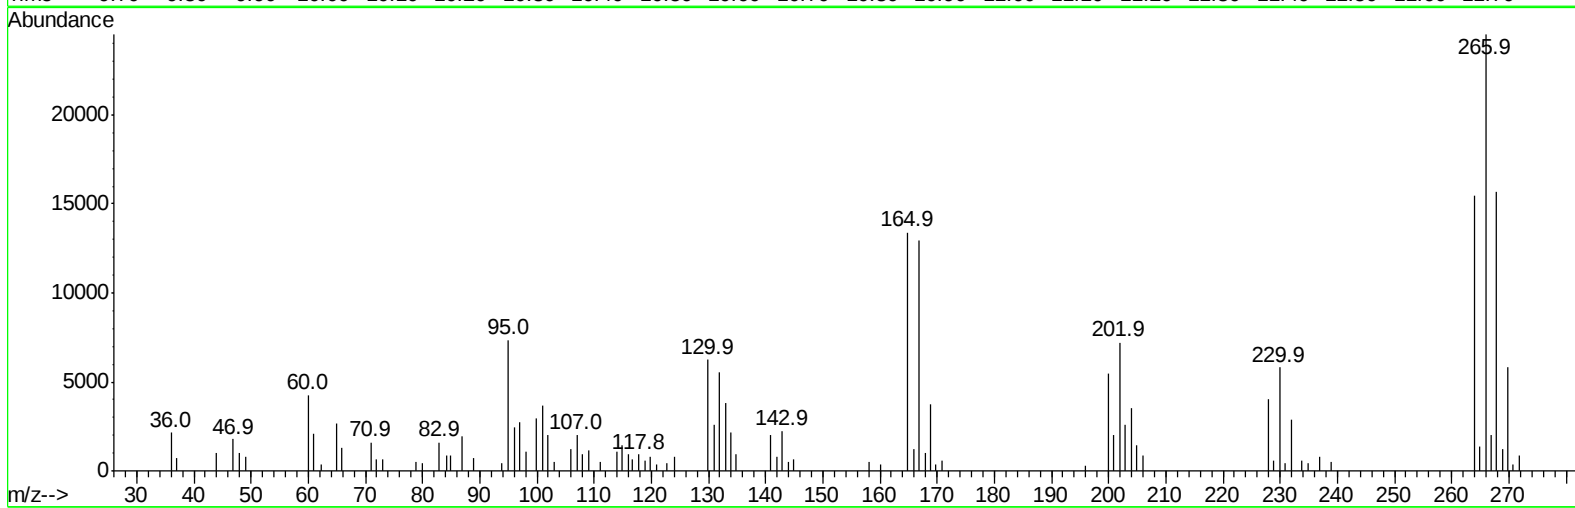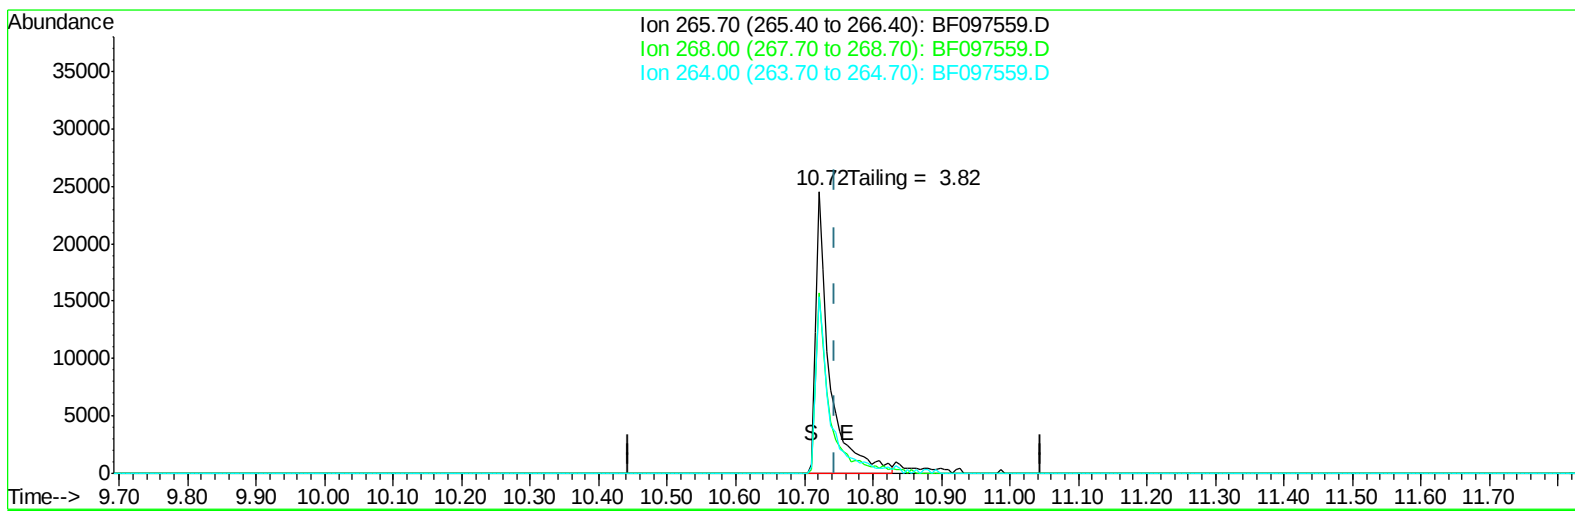

TIC: BF097559.D

(69) Pentachlorophenol (C)

10.722min (-0.023) 62838.08ng

response 35498

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.92
264.00	64.60	62.97
0.00	0.00	0.00