


Data Path : Z:\HPCHEM1\BNA F\Data\BF081017\
 Data File : BF097559.D
 Acq On : 10 Aug 2017 15:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

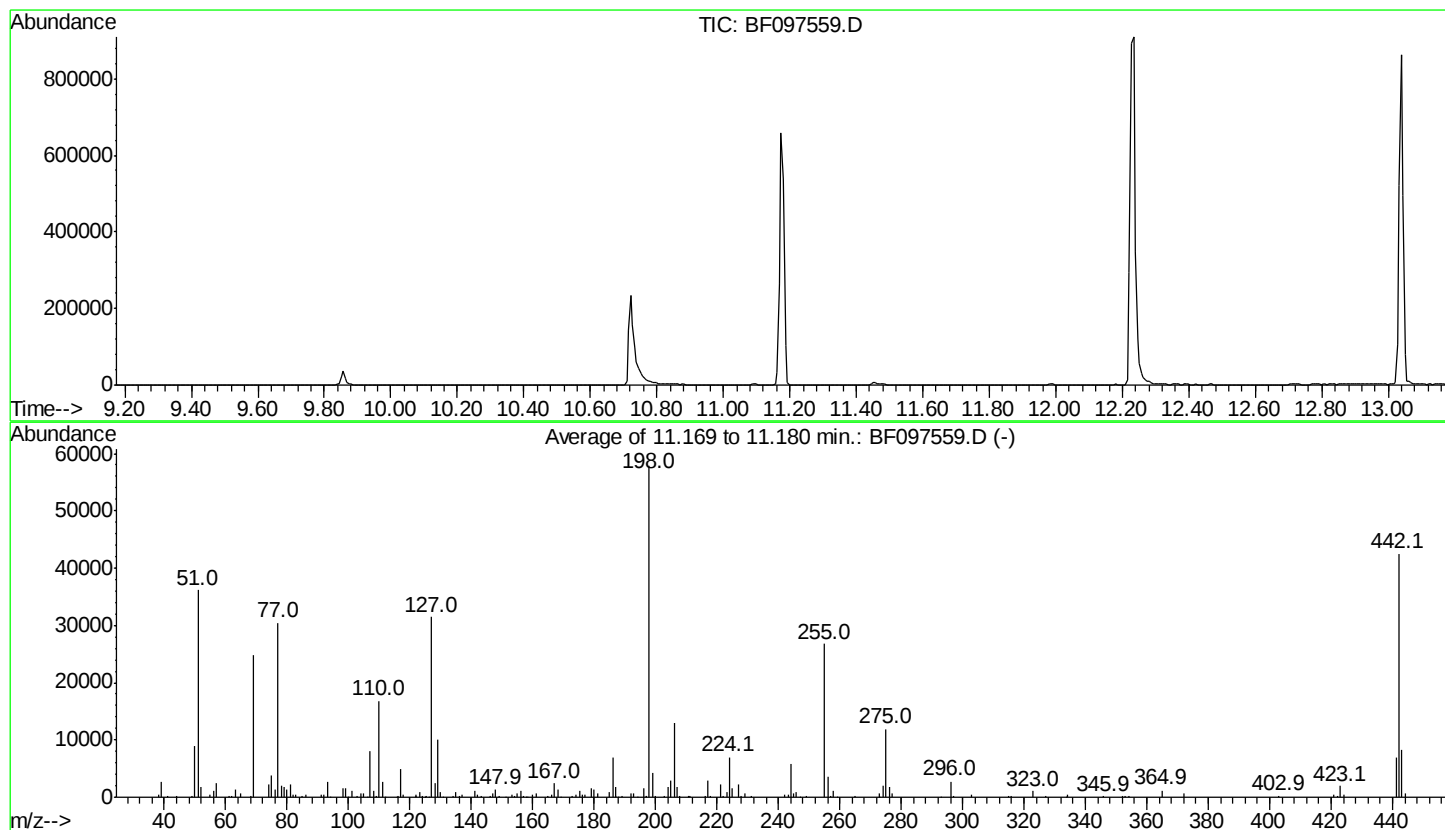

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.4	36112	PASS
68	69	0.00	2	1.3	330	PASS
69	198	0.00	100	42.9	24832	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	31445	PASS
197	198	0.00	2	0.4	248	PASS
198	198	100	100	100.0	57885	PASS
199	198	5	9	7.3	4216	PASS
275	198	10	60	20.5	11845	PASS
365	198	1	100	2.0	1136	PASS
441	442	0.01	24	16.5	6996	PASS
442	198	50	100	73.5	42525	PASS
443	442	15	24	19.2	8180	PASS