


Data Path : Z:\HPCHEM1\BNA F\Data\BF081017\
 Data File : BF097584.D
 Acq On : 11 Aug 2017 3:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

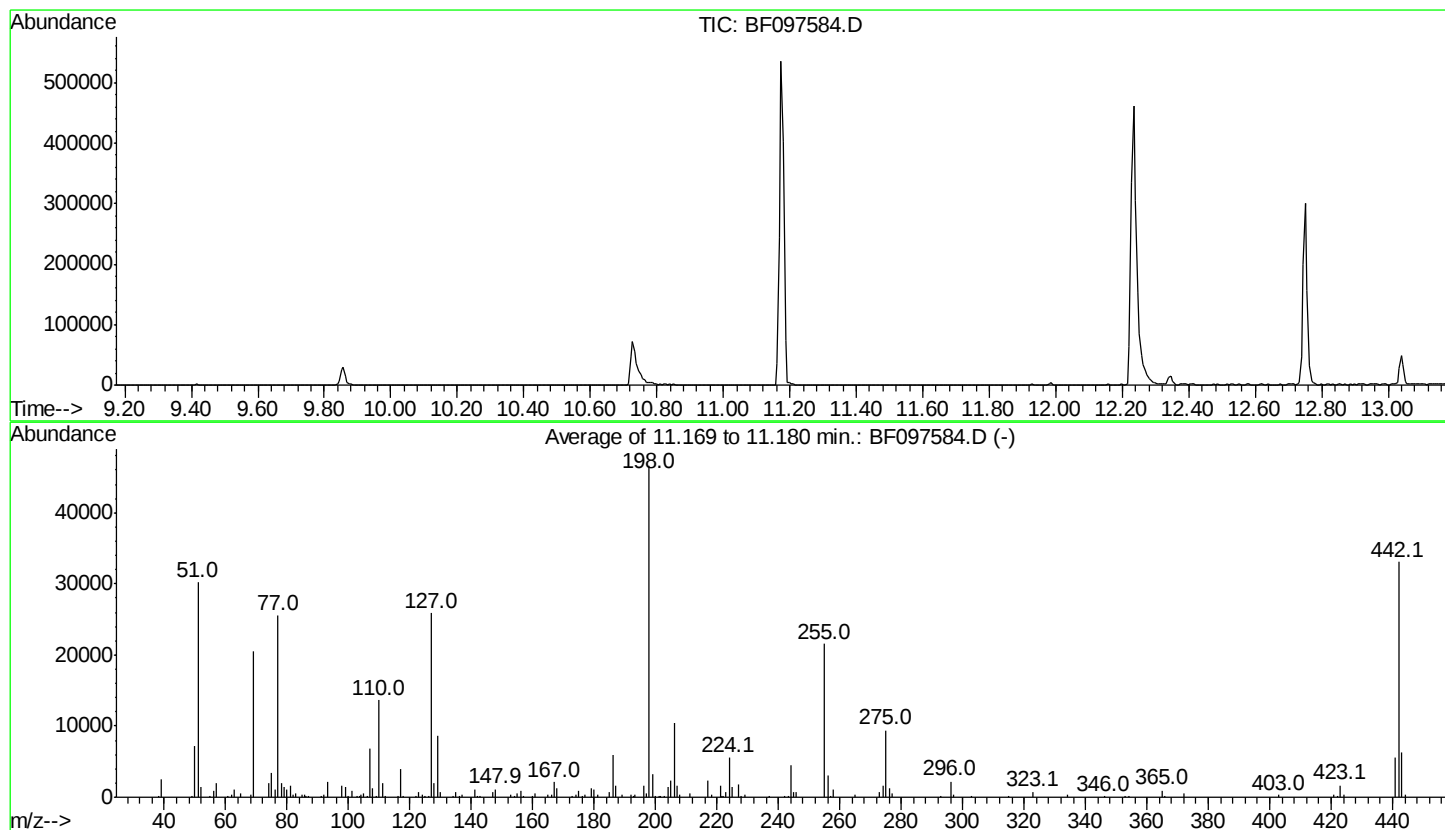

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.7	30189	PASS
68	69	0.00	2	1.8	370	PASS
69	198	0.00	100	44.2	20600	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.6	25912	PASS
197	198	0.00	2	1.1	501	PASS
198	198	100	100	100.0	46629	PASS
199	198	5	9	6.8	3156	PASS
275	198	10	60	20.1	9363	PASS
365	198	1	100	2.1	995	PASS
441	442	0.01	24	16.8	5566	PASS
442	198	50	100	70.9	33044	PASS
443	442	15	24	19.3	6372	PASS