
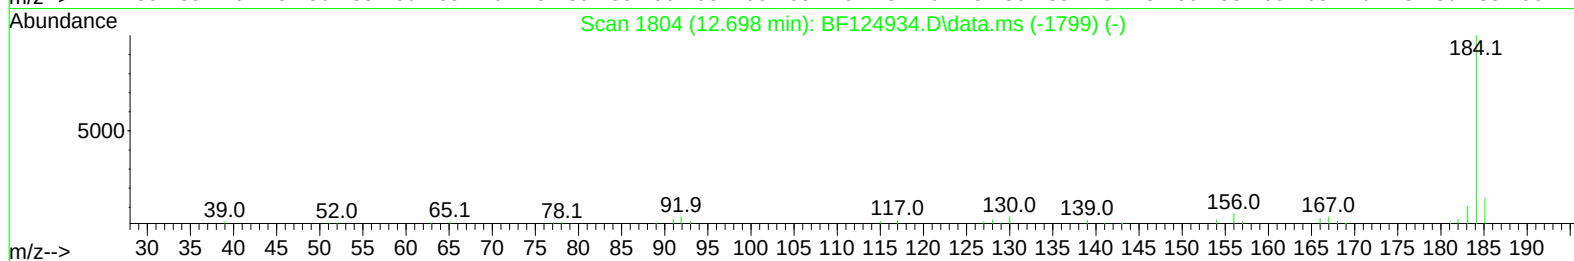
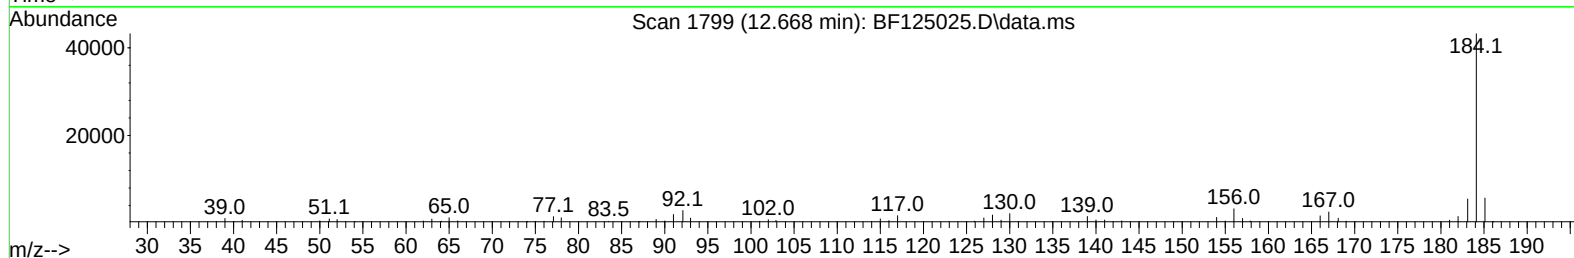


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125025.D
 Acq On : 10 Aug 2021 10:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 11:29:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 11:03:44 2021
 Response via : Initial Calibration

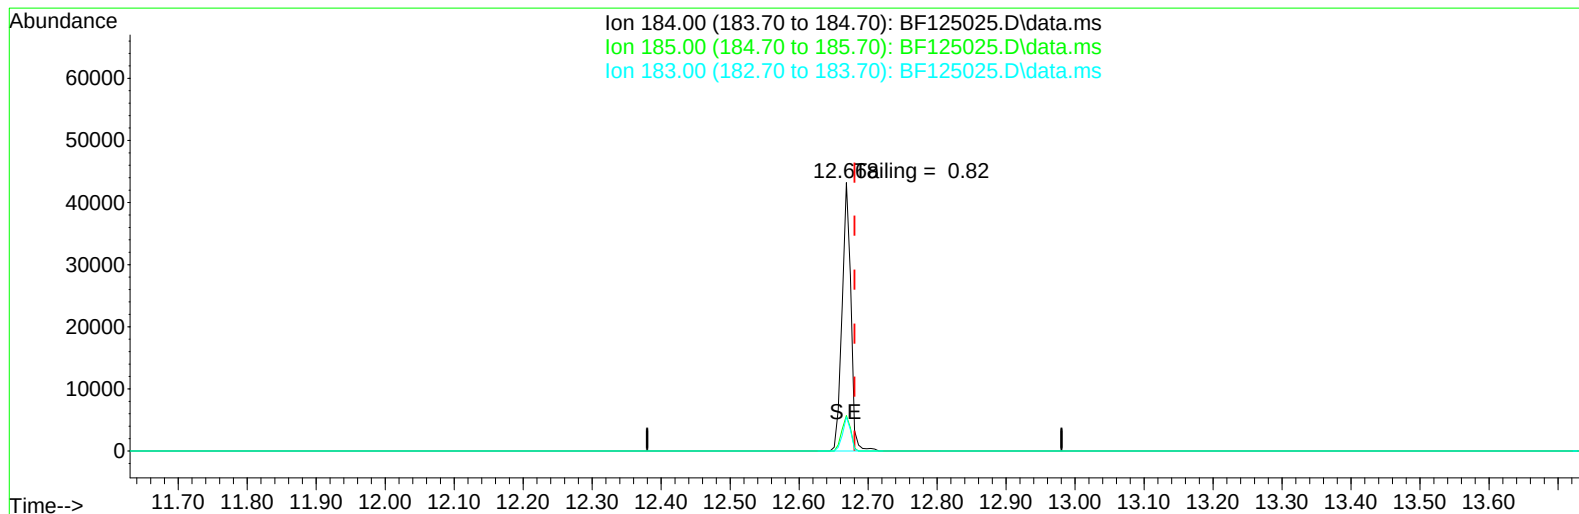

TIC: BF125025.D\data.ms

(77) Benzidine




12.668min (-0.012) 0.00 ng

response 38069

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.20
183.00	10.10	12.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125025.D
 Acq On : 10 Aug 2021 10:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 11:29:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 11:03:44 2021
 Response via : Initial Calibration

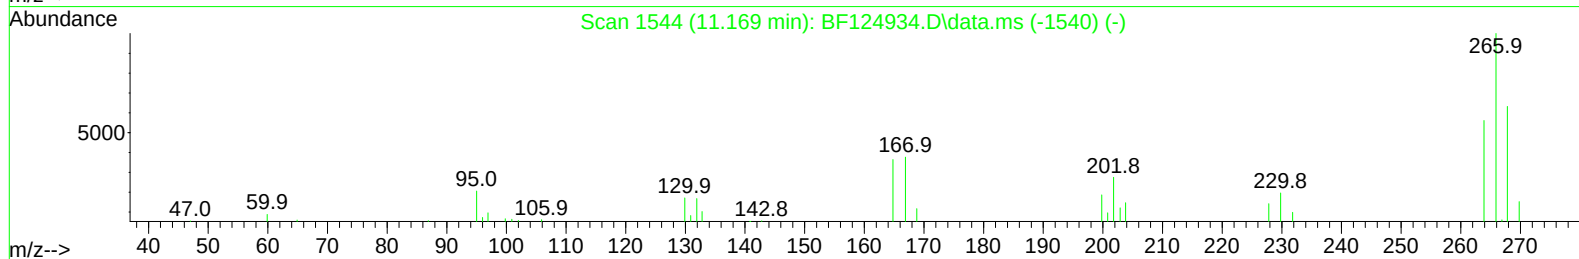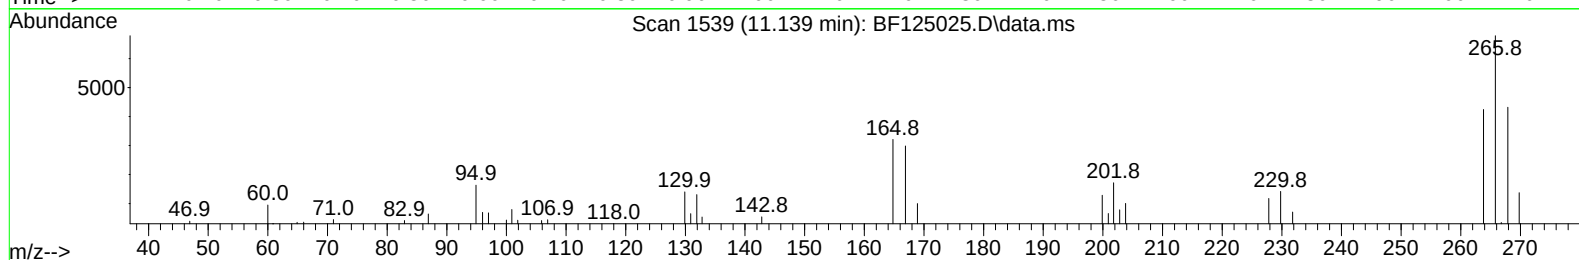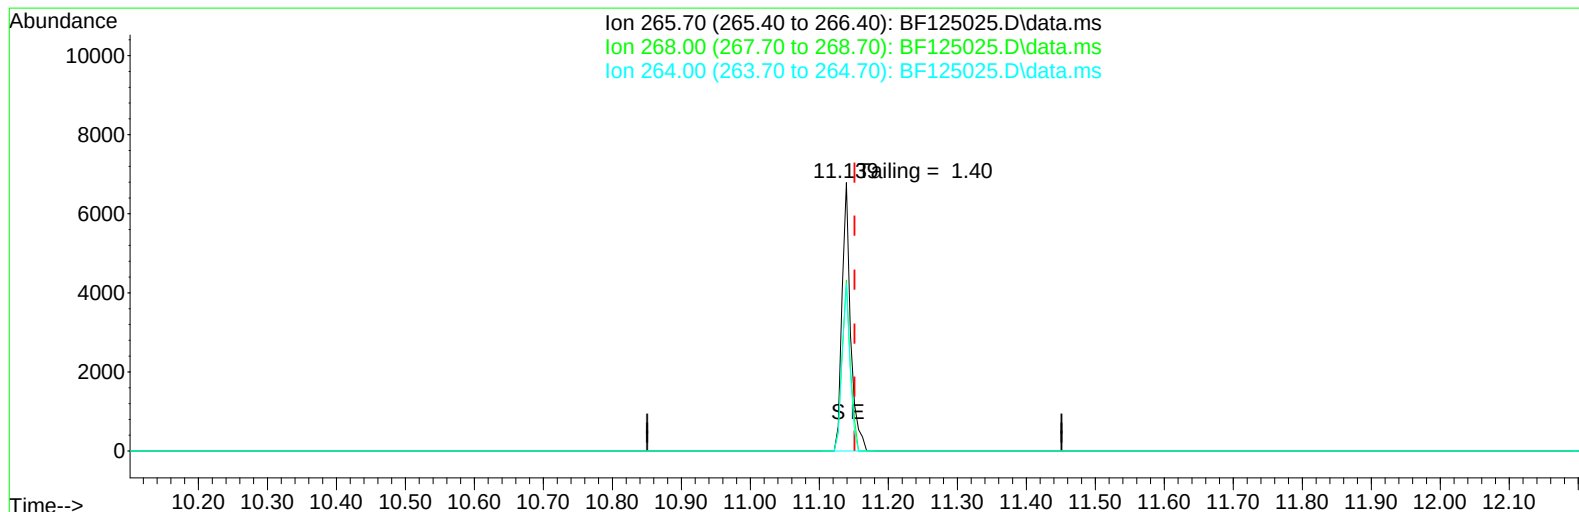

TIC: BF125025.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.012) 0.00 ng

response 5831

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.63
264.00	69.90	62.51
0.00	0.00	0.00