
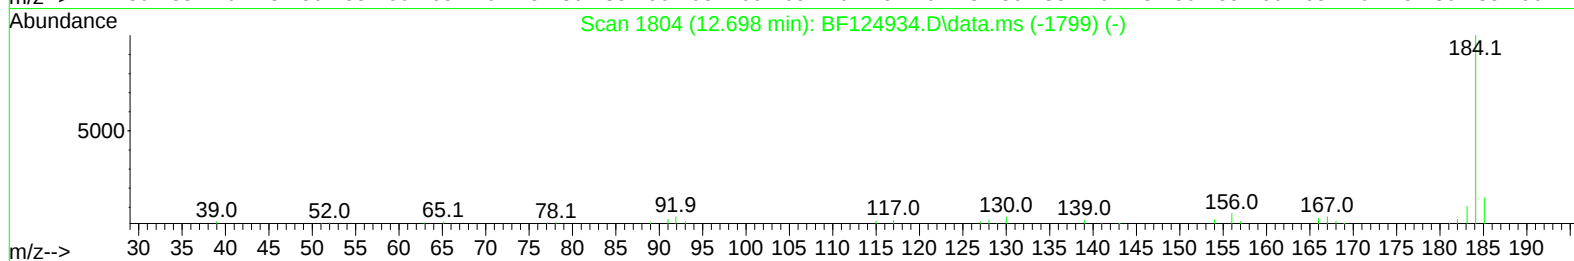
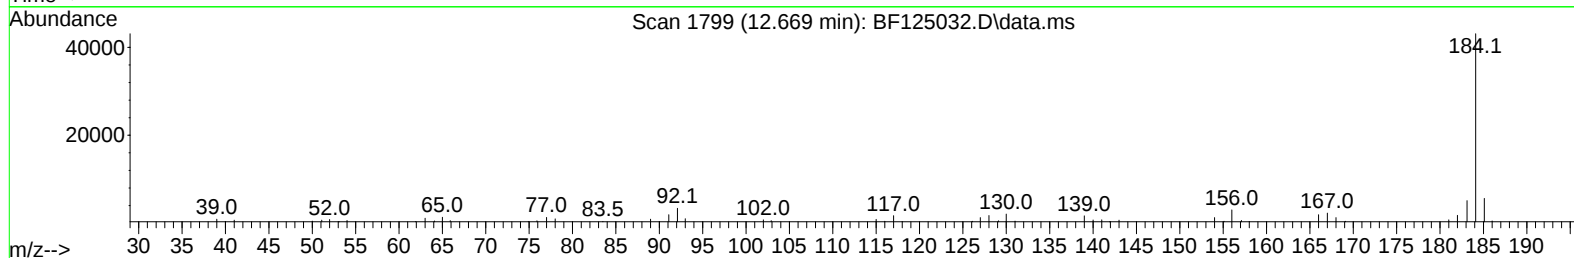


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125032.D
Acq On : 10 Aug 2021 15:54
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 18:10:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 10 11:32:36 2021
Response via : Initial Calibration

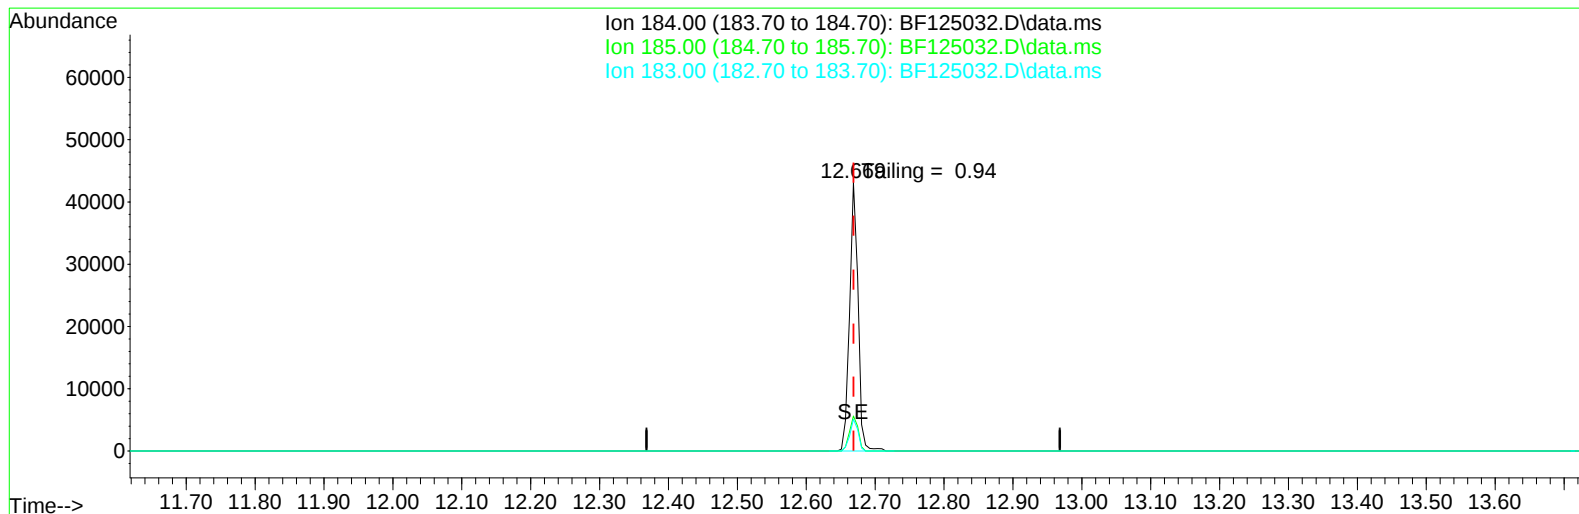

TIC: BF125032.D\data.ms

(77) Benzidine




12.669min (+ 0.000) 0.00 ng

response 36915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.08
183.00	10.10	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125032.D
 Acq On : 10 Aug 2021 15:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 18:10:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 10 11:32:36 2021
 Response via : Initial Calibration

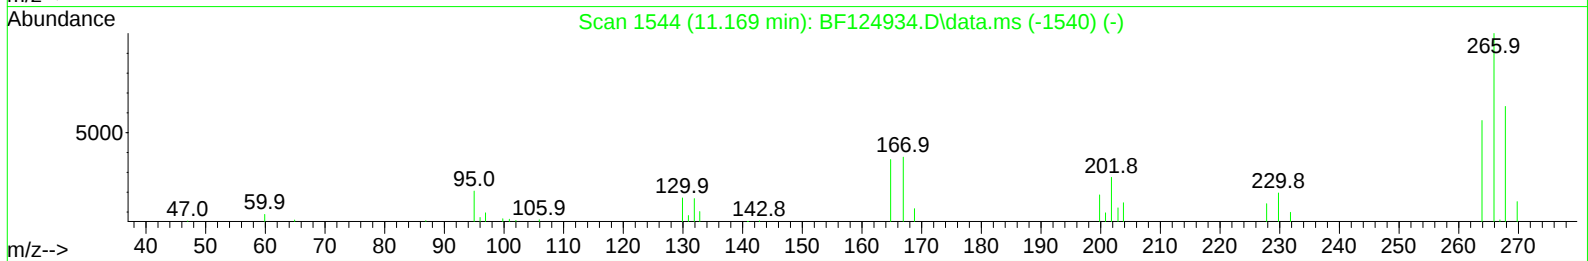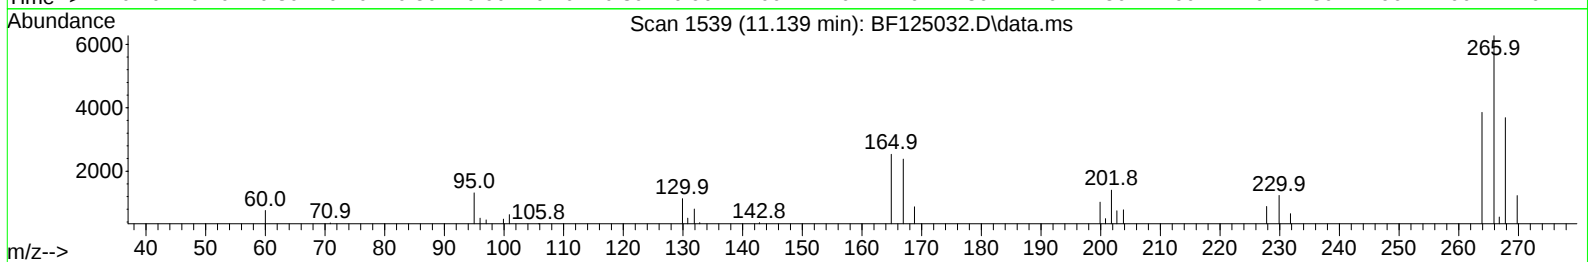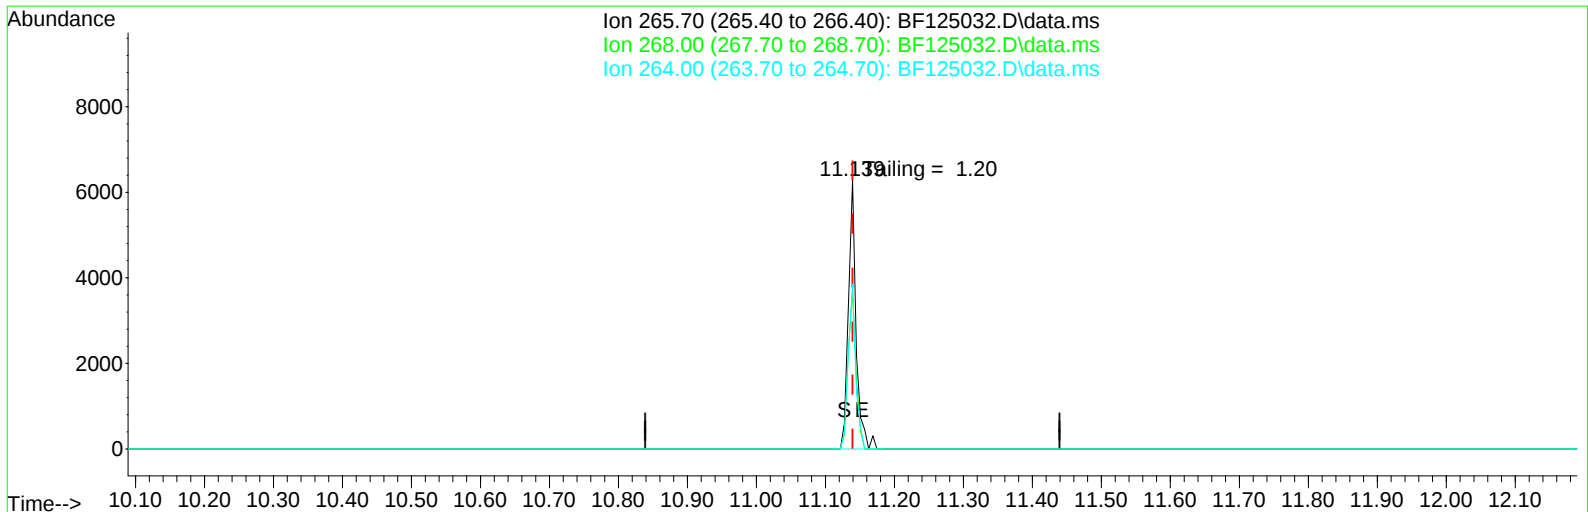

TIC: BF125032.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 0.00 ng

response 4942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	58.77
264.00	69.90	61.48
0.00	0.00	0.00