

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125030.D
 Acq On : 10 Aug 2021 14:36
 Operator : JU/CG
 Sample : SP5637
 Misc : 625 SURROGATE
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP5637

Quant Time: Aug 10 15:13:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 10 11:32:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.810	152	6069	20.000	ng	0.00
21) Naphthalene-d8	8.092	136	24428	20.000	ng	0.00
39) Acenaphthene-d10	9.845	164	9726	20.000	ng	0.00
64) Phenanthrene-d10	11.333	188	26399	20.000	ng	0.00
76) Chrysene-d12	13.968	240	19875	20.000	ng	# 0.00
86) Perylene-d12	15.415	264	17038	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.445	112	37387	100.913	ng	0.01
7) Phenol-d6	6.445	99	52522	112.428	ng	0.00
23) Nitrobenzene-d5	7.375	82	52355	112.119	ng	0.00
42) 2,4,6-Tribromophenol	10.639	330	13528	155.688	ng	0.00
45) 2-Fluorobiphenyl	9.169	172	71543	107.634	ng	0.00
79) Terphenyl-d14	12.921	244	127173	107.934	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125030.D
Acq On : 10 Aug 2021 14:36
Operator : JU/CG
Sample : SP5637
Misc : 625 SURROGATE
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP5637

Quant Time: Aug 10 15:13:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 10 11:32:36 2021
Response via : Initial Calibration




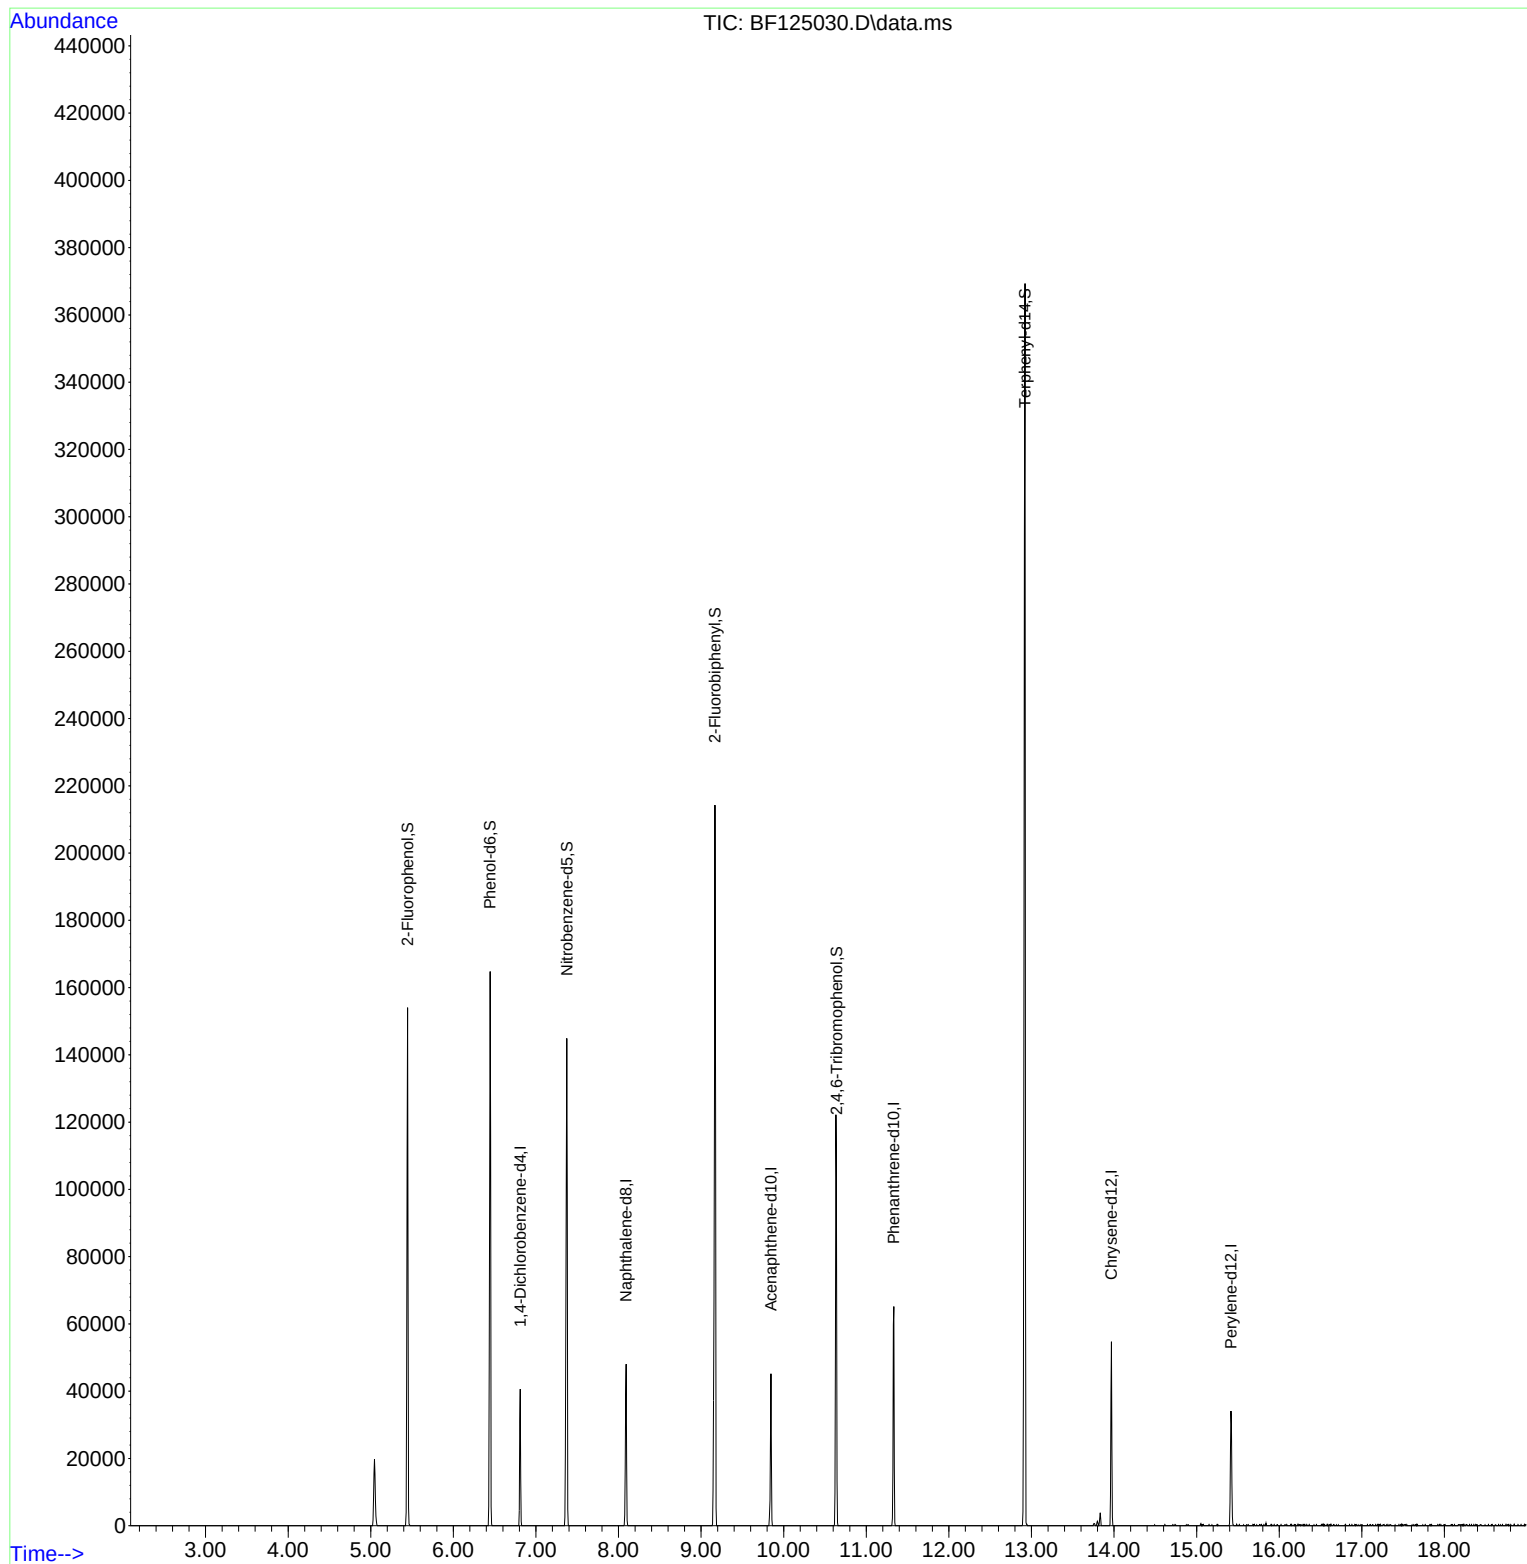


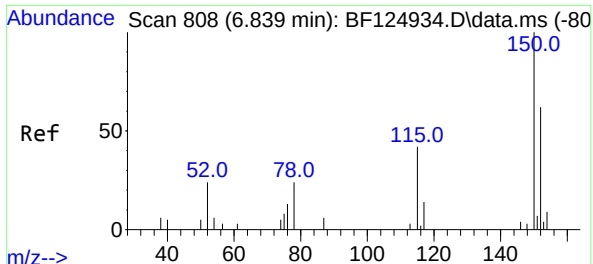

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.810 min Scan# 803
Delta R.T. -0.006 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36




Instrument :
BNA_F
ClientSampled :
SP5637

Tgt Ion:152 Resp: 6069
Ion Ratio Lower Upper
152 100
150 144.1 117.6 176.4
115 60.3 47.1 70.7

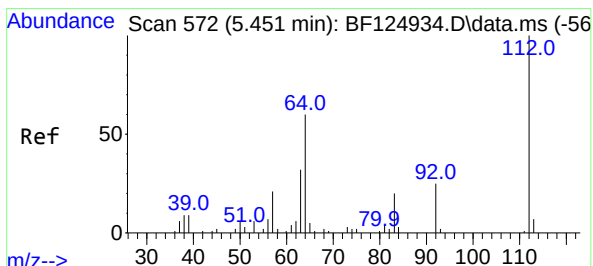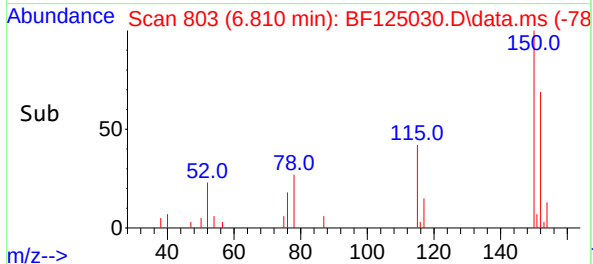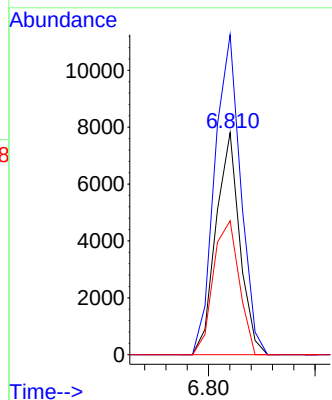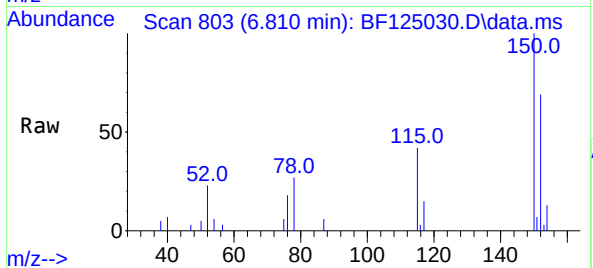


#5
2-Fluorophenol
Concen: 100.913 ng
RT: 5.445 min Scan# 571
Delta R.T. 0.012 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36


Tgt Ion:112 Resp: 37387
Ion Ratio Lower Upper
112 100
64 64.6 44.2 66.2
63 36.2 26.2 39.2

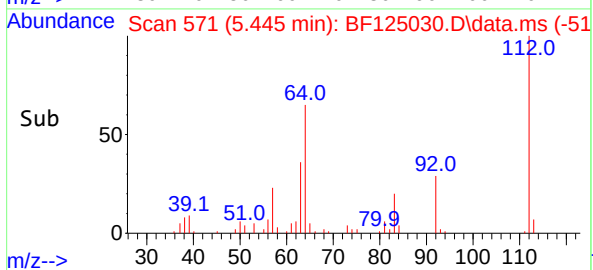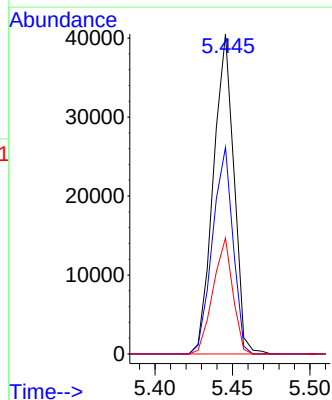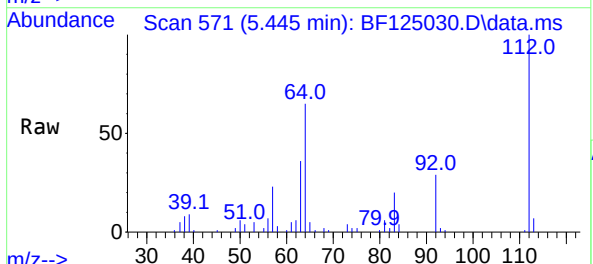


Abundance Scan 745 (6.469 min): BF124934.D\data.ms (-73

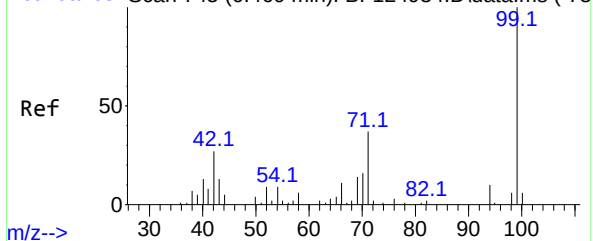


m/z--> Scan 741 (6.445 min): BF125030.D\data.ms

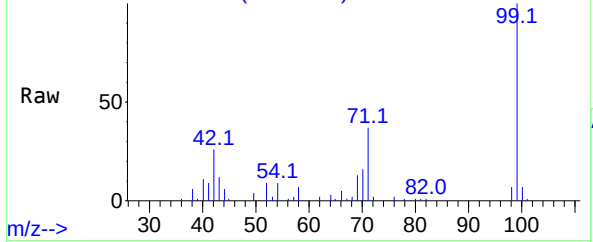


Abundance Scan 741 (6.445 min): BF125030.D\data.ms (-69

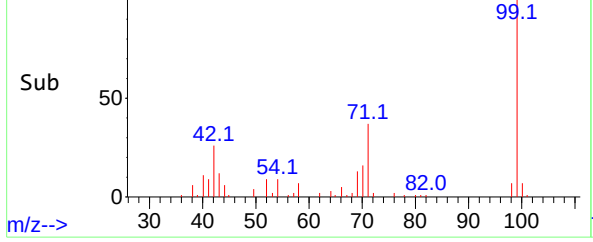


m/z--> Scan 1026 (8.122 min): BF124934.D\data.ms (-1

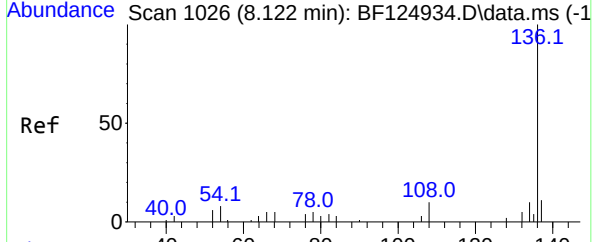

m/z--> Scan 1021 (8.092 min): BF125030.D\data.ms

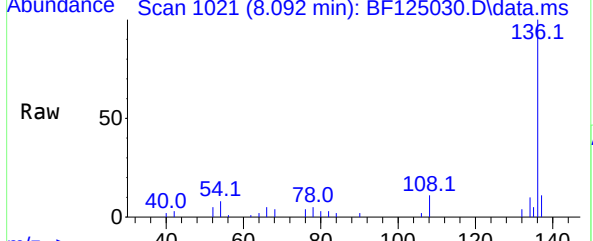

Abundance Scan 1021 (8.092 min): BF125030.D\data.ms (-9

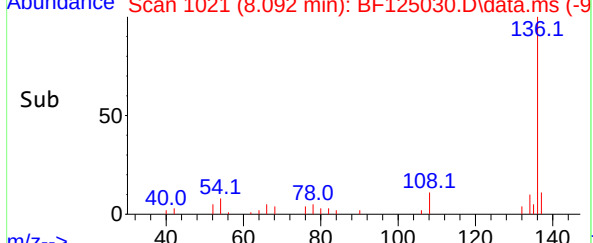

m/z--> Scan 1021 (8.092 min): BF125030.D\data.ms (-9

#7

Phenol-d6

Concen: 112.428 ng

RT: 6.445 min Scan# 741

Delta R.T. -0.006 min


Lab File: BF125030.D

Acq: 10 Aug 2021 14:36

Tgt Ion: 99 Resp: 52522

Ion	Ratio	Lower	Upper
99	100		
42	26.1	23.5	35.3
71	36.8	25.6	38.4

Abundance

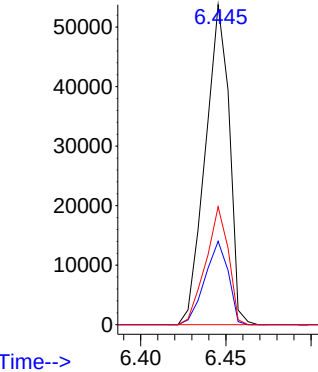

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.092 min Scan# 1021

Delta R.T. -0.006 min


Lab File: BF125030.D


Acq: 10 Aug 2021 14:36

Tgt Ion: 136 Resp: 24428

Ion	Ratio	Lower	Upper
136	100		
137	10.5	9.8	14.6
54	8.3	6.4	9.6
68	4.4	3.3	4.9

Abundance

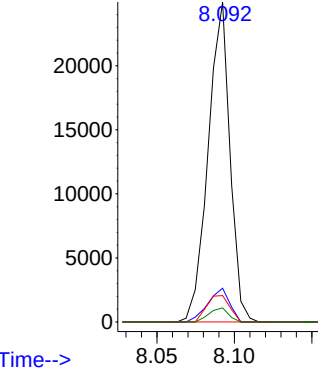

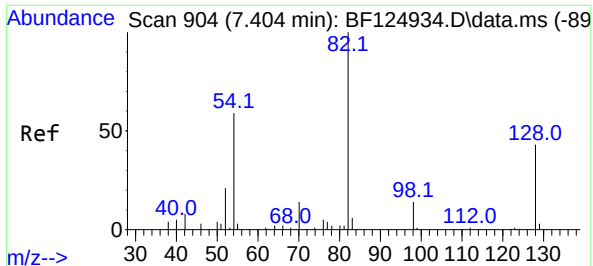

#23

Nitrobenzene-d5

Concen: 112.119 ng

RT: 7.375 min Scan# 899

Delta R.T. -0.006 min

Lab File: BF125030.D

Acq: 10 Aug 2021 14:36





Tgt Ion: 82 Resp: 52355

Ion Ratio Lower Upper

82 100

128 43.2 40.6 60.8

54 59.1 49.6 74.4

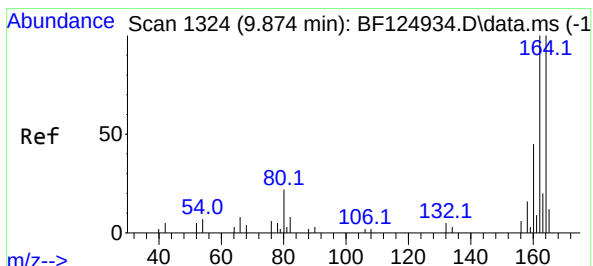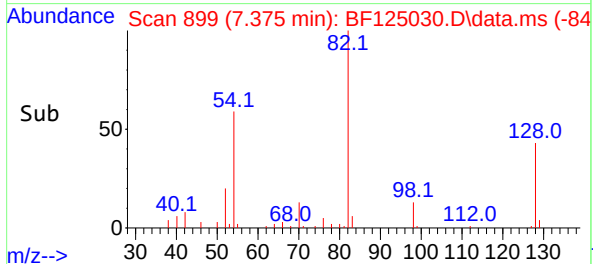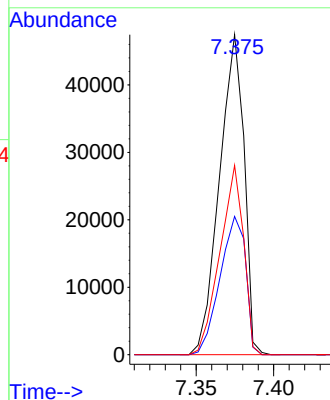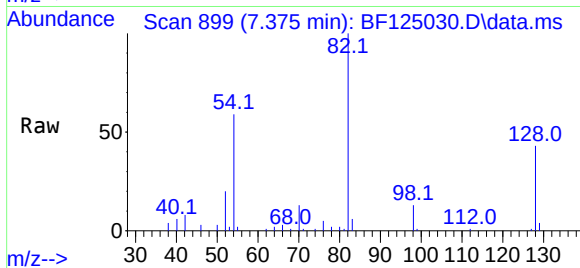

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.845 min Scan# 1319

Delta R.T. -0.006 min

Lab File: BF125030.D

Acq: 10 Aug 2021 14:36




Tgt Ion: 164 Resp: 9726


Ion Ratio Lower Upper

164 100

162 103.7 81.3 121.9

160 45.3 38.0 57.0


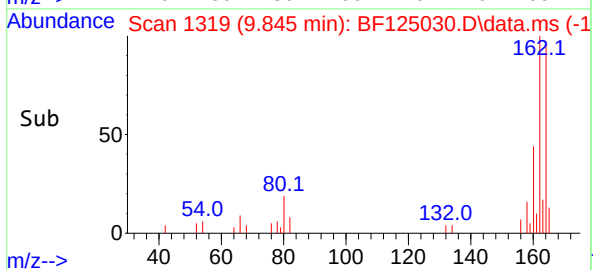
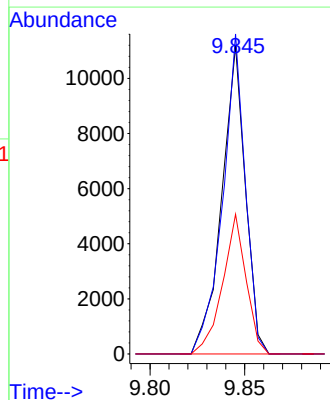
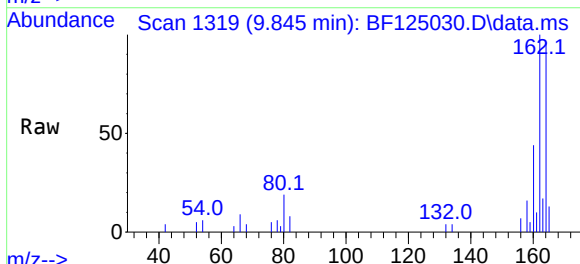


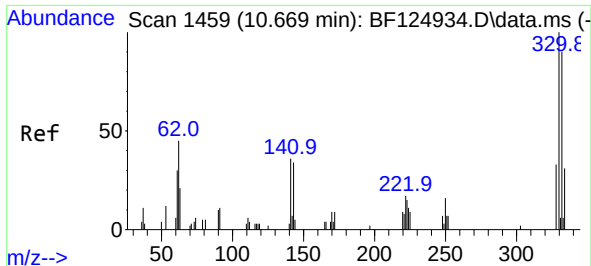

#42
2,4,6-Tribromophenol
Concen: 155.688 ng
RT: 10.639 min Scan# 1454
Delta R.T. 0.000 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36




Instrument :
BNA_F
ClientSampled :
SP5637


Tgt Ion: 330 Resp: 13528
Ion Ratio Lower Upper
330 100
332 95.4 76.2 114.4
141 40.5 44.6 66.8#

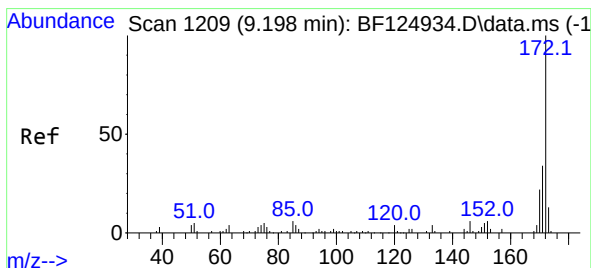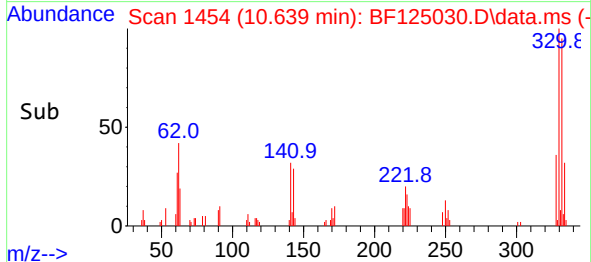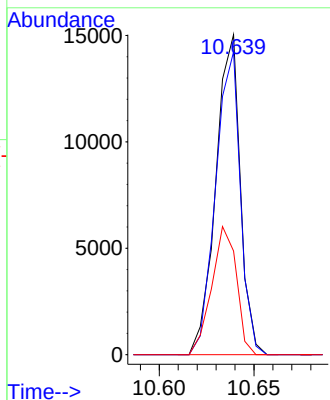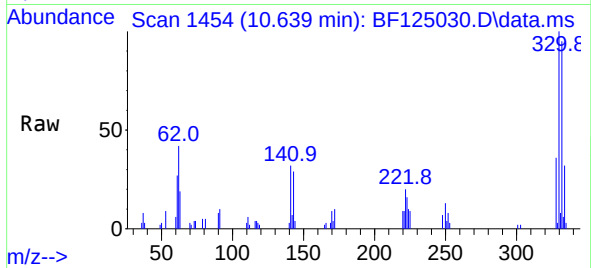

#45
2-Fluorobiphenyl
Concen: 107.634 ng
RT: 9.169 min Scan# 1204
Delta R.T. -0.006 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36

Tgt Ion: 172 Resp: 71543
Ion Ratio Lower Upper
172 100
171 36.6 26.5 39.7
170 22.2 18.8 28.2


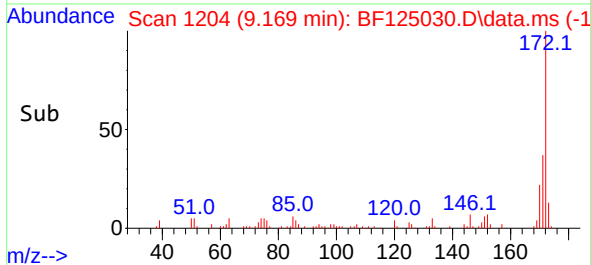
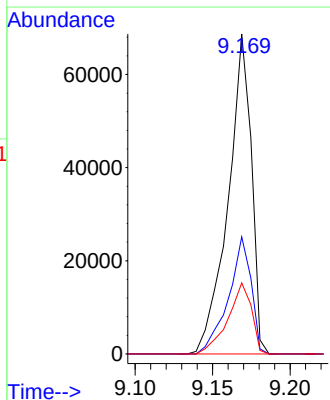
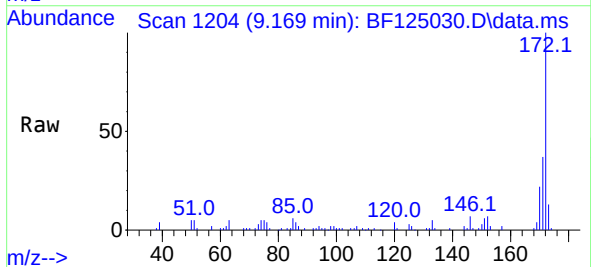


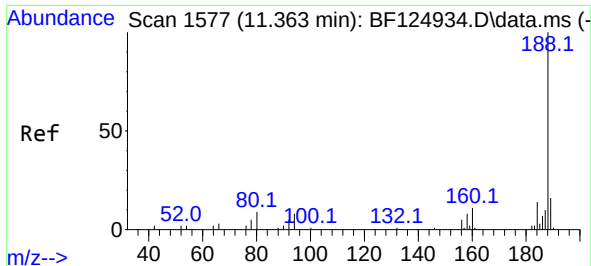

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.333 min Scan# 1572
Delta R.T. 0.000 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36




Instrument :
BNA_F
ClientSampleID :
SP5637


Tgt Ion:188 Resp: 26399
Ion Ratio Lower Upper
188 100
94 7.8 6.7 10.1
80 9.4 7.5 11.3

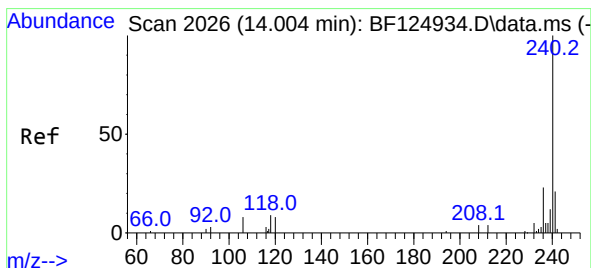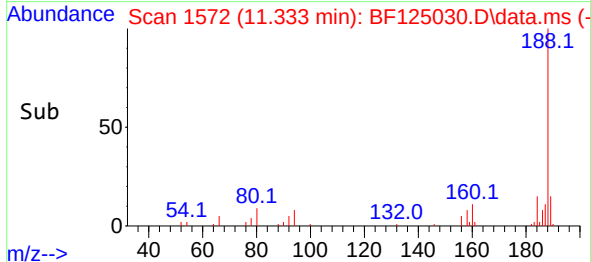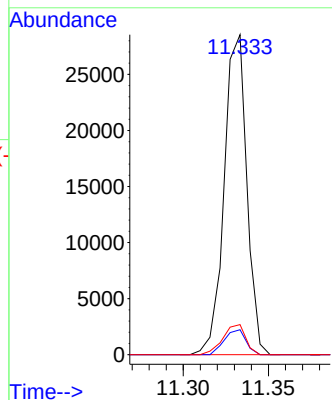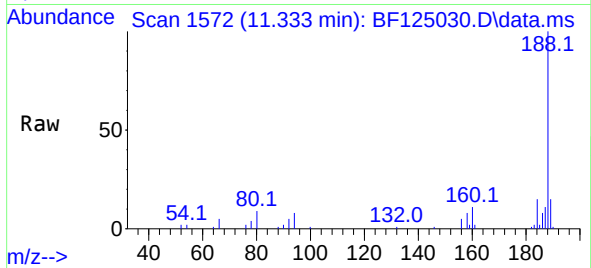

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.968 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36

Tgt Ion:240 Resp: 19875
Ion Ratio Lower Upper
240 100
120 10.3 10.8 16.2#
236 25.7 21.6 32.4


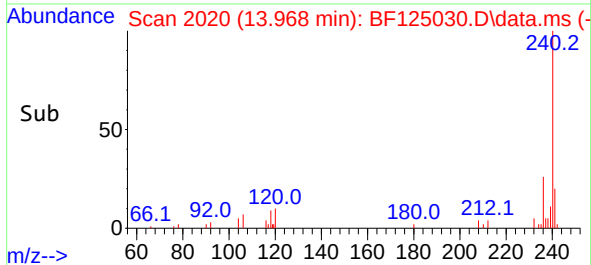
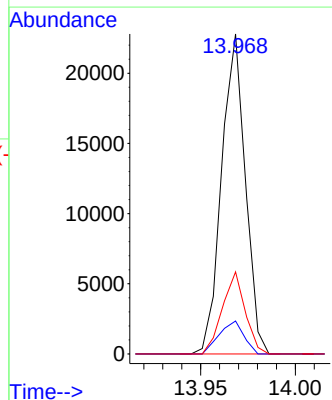
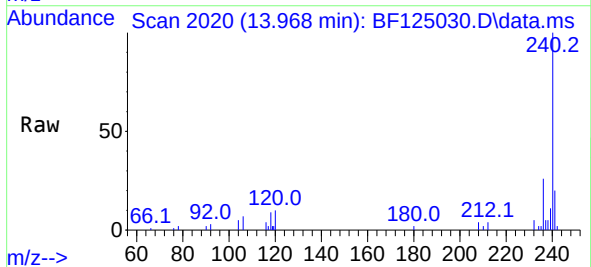


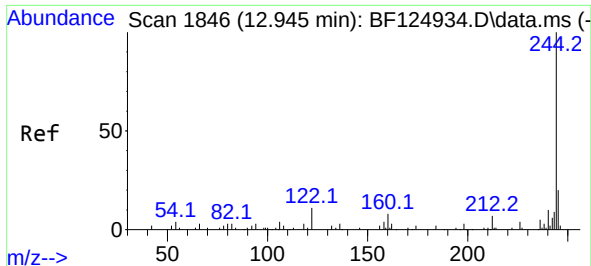

#79
Terphenyl-d14
Concen: 107.934 ng
RT: 12.921 min Scan# 1842
Delta R.T. 0.006 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36

Instrument :
BNA_F
ClientSampled :
SP5637

Tgt Ion:244 Resp: 127173
Ion Ratio Lower Upper
244 100
212 6.7 5.9 8.9
122 9.4 9.0 13.4

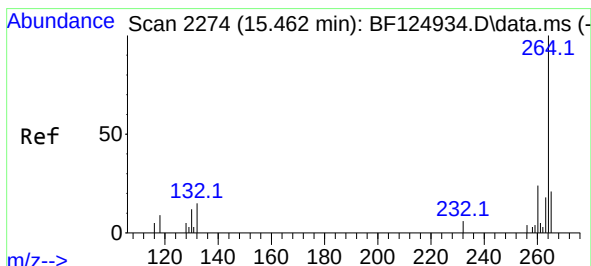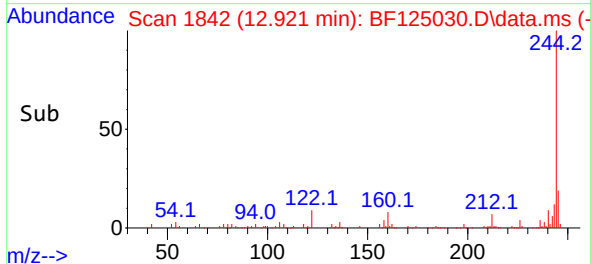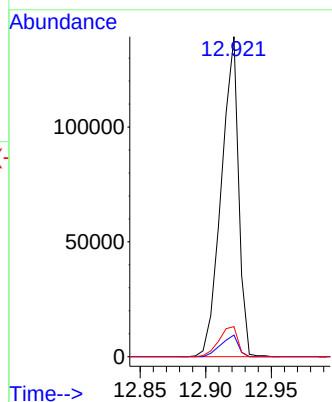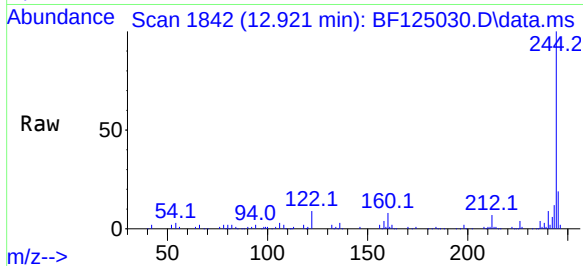

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.415 min Scan# 2266
Delta R.T. 0.000 min
Lab File: BF125030.D
Acq: 10 Aug 2021 14:36

Tgt Ion:264 Resp: 17038
Ion Ratio Lower Upper
264 100
260 23.3 19.6 29.4
265 21.3 17.2 25.8

