

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125041.D
 Acq On : 10 Aug 2021 21:05
 Operator : JU/CG
 Sample : M3318-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20210540-COM-13

Quant Time: Aug 11 04:15:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 10 11:32:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.810	152	3870	20.000	ng	# 0.00
21) Naphthalene-d8	8.092	136	16479	20.000	ng	# 0.00
39) Acenaphthene-d10	9.845	164	9745	20.000	ng	0.00
64) Phenanthrene-d10	11.333	188	18691	20.000	ng	0.00
76) Chrysene-d12	13.969	240	13250	20.000	ng	0.00
86) Perylene-d12	15.415	264	10683	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	22315	94.456	ng	0.00
7) Phenol-d6	6.445	99	28510	95.706	ng	0.00
23) Nitrobenzene-d5	7.375	82	20806	66.049	ng	0.00
42) 2,4,6-Tribromophenol	10.639	330	8570	98.436	ng	0.00
45) 2-Fluorobiphenyl	9.169	172	32606	48.959	ng	0.00
79) Terphenyl-d14	12.916	244	38361	48.836	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125041.D
Acq On : 10 Aug 2021 21:05
Operator : JU/CG
Sample : M3318-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13

Quant Time: Aug 11 04:15:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 10 11:32:36 2021
Response via : Initial Calibration




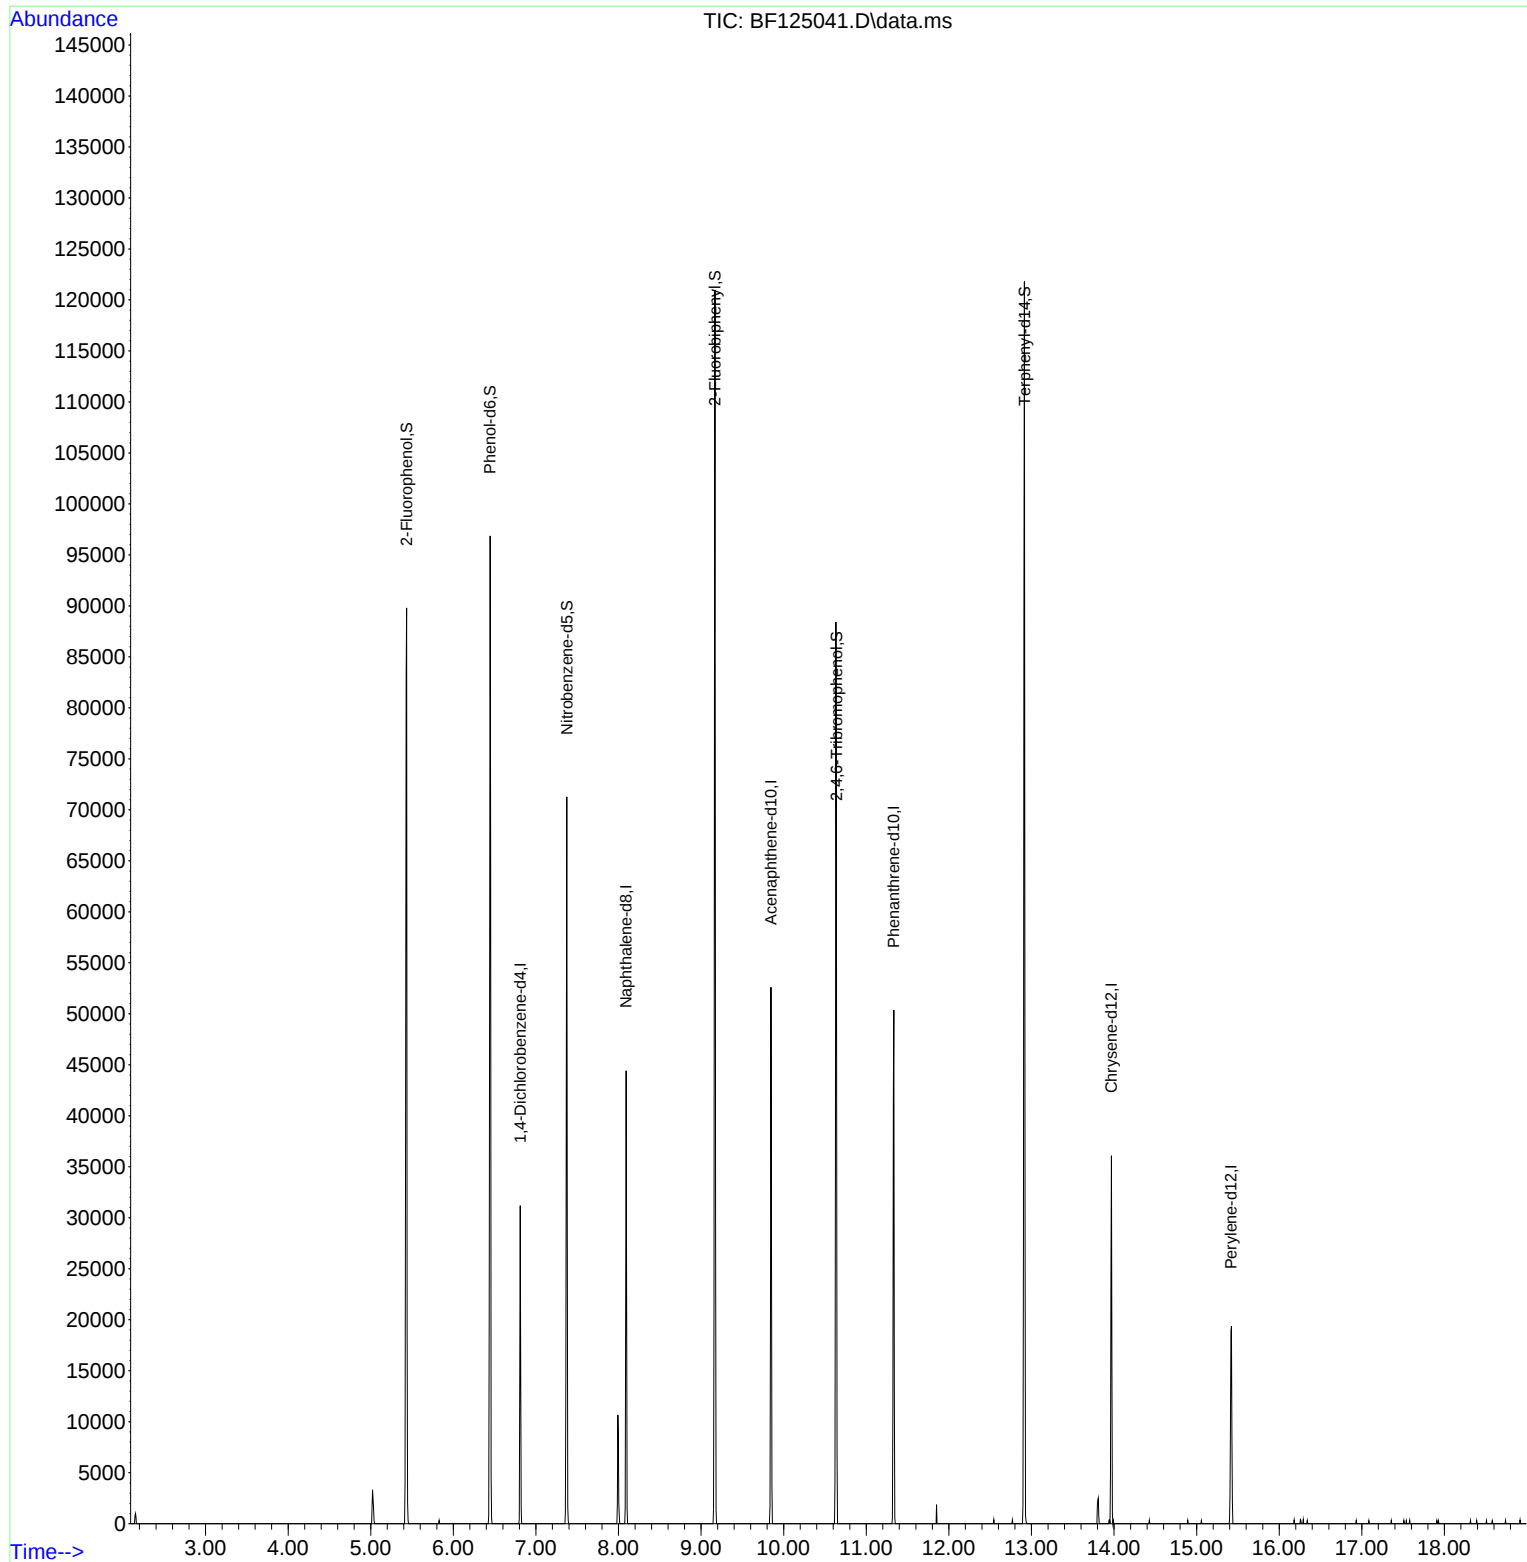


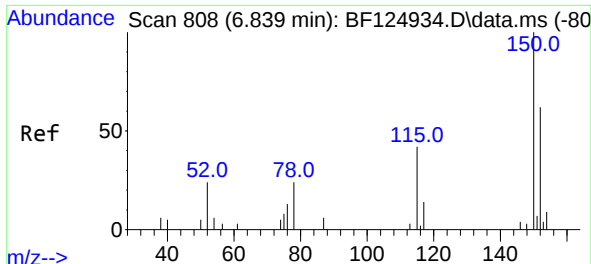

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.810 min Scan# 803
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05




Instrument :
BNA_F
ClientSampleId :
20210540-COM-13


Tgt Ion:152 Resp: 3870
Ion Ratio Lower Upper
152 100
150 181.0 117.6 176.4#
115 82.2 47.1 70.7#

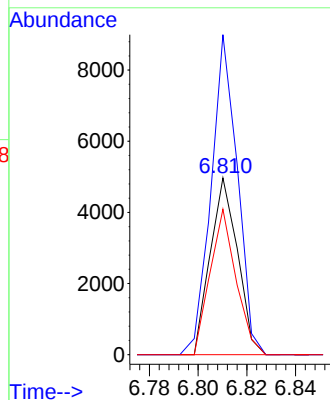

#5
2-Fluorophenol
Concen: 94.456 ng
RT: 5.434 min Scan# 569
Delta R.T. 0.000 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Tgt Ion:112 Resp: 22315
Ion Ratio Lower Upper
112 100
64 67.4 44.2 66.2#
63 36.4 26.2 39.2

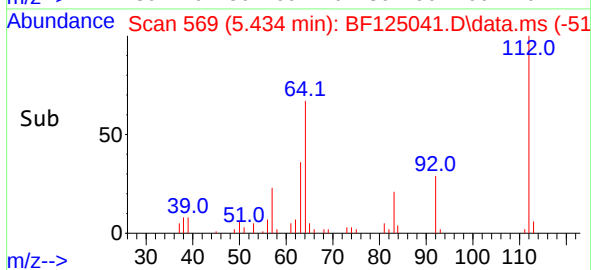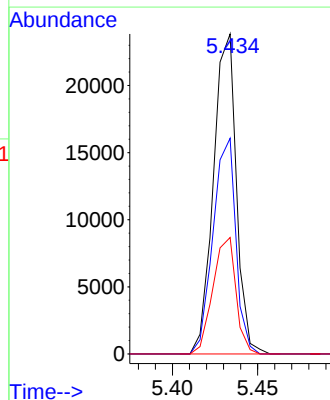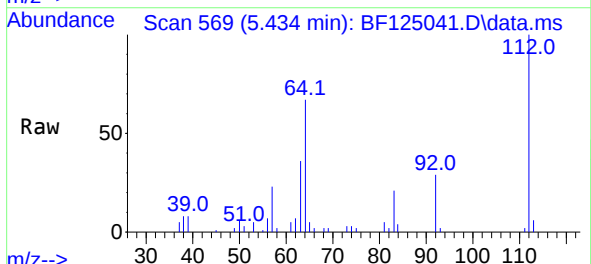




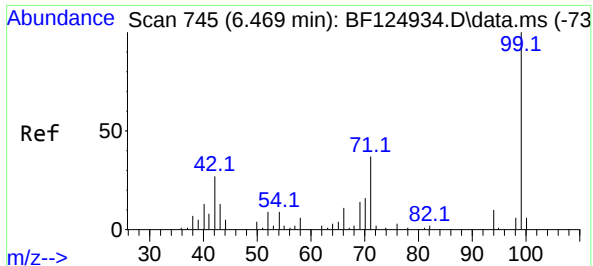


#7
Phenol-d6
Concen: 95.706 ng
RT: 6.445 min Scan# 741
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13

Tgt Ion: 99 Resp: 28510




Ion	Ratio	Lower	Upper
99	100		
42	26.4	23.5	35.3
71	41.8	25.6	38.4#

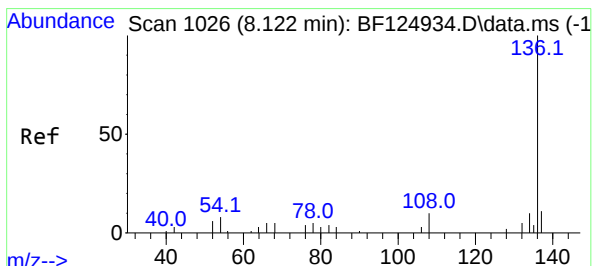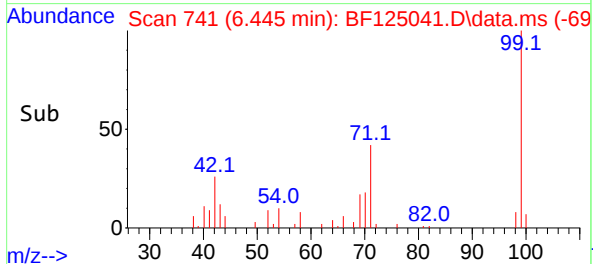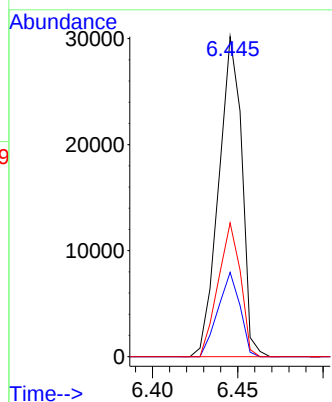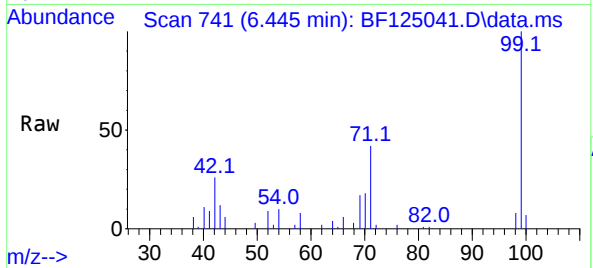


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.092 min Scan# 1021
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Tgt Ion: 136 Resp: 16479

Ion	Ratio	Lower	Upper
136	100		
137	12.2	9.8	14.6
54	8.5	6.4	9.6
68	5.7	3.3	4.9#


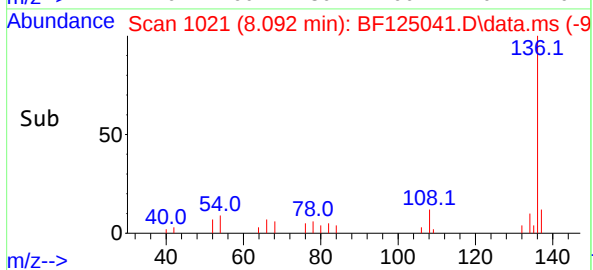
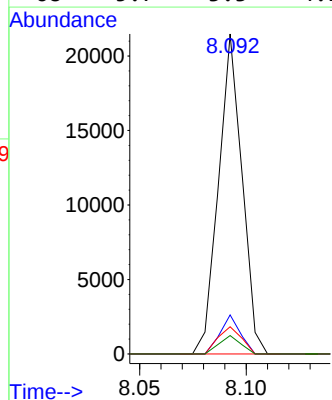
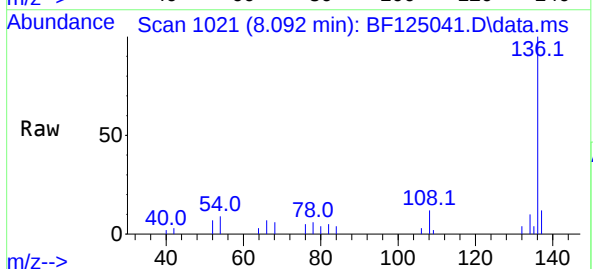




#23
Nitrobenzene-d5
Concen: 66.049 ng
RT: 7.375 min Scan# 899
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05




Instrument :
BNA_F
ClientSampleId :
20210540-COM-13


Tgt Ion: 82 Resp: 20806
Ion Ratio Lower Upper
82 100
128 38.4 40.6 60.8#
54 53.4 49.6 74.4

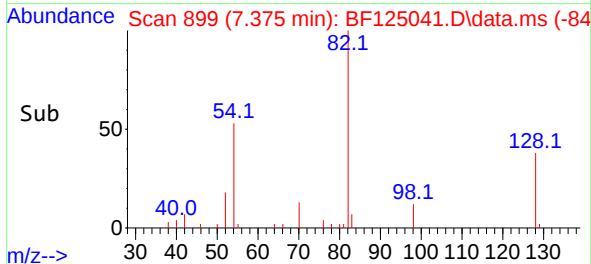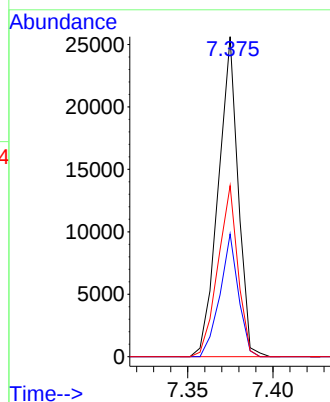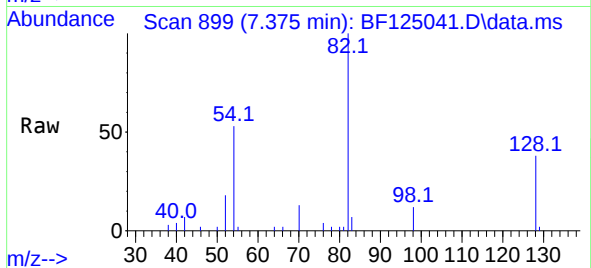

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.845 min Scan# 1319
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Tgt Ion:164 Resp: 9745
Ion Ratio Lower Upper
164 100
162 105.3 81.3 121.9
160 44.9 38.0 57.0


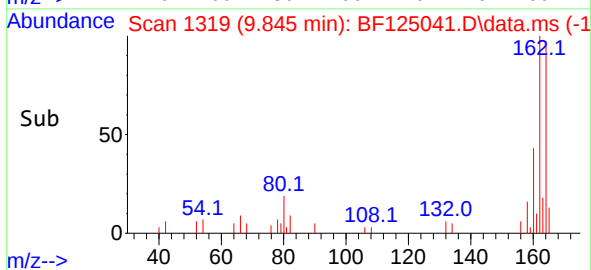
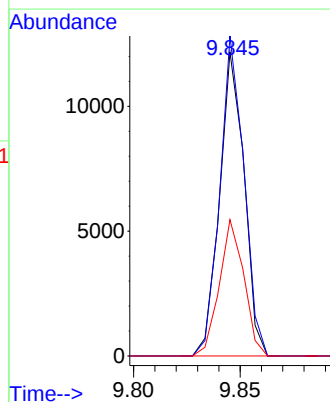
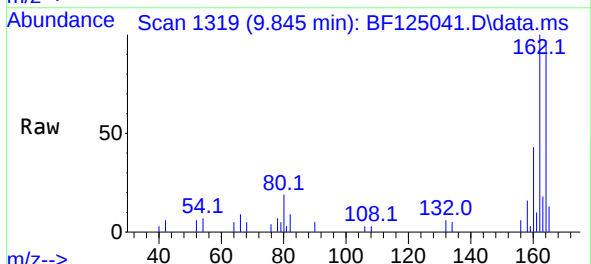




#42
2,4,6-Tribromophenol
Concen: 98.436 ng
RT: 10.639 min Scan# 1454
Delta R.T. 0.000 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05




Instrument :
BNA_F
ClientSampleId :
20210540-COM-13


Tgt Ion:330 Resp: 8570
Ion Ratio Lower Upper
330 100
332 96.0 76.2 114.4
141 42.6 44.6 66.8#

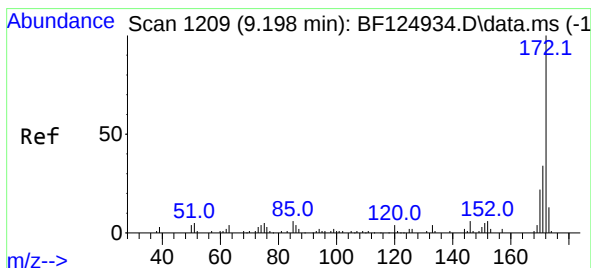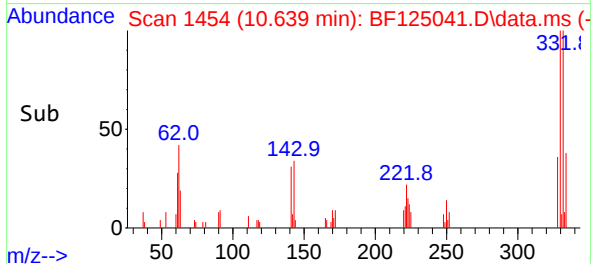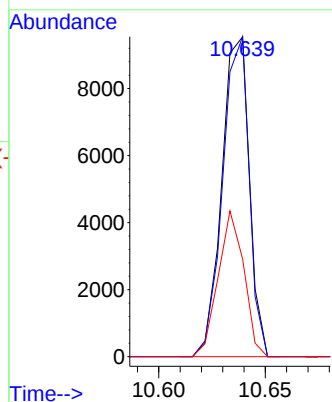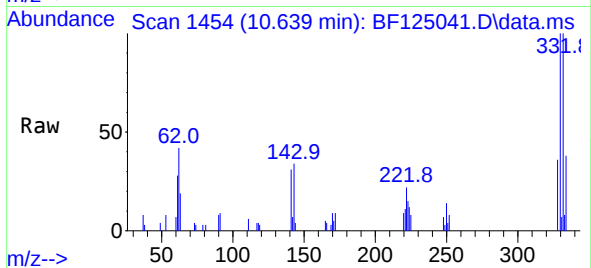

#45
2-Fluorobiphenyl
Concen: 48.959 ng
RT: 9.169 min Scan# 1204
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Tgt Ion:172 Resp: 32606
Ion Ratio Lower Upper
172 100
171 36.4 26.5 39.7
170 24.1 18.8 28.2


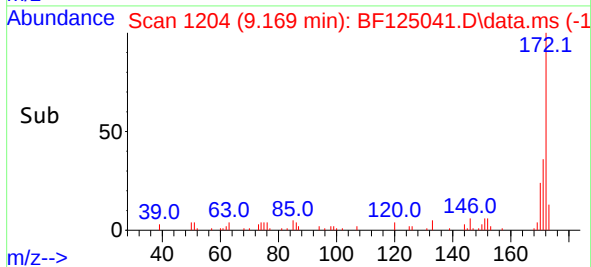
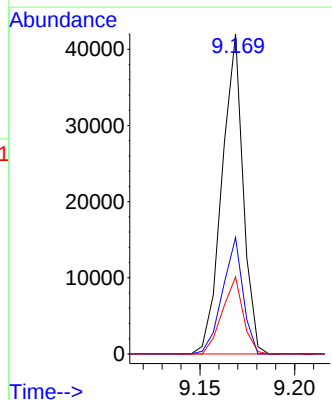
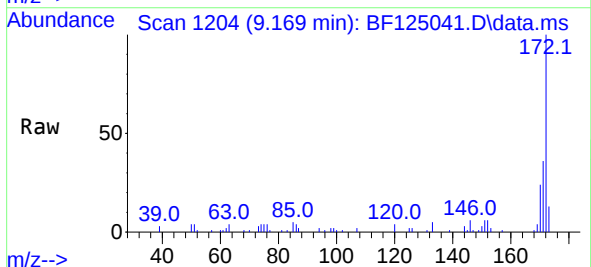




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.333 min Scan# 1572
Delta R.T. 0.000 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05




Instrument :
BNA_F
ClientSampleId :
20210540-COM-13


Tgt Ion:188 Resp: 18691
Ion Ratio Lower Upper
188 100
94 8.3 6.7 10.1
80 9.9 7.5 11.3

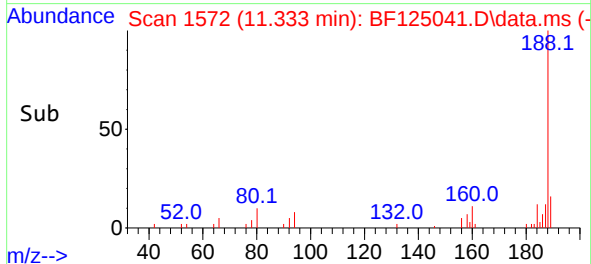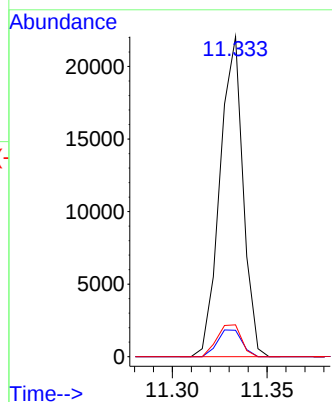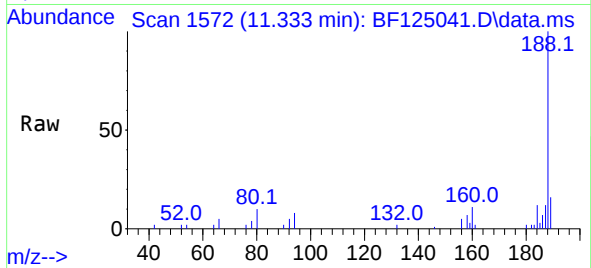

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.969 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05


Tgt Ion:240 Resp: 13250
Ion Ratio Lower Upper
240 100
120 11.0 10.8 16.2
236 26.5 21.6 32.4

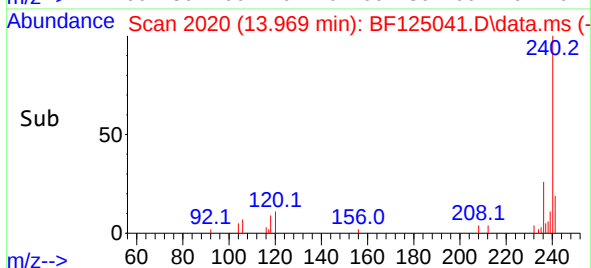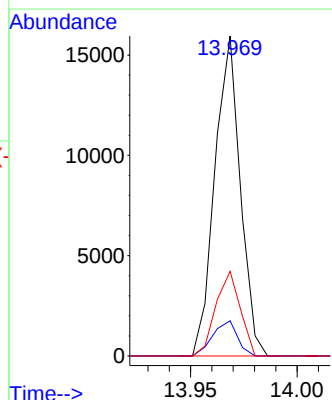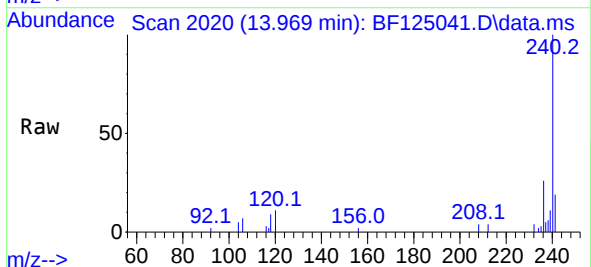






#79
Terphenyl-d14
Concen: 48.836 ng
RT: 12.916 min Scan# 1841
Delta R.T. 0.000 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13



Tgt Ion:244 Resp: 38361
Ion Ratio Lower Upper
244 100
212 6.6 5.9 8.9
122 8.6 9.0 13.4#

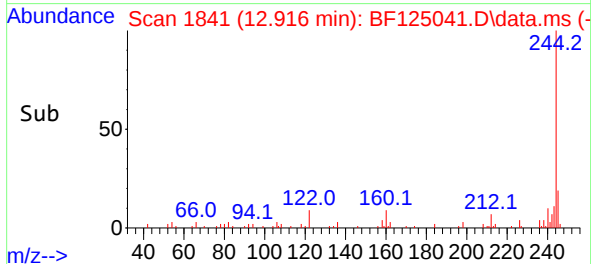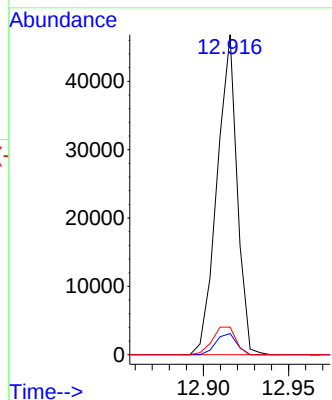

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.415 min Scan# 2266
Delta R.T. 0.000 min
Lab File: BF125041.D
Acq: 10 Aug 2021 21:05

Tgt Ion:264 Resp: 10683
Ion Ratio Lower Upper
264 100
260 24.1 19.6 29.4
265 21.3 17.2 25.8

