

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
 Data File : BF125027.D  
 Acq On : 10 Aug 2021 12:22  
 Operator : JU/CG  
 Sample : PB138288BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB138288BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125027.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.063       | 503           | 506         | 510          | rBB      | 2950           | 3707          | 1.25%           | 0.223%        |
| 2         | 5.445       | 567           | 571         | 574          | rBV      | 233089         | 215601        | 72.68%          | 12.955%       |
| 3         | 6.451       | 737           | 742         | 745          | rBV      | 219148         | 216322        | 72.93%          | 12.998%       |
| 4         | 6.810       | 800           | 803         | 806          | rBB      | 56163          | 42128         | 14.20%          | 2.531%        |
| 5         | 7.375       | 894           | 899         | 902          | rBV      | 141027         | 144571        | 48.74%          | 8.687%        |
| 6         | 8.092       | 1017          | 1021        | 1024         | rBB      | 66668          | 56866         | 19.17%          | 3.417%        |
| 7         | 9.169       | 1199          | 1204        | 1207         | rBV      | 293015         | 278460        | 93.87%          | 16.732%       |
| 8         | 9.845       | 1315          | 1319        | 1322         | rBB      | 83657          | 69240         | 23.34%          | 4.160%        |
| 9         | 10.639      | 1449          | 1454        | 1457         | rBV      | 198671         | 166348        | 56.08%          | 9.995%        |
| 10        | 11.333      | 1568          | 1572        | 1575         | rBV      | 87331          | 69733         | 23.51%          | 4.190%        |
| 11        | 12.921      | 1837          | 1842        | 1844         | rBV      | 313725         | 296634        | 100.00%         | 17.824%       |
| 12        | 13.833      | 1993          | 1997        | 1999         | rVB      | 3819           | 3315          | 1.12%           | 0.199%        |
| 13        | 13.968      | 2016          | 2020        | 2023         | rBB      | 64168          | 53542         | 18.05%          | 3.217%        |
| 14        | 15.415      | 2262          | 2266        | 2271         | rBB      | 36680          | 44764         | 15.09%          | 2.690%        |
| 15        | 15.845      | 2336          | 2339        | 2342         | rBB      | 2646           | 3035          | 1.02%           | 0.182%        |




Sum of corrected areas: 1664266

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
Data File : BF125027.D  
Acq On : 10 Aug 2021 12:22  
Operator : JU/CG  
Sample : PB138288BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB138288BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

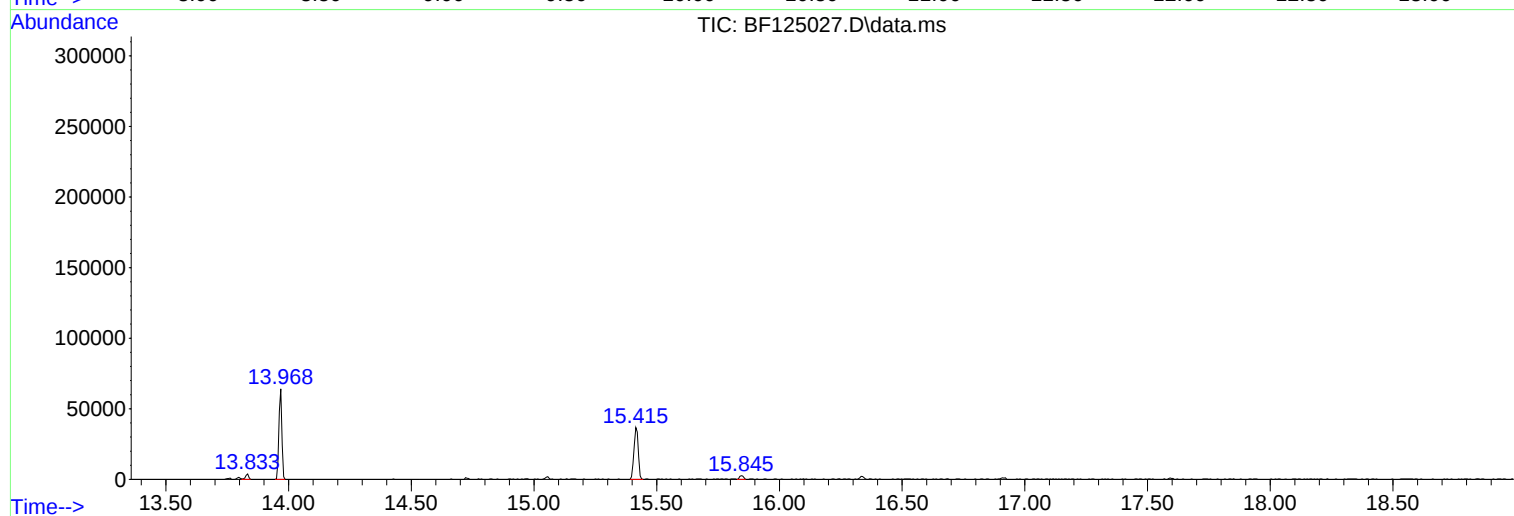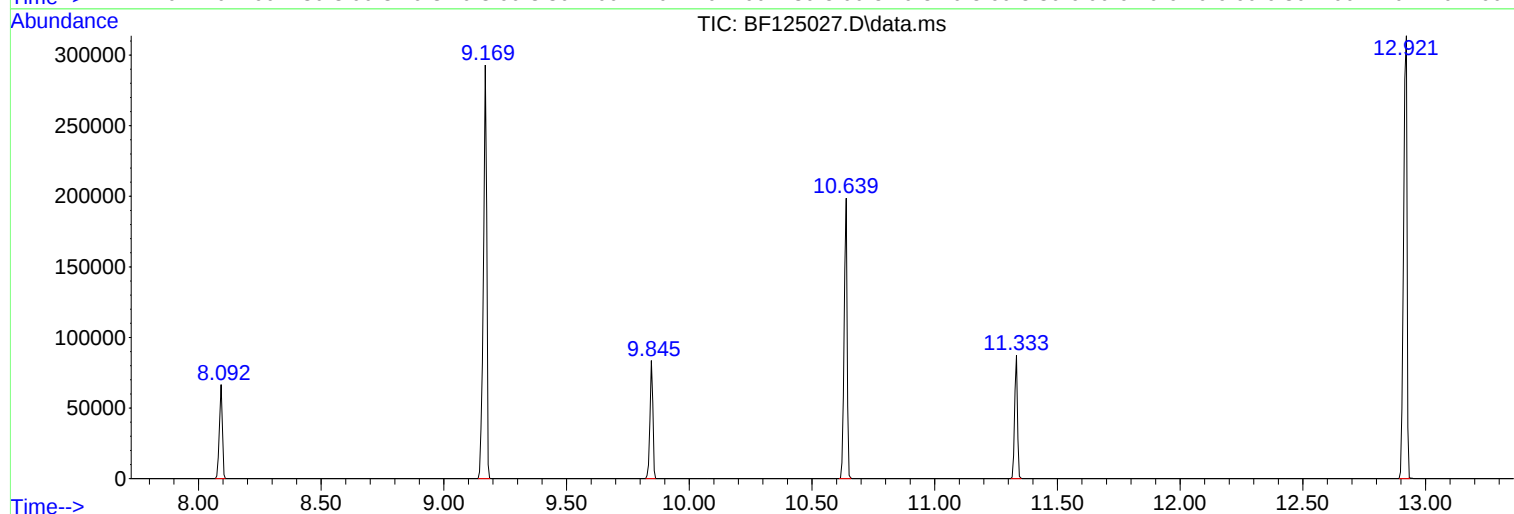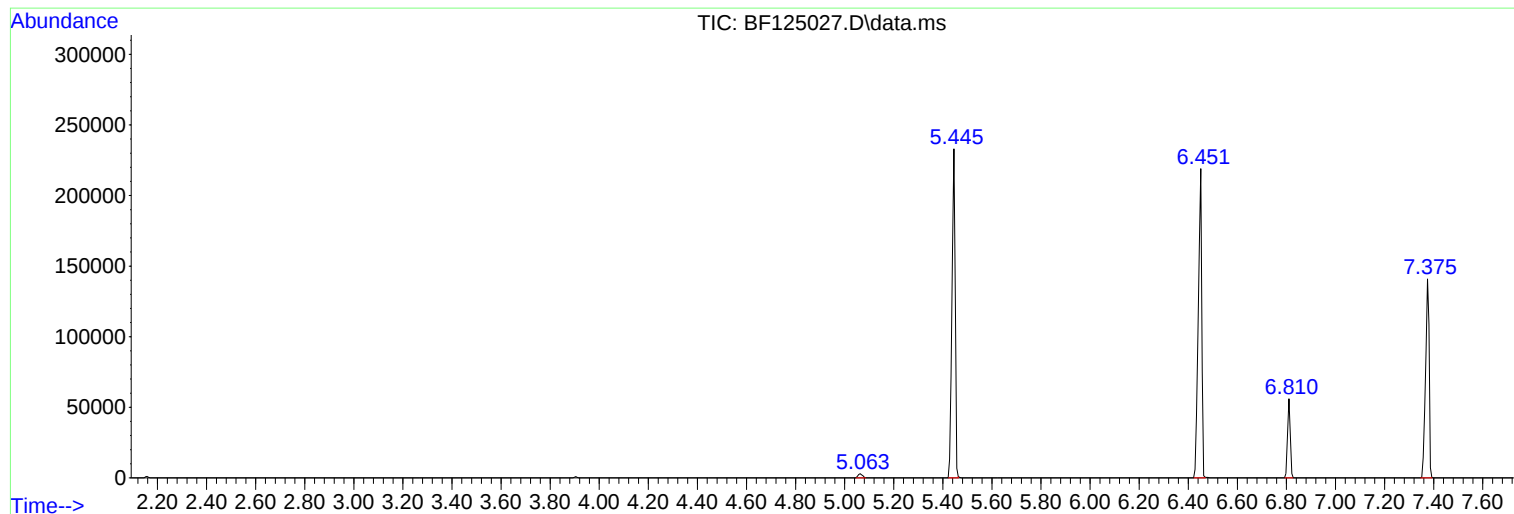

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
Data File : BF125027.D  
Acq On : 10 Aug 2021 12:22  
Operator : JU/CG  
Sample : PB138288BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB138288BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
Data File : BF125027.D  
Acq On : 10 Aug 2021 12:22  
Operator : JU/CG  
Sample : PB138288BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB138288BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|