

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125041.D
 Acq On : 10 Aug 2021 21:05
 Operator : JU/CG
 Sample : M3318-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20210540-COM-13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	497	499	503	rBB	3331	3357	3.50%	0.491%
2	5.434	565	569	572	rBV	89800	82259	85.70%	12.031%
3	6.445	737	741	744	rBV	96878	87171	90.82%	12.749%
4	6.810	800	803	806	rBB	31194	21985	22.90%	3.215%
5	7.375	895	899	902	rBV	71279	56834	59.21%	8.312%
6	7.992	1002	1004	1008	rBB	10666	8492	8.85%	1.242%
7	8.092	1018	1021	1024	rBB	44429	31932	33.27%	4.670%
8	9.169	1200	1204	1207	rBB	120990	90744	94.54%	13.272%
9	9.845	1316	1319	1322	rBB	52604	39117	40.75%	5.721%
10	10.633	1450	1453	1456	rBB	88437	70391	73.33%	10.295%
11	11.333	1568	1572	1575	rBB	50378	41915	43.67%	6.130%
12	12.916	1837	1841	1844	rBV	121814	95987	100.00%	14.038%
13	13.810	1990	1993	1995	rBB	2514	2580	2.69%	0.377%
14	13.969	2017	2020	2023	rBB	36086	29005	30.22%	4.242%
15	15.421	2262	2267	2270	rBB	19373	21977	22.90%	3.214%




Sum of corrected areas: 683746

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125041.D
Acq On : 10 Aug 2021 21:05
Operator : JU/CG
Sample : M3318-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

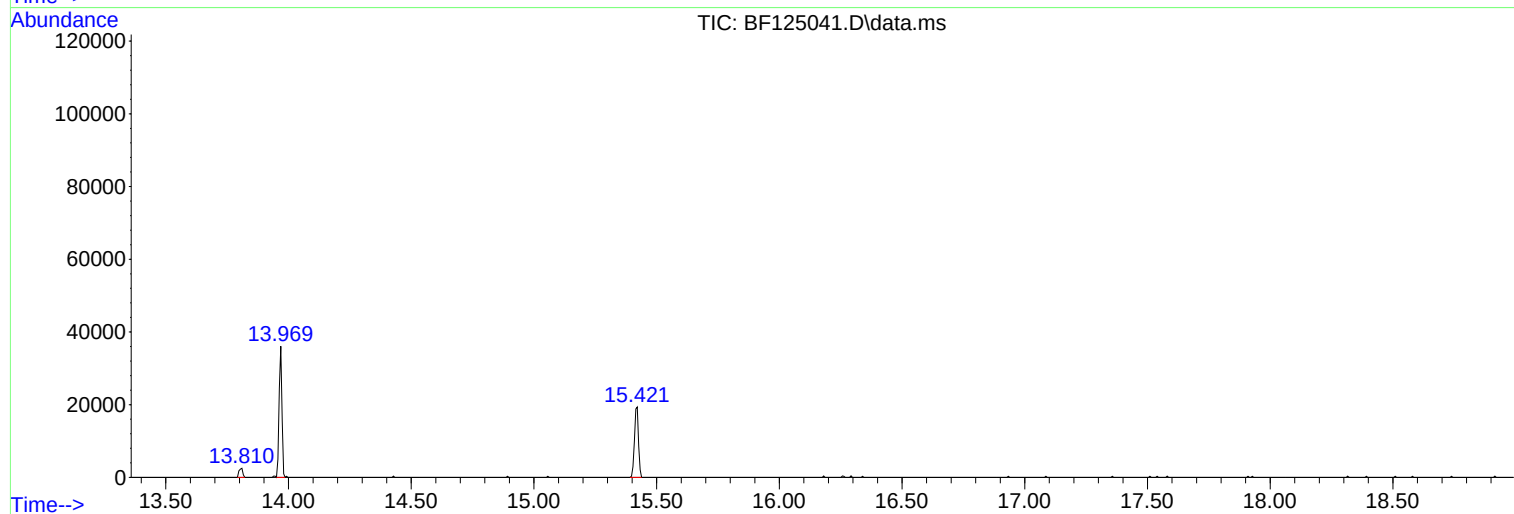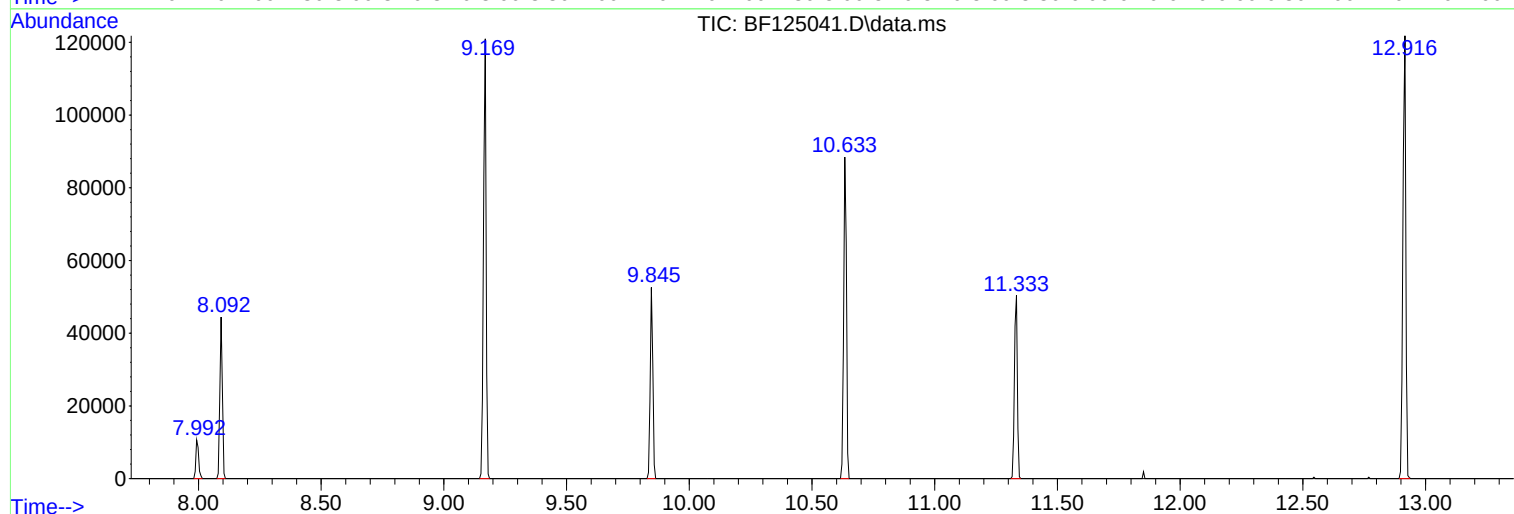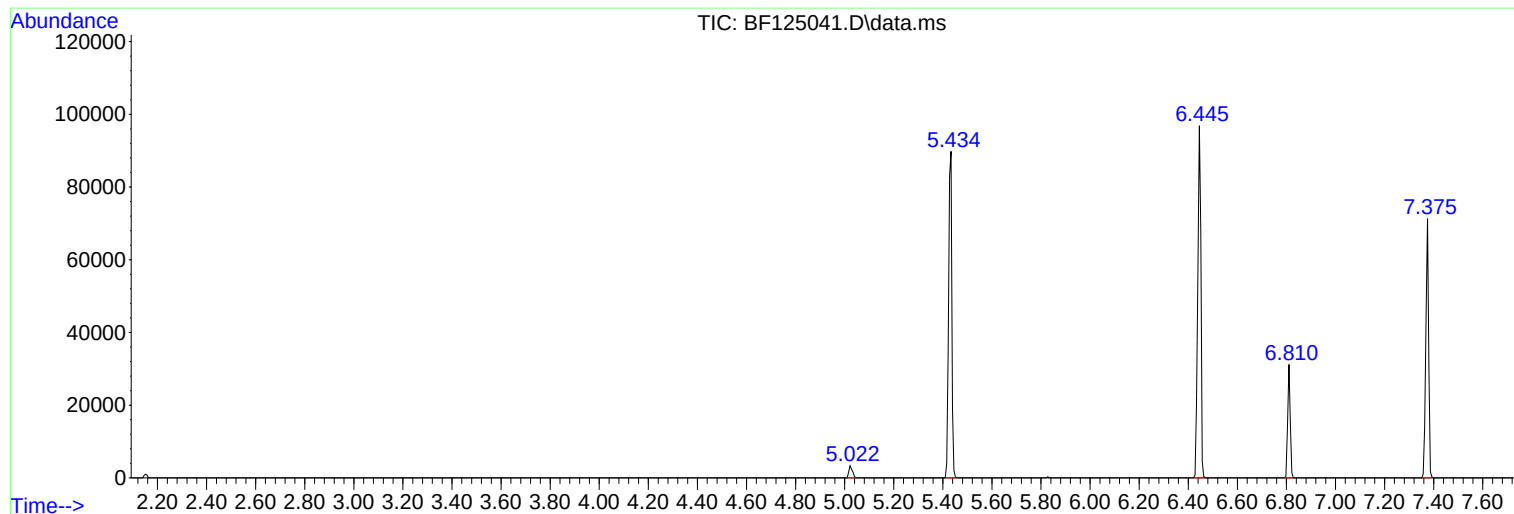

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125041.D
Acq On : 10 Aug 2021 21:05
Operator : JU/CG
Sample : M3318-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13








Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.022 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.022	3.05 ng	3357	1,4-Dichlorobenzene-d4	6.810

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diacetamide	101	C4H7NO2	000625-77-4	4
2			Guanidine	59	CH5N3	000113-00-8	4
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	4
4			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	4
5			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	4

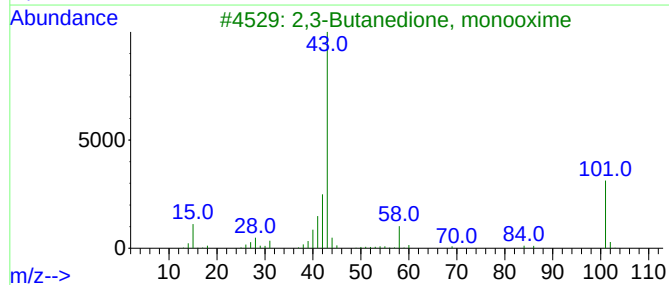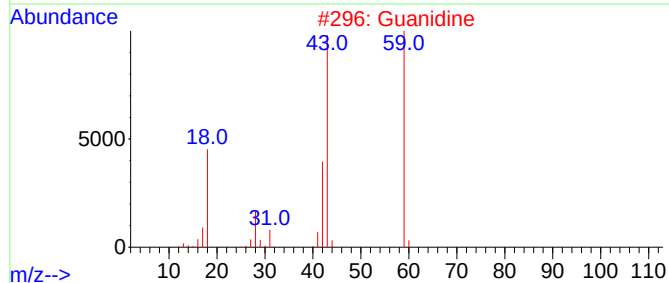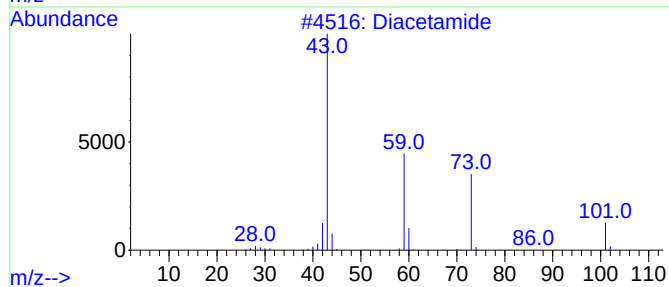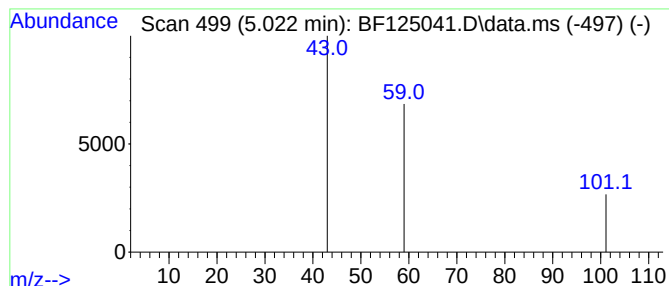

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125041.D
Acq On : 10 Aug 2021 21:05
Operator : JU/CG
Sample : M3318-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.992 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.992	5.32 ng	8492	Naphthalene-d8	8.092

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3,3-Dimethylbutane-2-ol	102	C6H14O	000464-07-3	9
2			Aziridine, 1-(methoxymethyl)-	87	C4H9NO	001497-83-2	7
3			Methane, nitroso-	45	CH3NO	000865-40-7	4
4			Morpholine	87	C4H9NO	000110-91-8	4
5			Ethanamine, 2-methoxy-	75	C3H9NO	000109-85-3	4

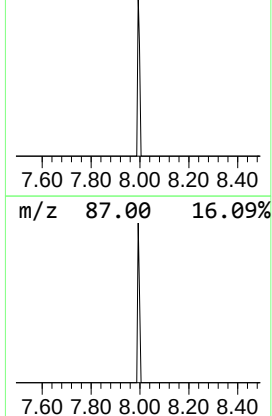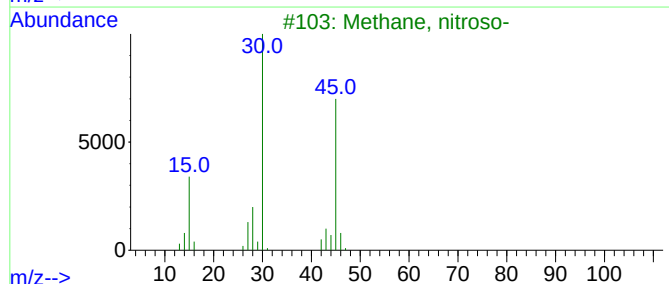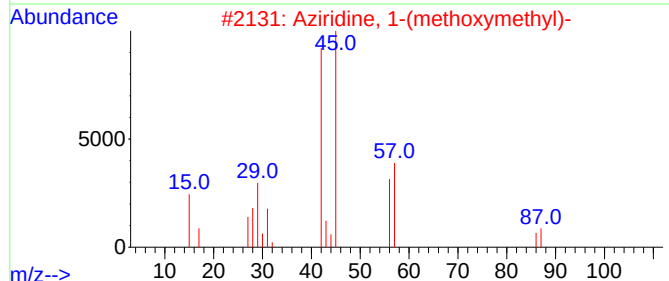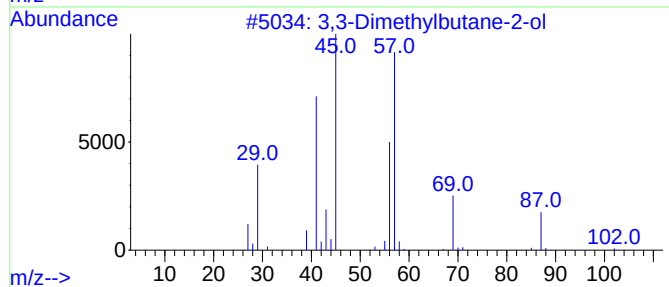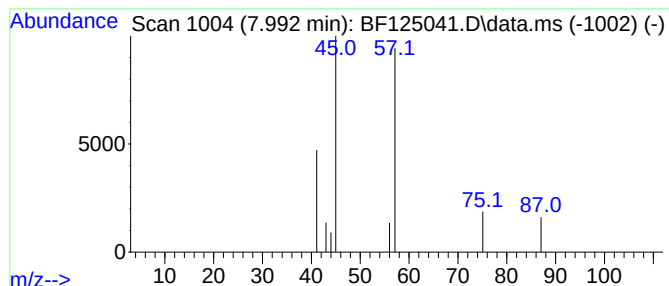

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
Data File : BF125041.D
Acq On : 10 Aug 2021 21:05
Operator : JU/CG
Sample : M3318-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20210540-COM-13

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.022	5.022	3.0	ng	3357	1	6.810	21985	20.0
unknown7.992	7.992	5.3	ng	8492	2	8.092	31932	20.0