
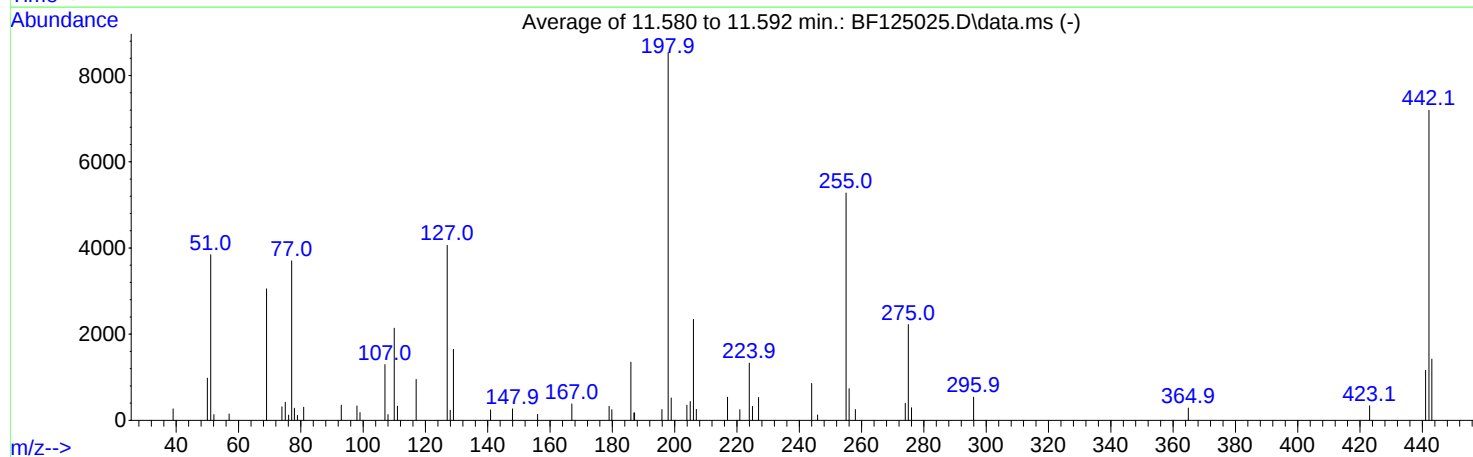


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
 Data File : BF125025.D  
 Acq On : 10 Aug 2021 10:10  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Aug 10 11:32:36 2021

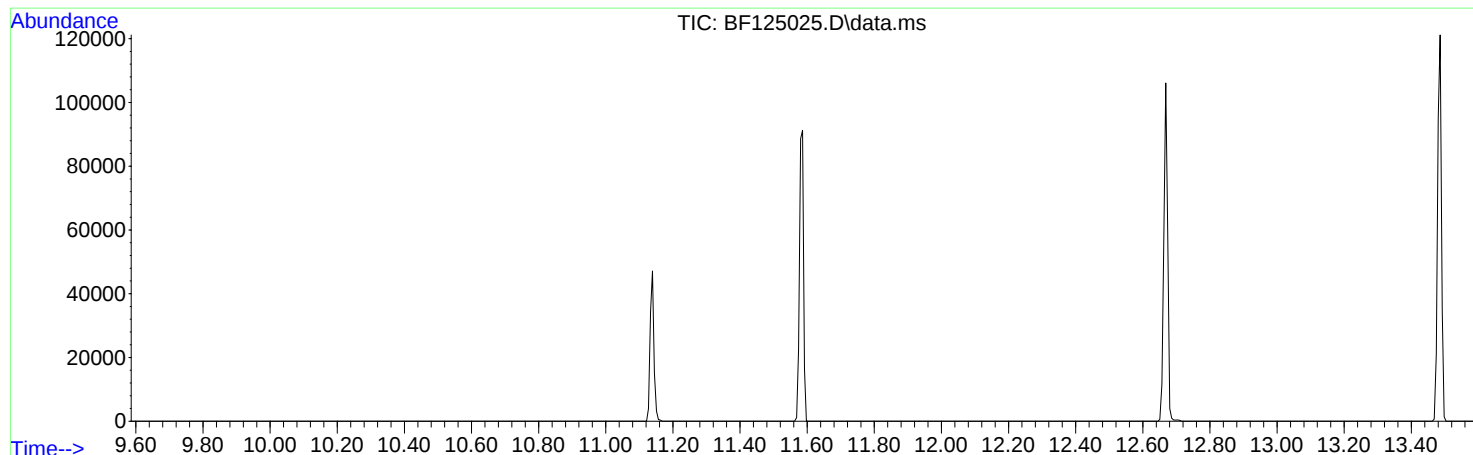




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 45.0         | 3843       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 35.8         | 3053       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 47.6         | 4063       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 8535       | PASS                |
| 199            | 198             | 5               | 9               | 6.1          | 520        | PASS                |
| 275            | 198             | 10              | 60              | 26.1         | 2224       | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 285        | PASS                |
| 441            | 198             | 0.01            | 100             | 13.6         | 1163       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 7196       | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 1422       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
 Data File : BF125025.D  
 Acq On : 10 Aug 2021 10:10  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 10 11:29:27 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 09 11:03:44 2021  
 Response via : Initial Calibration

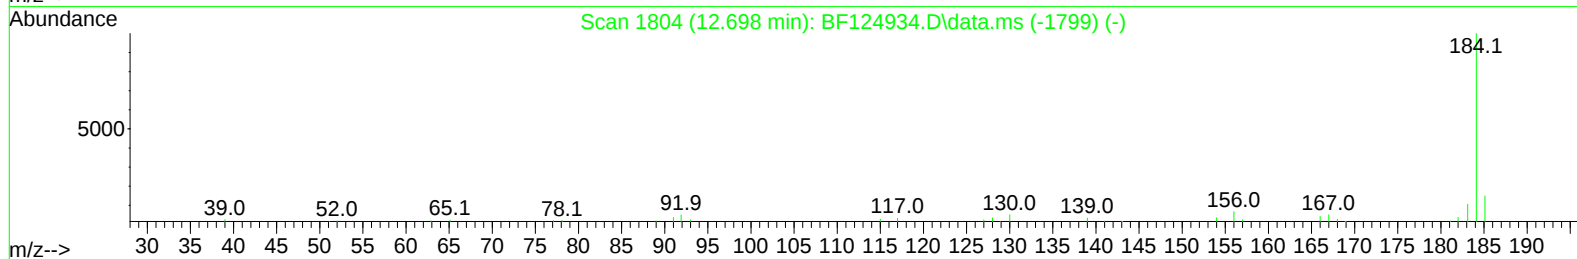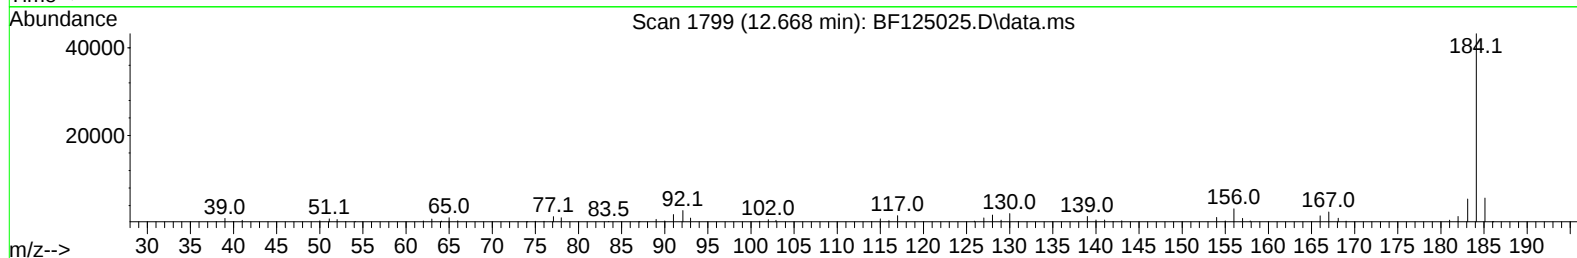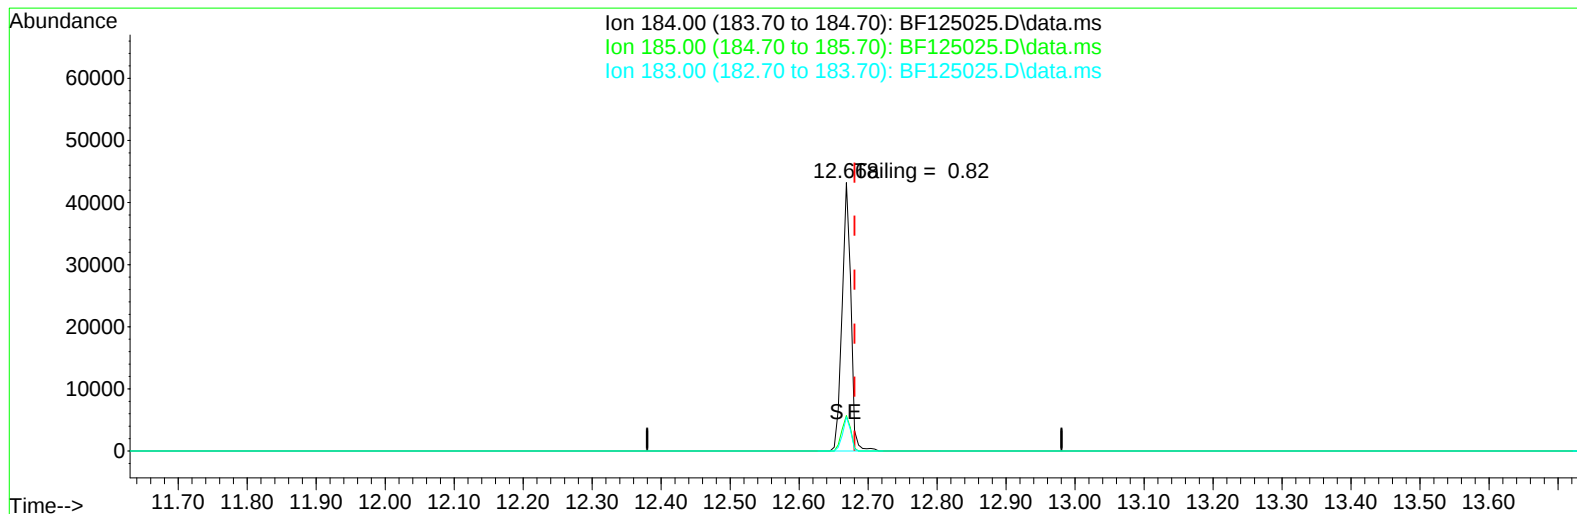

TIC: BF125025.D\data.ms

**(77) Benzidine**

12.668min (-0.012) 0.00 ng




response 38069

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.20  |
| 183.00 | 10.10  | 12.74# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081021\  
 Data File : BF125025.D  
 Acq On : 10 Aug 2021 10:10  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 10 11:29:27 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 09 11:03:44 2021  
 Response via : Initial Calibration

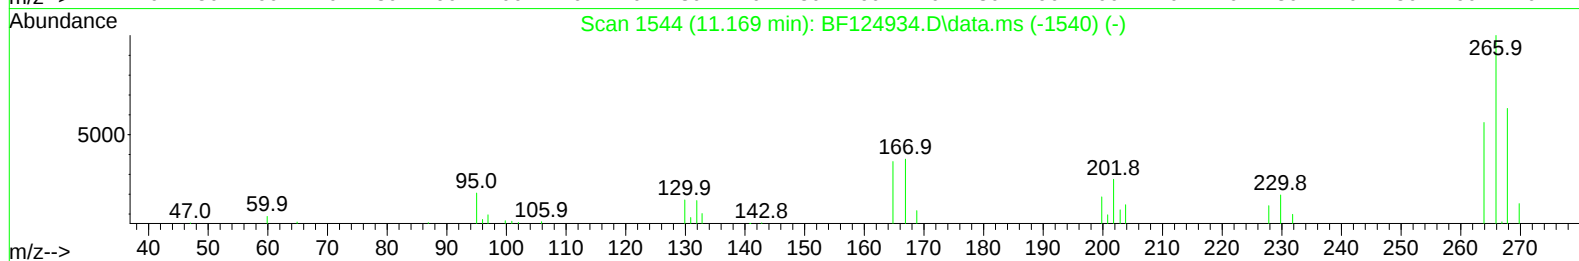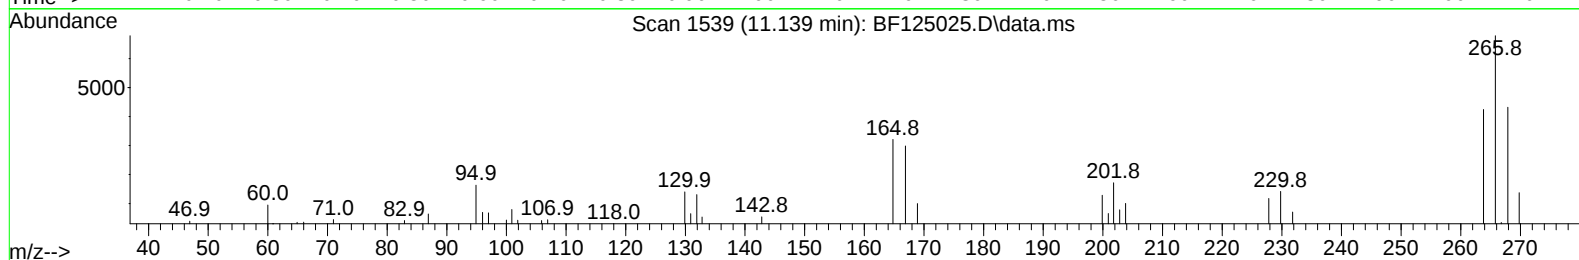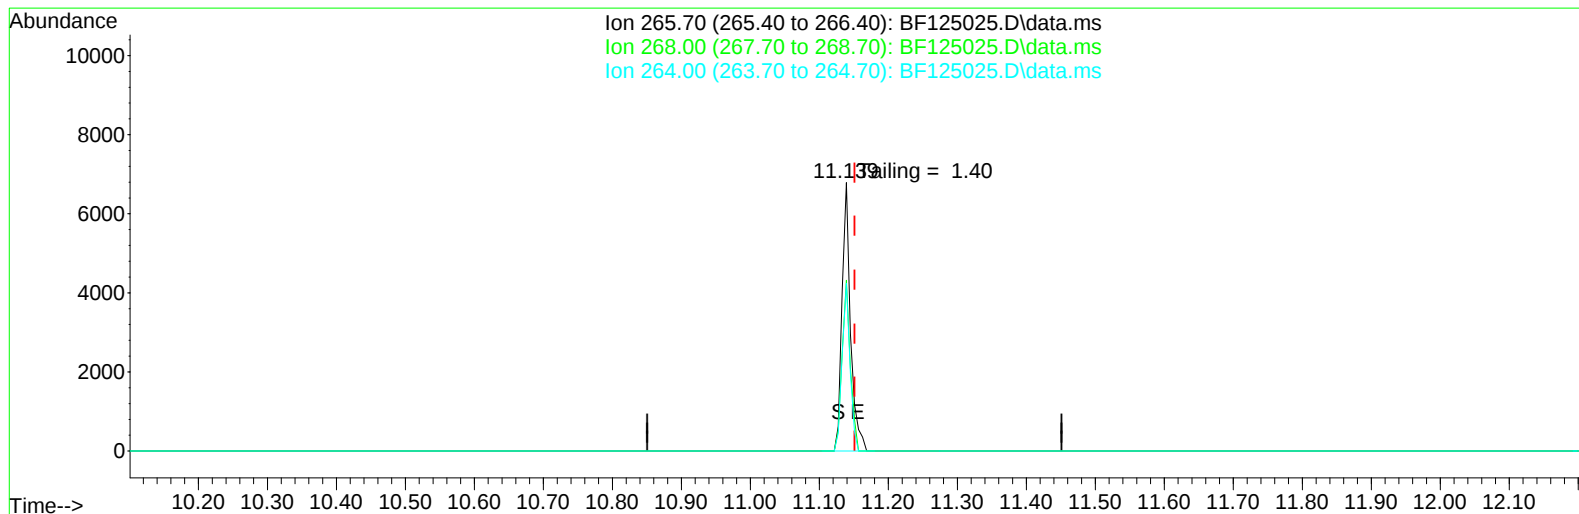

TIC: BF125025.D\data.ms

**(70) Pentachlorophenol (C)**

11.139min (-0.012) 0.00 ng

response 5831

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 63.63  |
| 264.00 | 69.90  | 62.51  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/10/2021     | BNA_F            | <u>BF125025.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 20720            | 13.48              |
| DDD           | 0                | 13.23              |
| DDE           | 0                | 12.745             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 0             | 20720            | 0.00               |
|               |                  |                    |

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP