
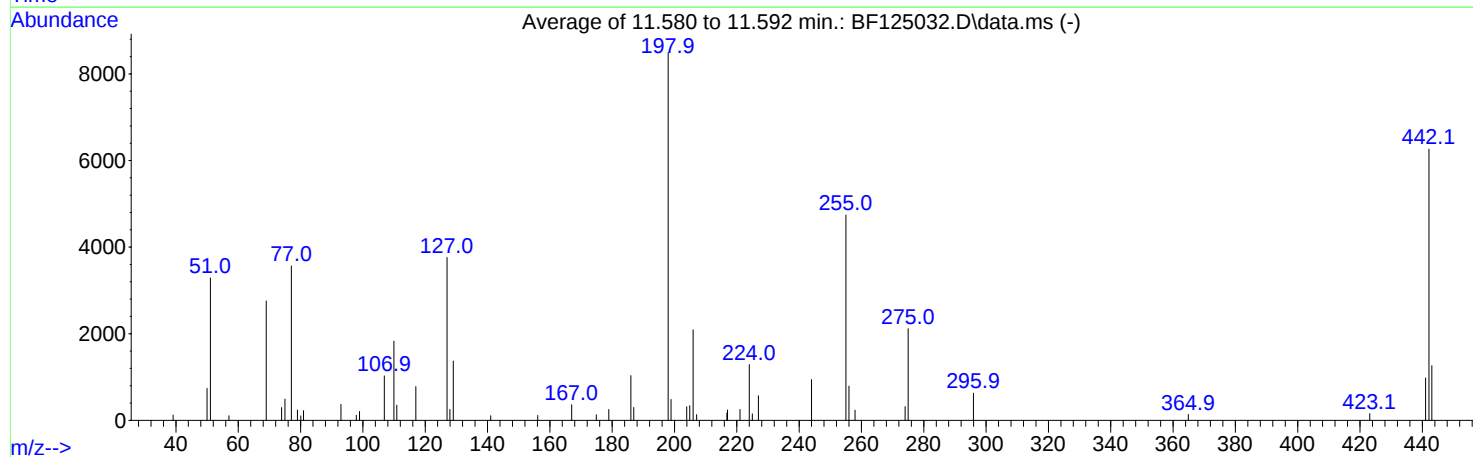


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125032.D
 Acq On : 10 Aug 2021 15:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 10 11:32:36 2021

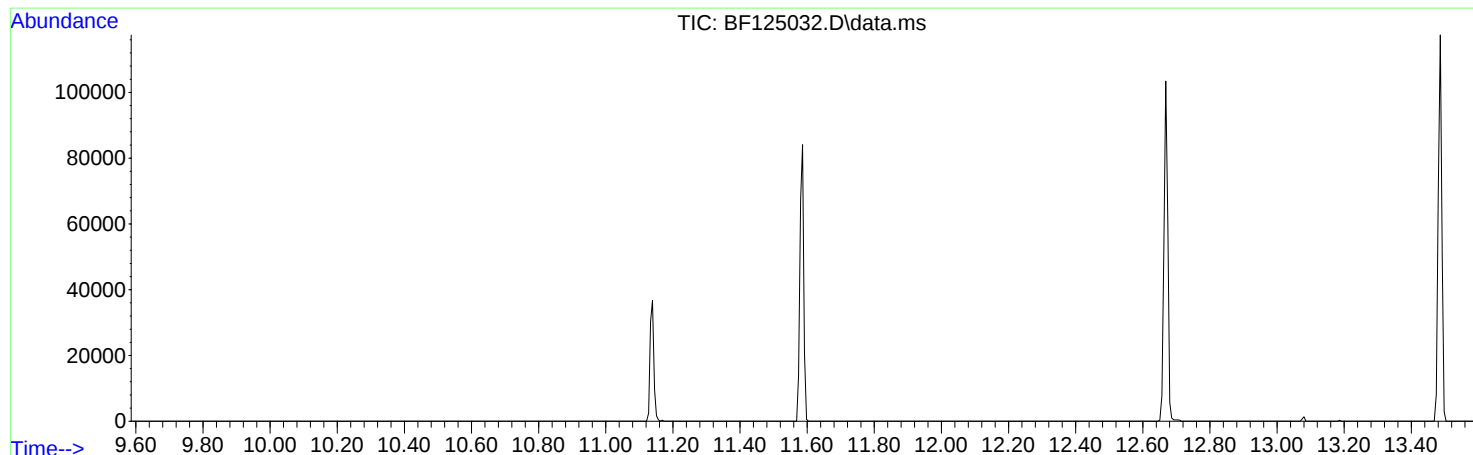




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	3290	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	2755	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	3761	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8494	PASS
199	198	5	9	5.7	485	PASS
275	198	10	60	24.9	2117	PASS
365	198	1	100	1.6	135	PASS
441	198	0.01	100	11.5	981	PASS
442	442	50	100	100.0	6263	PASS
443	442	15	24	20.2	1265	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125032.D
 Acq On : 10 Aug 2021 15:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 10 18:10:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 10 11:32:36 2021
 Response via : Initial Calibration

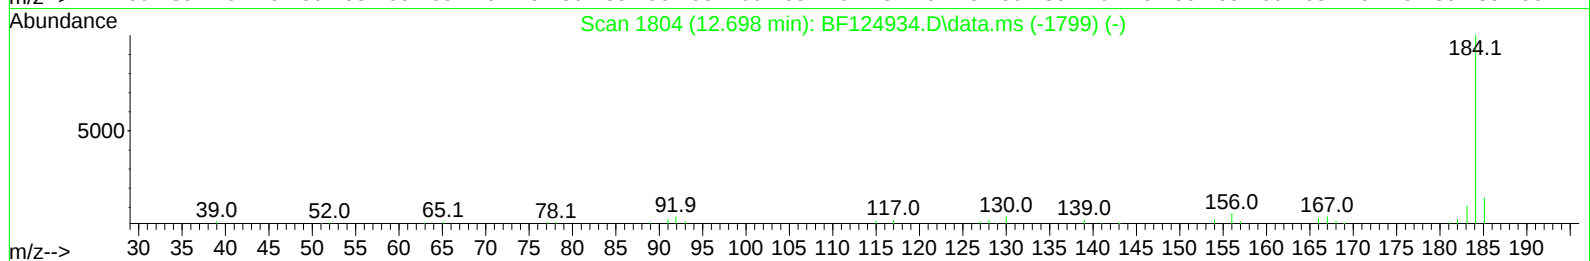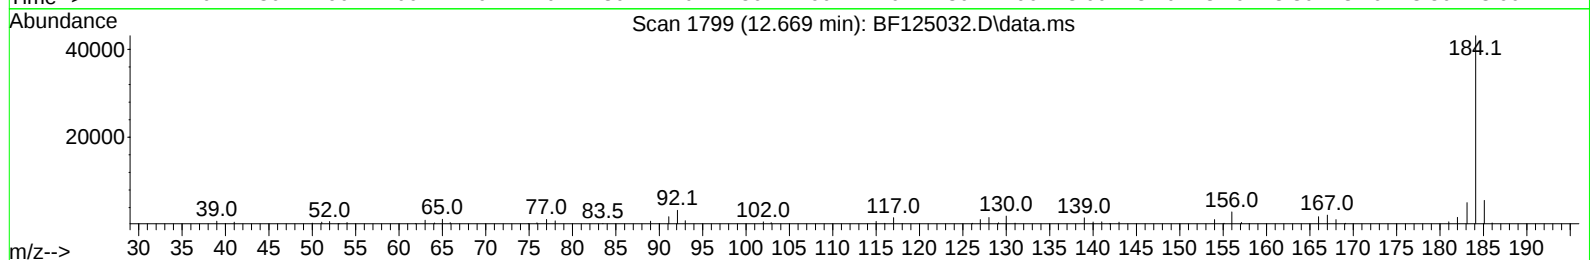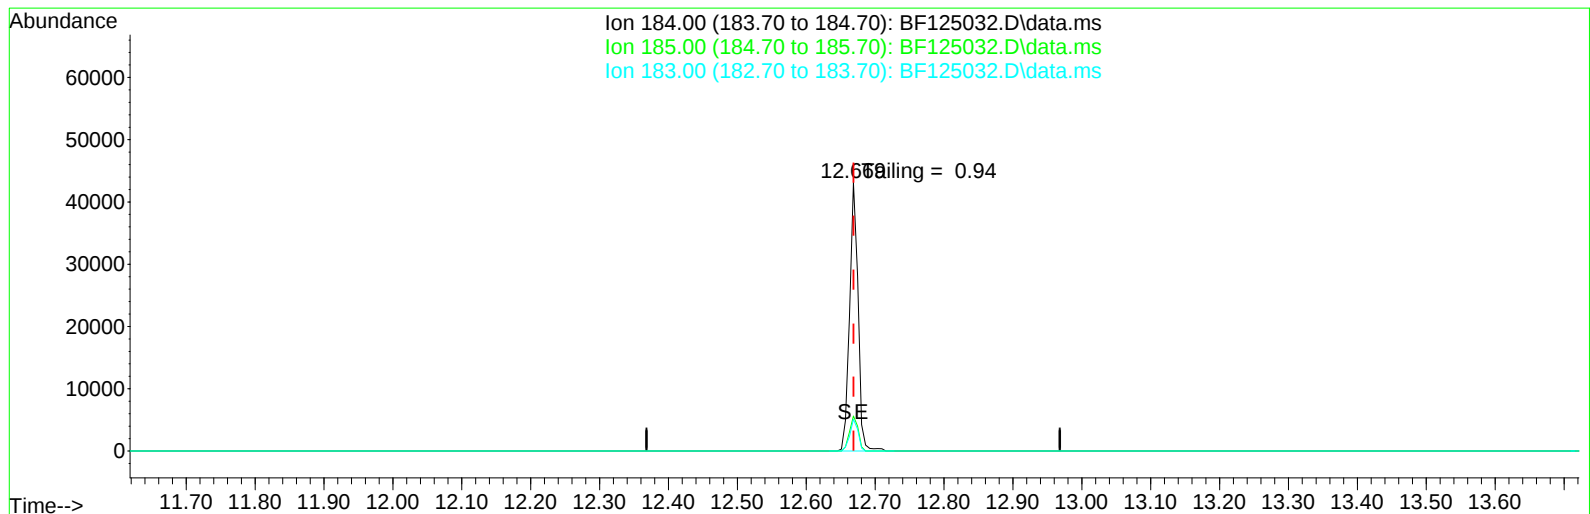

TIC: BF125032.D\data.ms

(77) Benzidine

12.669min (+ 0.000) 0.00 ng




response 36915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.08
183.00	10.10	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081021\
 Data File : BF125032.D
 Acq On : 10 Aug 2021 15:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 10 18:10:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 10 11:32:36 2021
 Response via : Initial Calibration

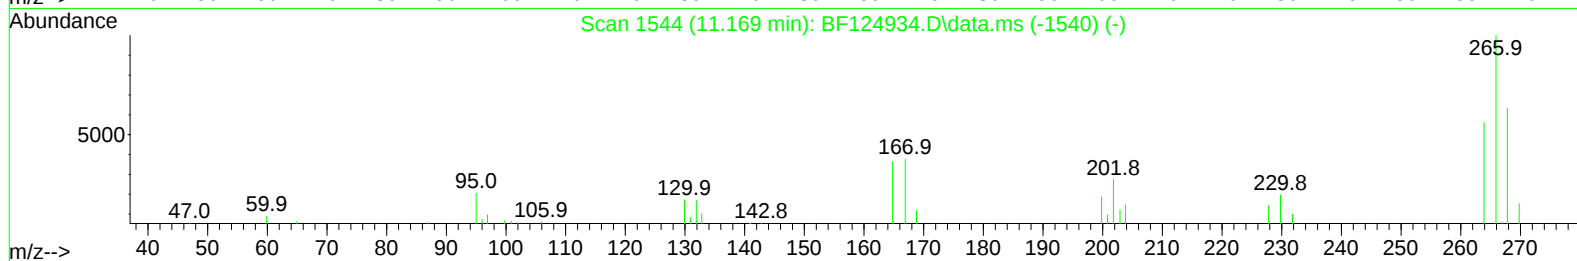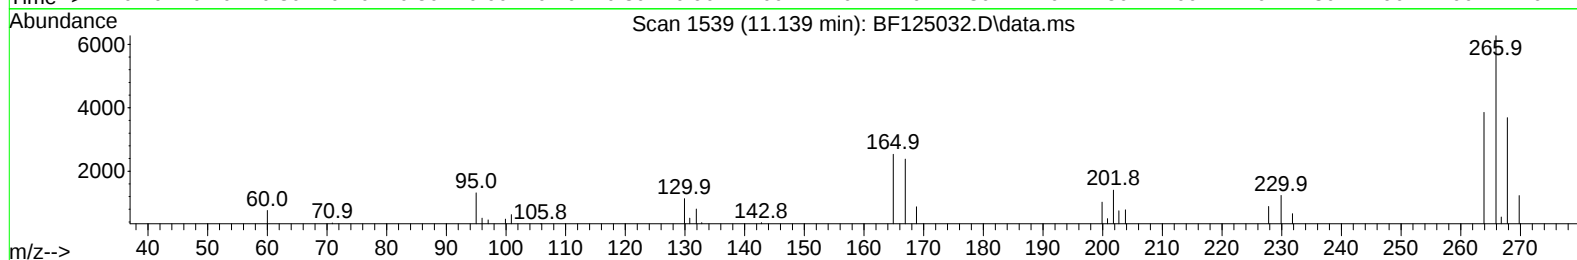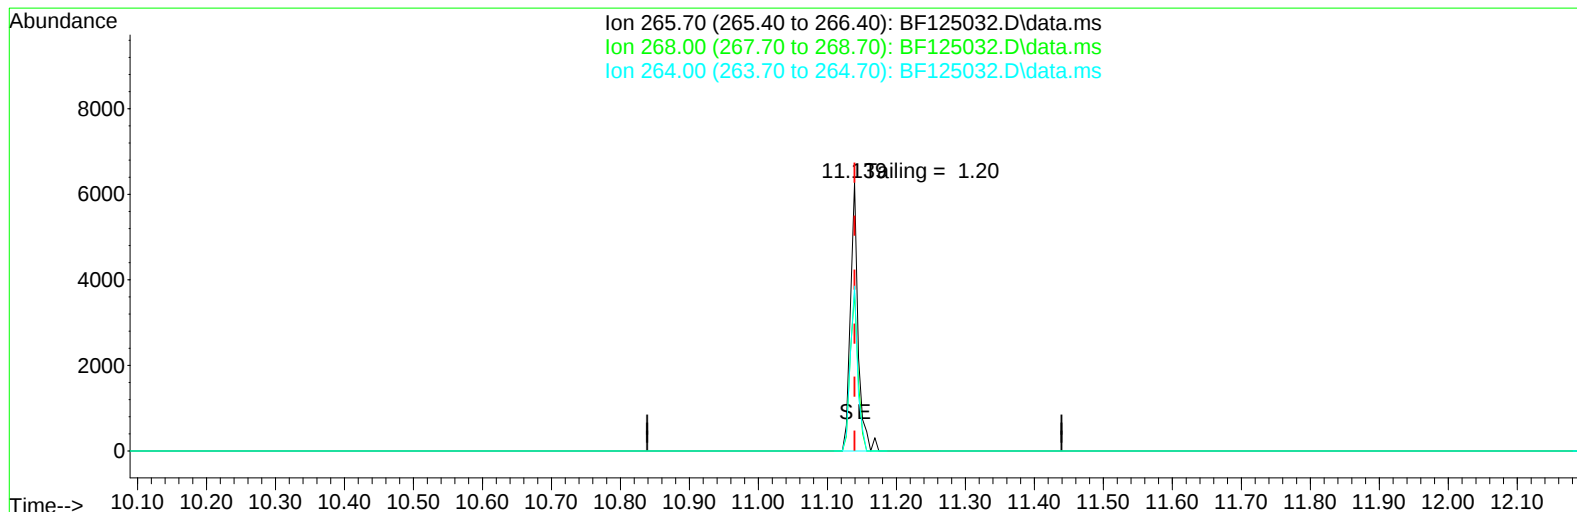

TIC: BF125032.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 0.00 ng

response 4942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	58.77
264.00	69.90	61.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2021	BNA_F	<u>BF125032.D</u>
Compound Name	Response	Retention Time
DDT	19297	13.48
DDD	106	13.18
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
106	19403	0.55

Instrument :
BNA_F
ClientSampleId :
DFTPP