


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081115\
 Data File : BF080960.D
 Acq On : 11 Aug 2015 9:14
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 08 01:33:05 2015

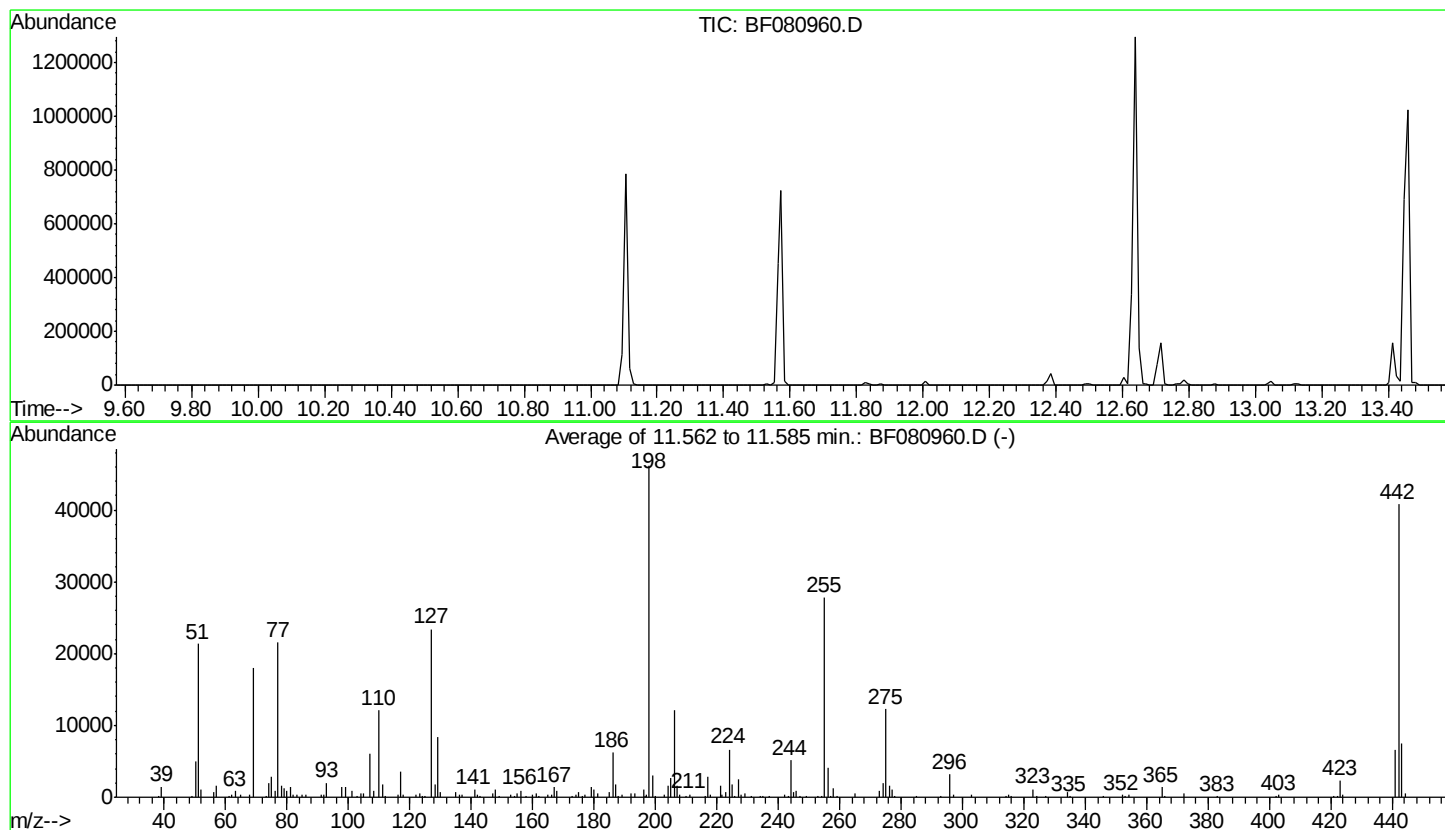

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	21328	PASS
68	69	0.00	2	1.6	282	PASS
69	198	0.00	100	38.9	17946	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	23432	PASS
197	198	0.00	2	0.7	311	PASS
198	198	100	100	100.0	46163	PASS
199	198	5	9	6.6	3060	PASS
275	198	10	60	26.5	12234	PASS
365	198	1	100	3.0	1401	PASS
441	442	0.01	24	16.0	6519	PASS
442	198	50	100	88.2	40726	PASS
443	442	15	24	18.4	7479	PASS