
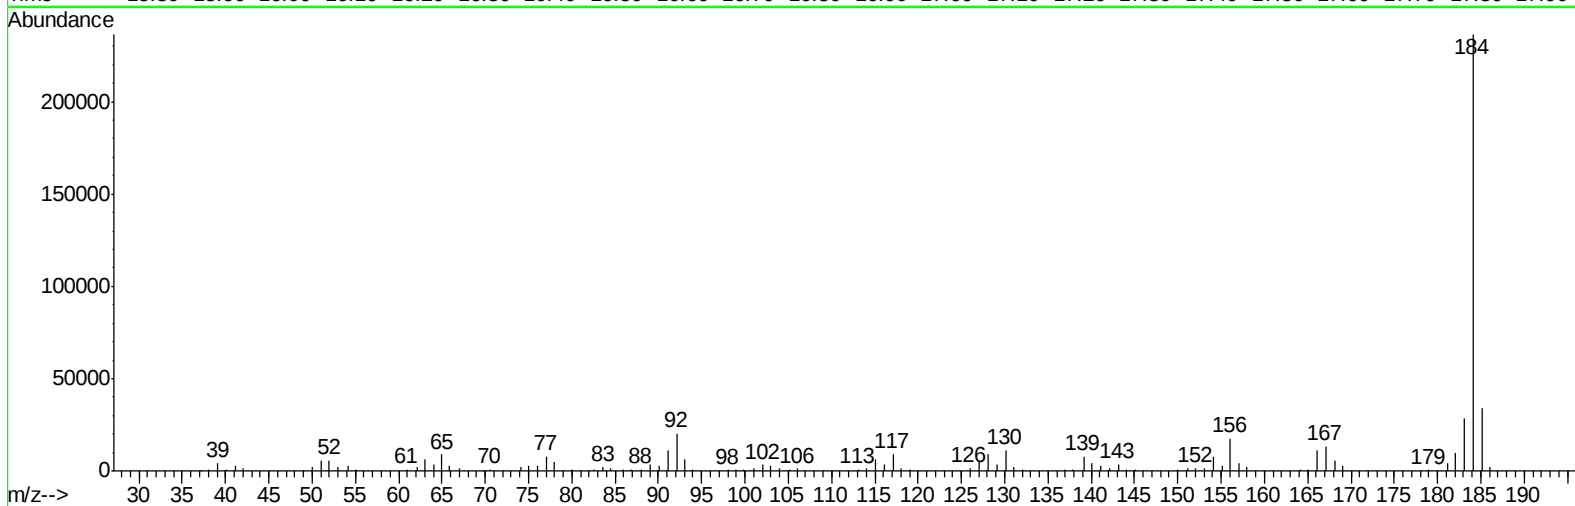


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081117\
Data File : BF097589.D
Acq On : 11 Aug 2017 11:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 02:33:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

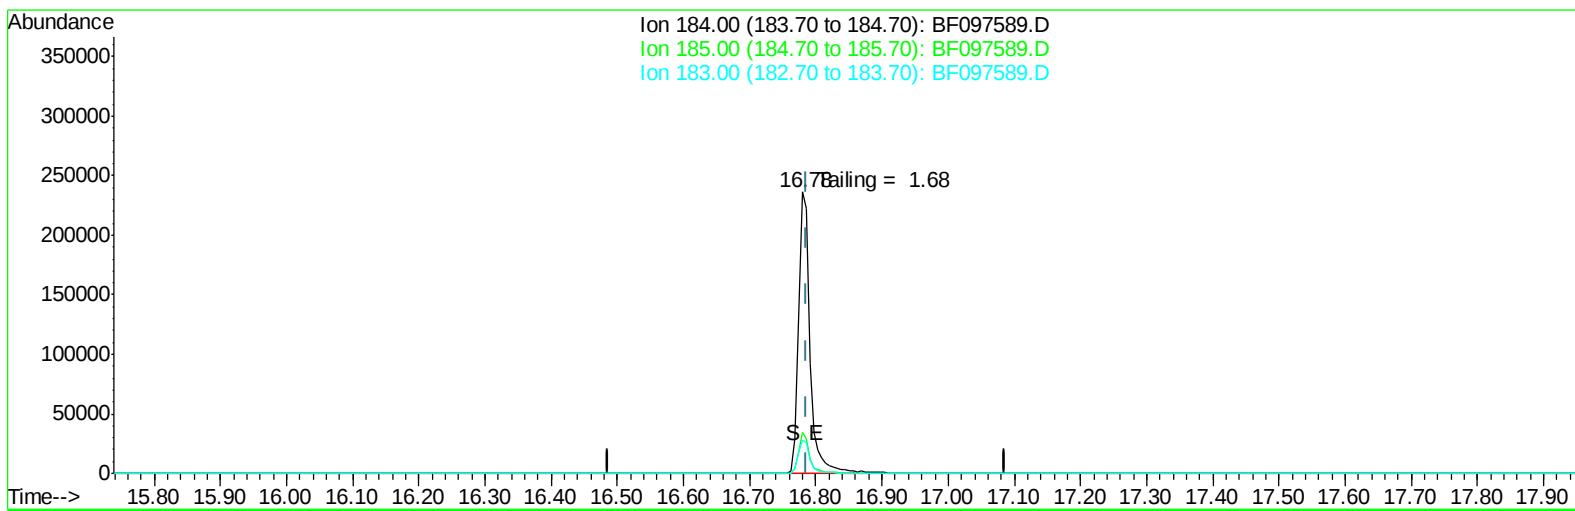

TIC: BF097589.D

(76) Benzidine



16.780min (-0.006) 0.00ng

response 291979

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.48#
183.00	12.20	11.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081117\
Data File : BF097589.D
Acq On : 11 Aug 2017 11:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 02:33:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

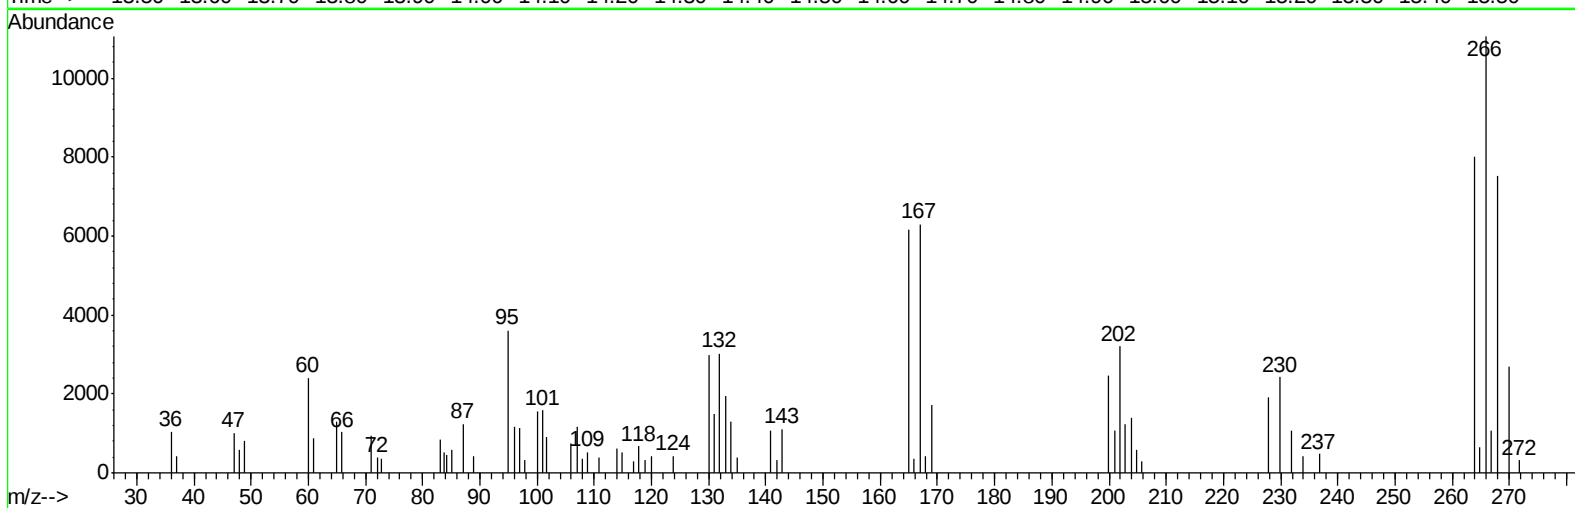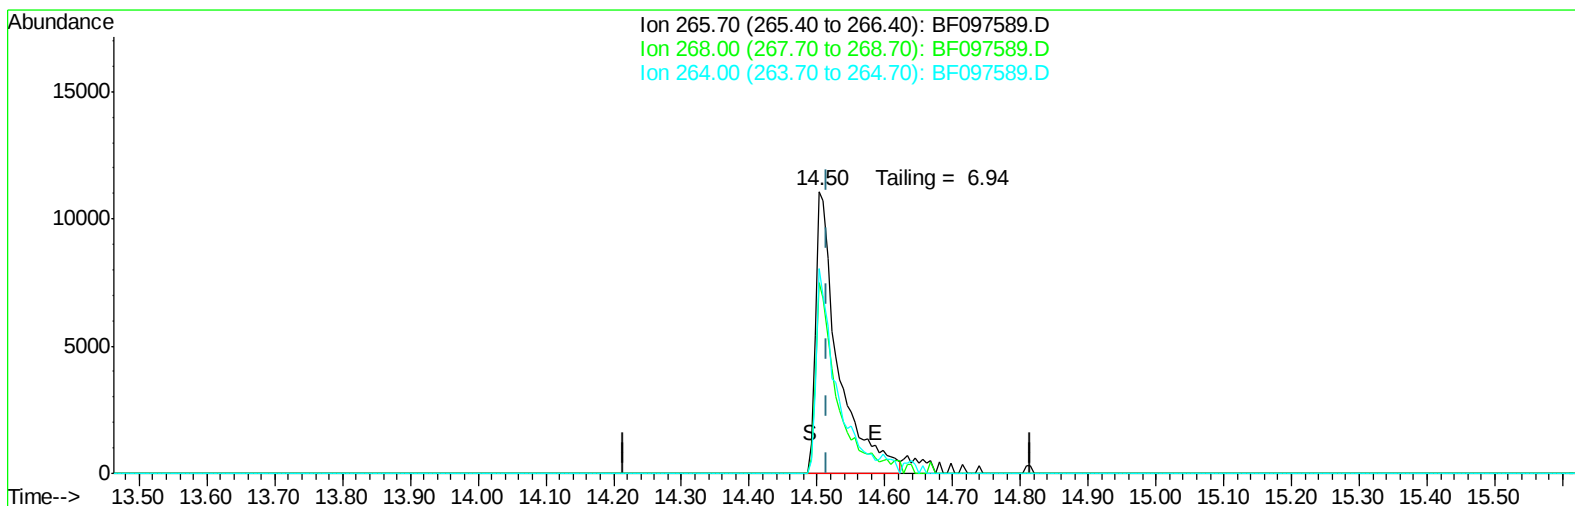

TIC: BF097589.D

(69) Pentachlorophenol (C)

14.504min (-0.011) 0.00ng

response 25198

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.93
264.00	64.60	72.57
0.00	0.00	0.00