


Data Path : Z:\HPCHEM1\BNA F\Data\BF081117\
 Data File : BF097598.D
 Acq On : 11 Aug 2017 16:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 11 15:55:57 2017

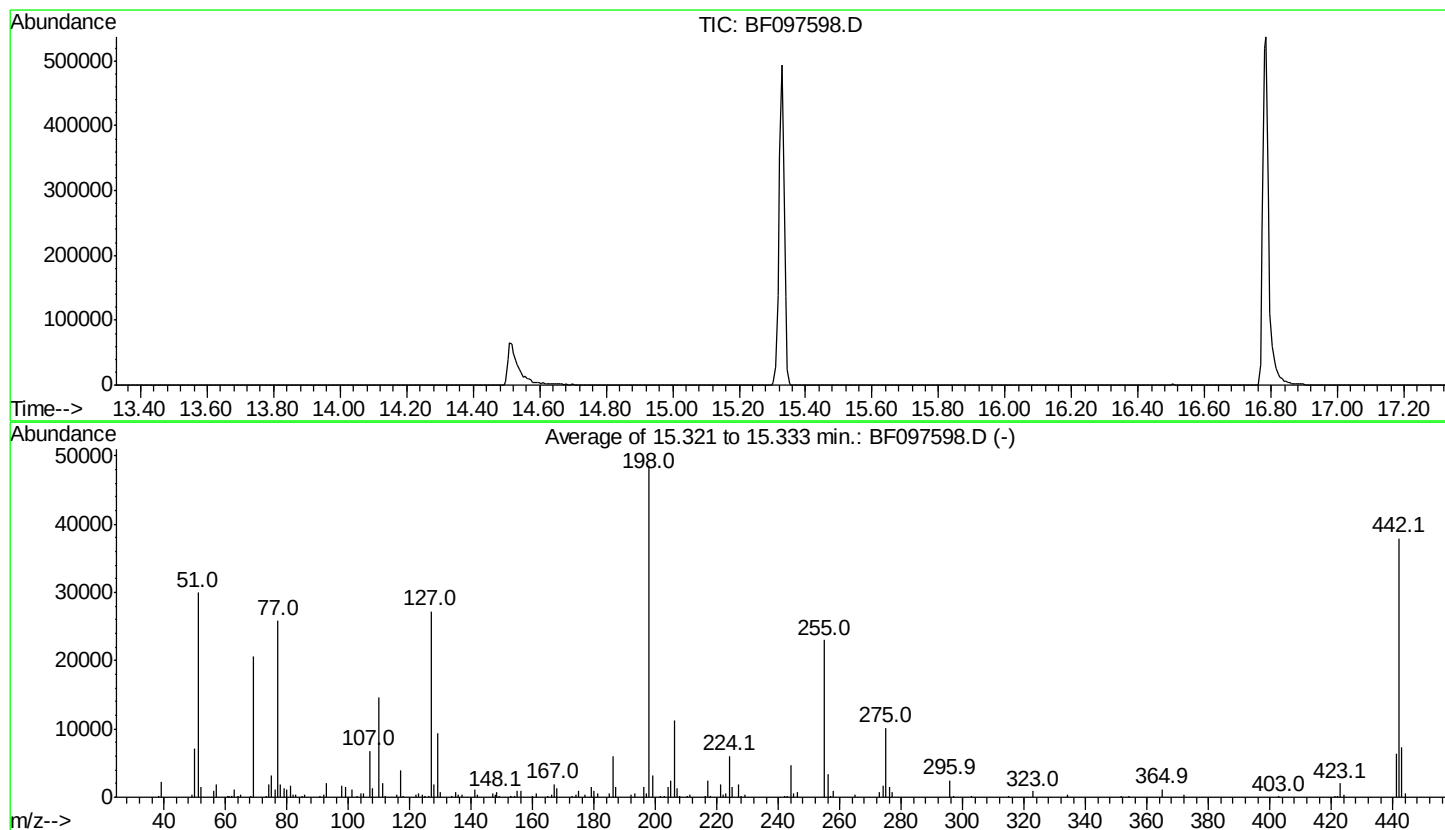

AutoFind: Scans 2318, 2319, 2320; Background Corrected with Scan 2312

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.6	29914	PASS
68	69	0.00	2	1.1	234	PASS
69	198	0.00	100	42.6	20693	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.0	27189	PASS
197	198	0.00	2	1.1	556	PASS
198	198	100	100	100.0	48565	PASS
199	198	5	9	6.7	3240	PASS
275	198	10	60	20.9	10136	PASS
365	198	1	100	2.5	1202	PASS
441	442	0.01	24	16.9	6420	PASS
442	198	50	100	78.0	37898	PASS
443	442	15	24	19.3	7328	PASS