


Data Path : Z:\HPCHEM1\BNA F\Data\BF081117\
 Data File : BF097619.D
 Acq On : 12 Aug 2017 4:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 11 15:55:57 2017

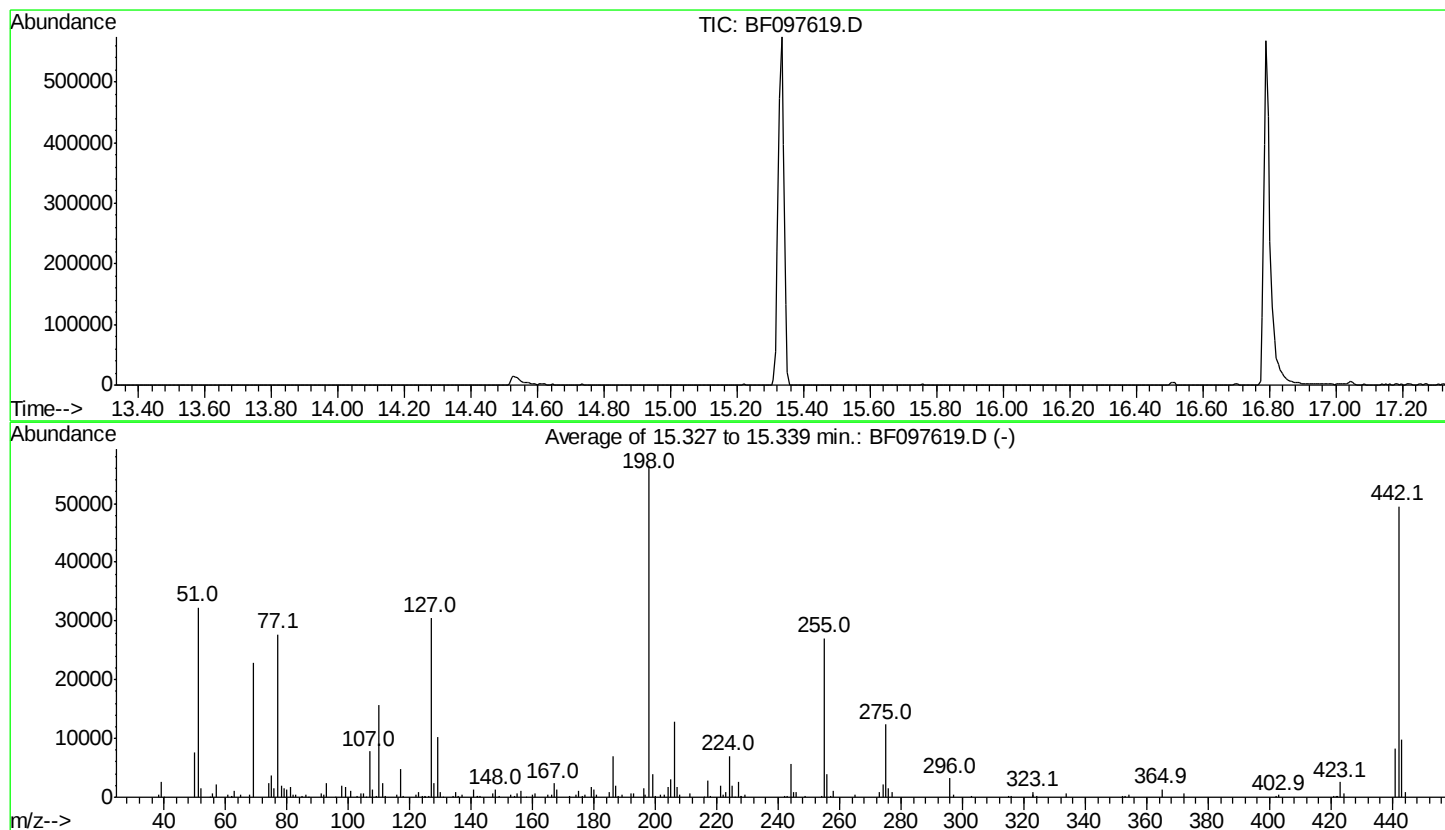

AutoFind: Scans 2319, 2320, 2321; Background Corrected with Scan 2313

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	32312	PASS
68	69	0.00	2	1.7	401	PASS
69	198	0.00	100	40.7	22952	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	30514	PASS
197	198	0.00	2	0.8	452	PASS
198	198	100	100	100.0	56440	PASS
199	198	5	9	7.1	3984	PASS
275	198	10	60	22.0	12413	PASS
365	198	1	100	2.5	1400	PASS
441	442	0.01	24	16.7	8272	PASS
442	198	50	100	87.6	49464	PASS
443	442	15	24	19.8	9778	PASS