

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081120\
 Data File : BF121238.D
 Acq On : 11 Aug 2020 14:08
 Operator : JU/CG
 Sample : PB130878BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130878BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	495	499	509	rBV	36480	55044	1.38%	0.218%
2	5.422	562	567	588	rBV	2808834	3003730	75.39%	11.901%
3	6.433	734	739	761	rBV	2634272	2988039	75.00%	11.838%
4	6.792	797	800	811	rVB	993475	814154	20.43%	3.226%
5	7.357	891	896	923	rBV	1944108	2191459	55.00%	8.682%
6	8.075	1014	1018	1043	rBV	978869	1080776	27.13%	4.282%
7	9.157	1196	1202	1227	rBV	3511198	3901420	97.92%	15.457%
8	9.833	1312	1317	1332	rBV	1152686	1220713	30.64%	4.836%
9	10.627	1447	1452	1484	rBV	1910336	2414929	60.61%	9.568%
10	11.321	1564	1570	1586	rBV	1204711	1289028	32.35%	5.107%
11	12.910	1835	1840	1843	rBV	3633704	3984293	100.00%	15.785%
12	13.962	2015	2019	2034	rVB	1045640	1156325	29.02%	4.581%
13	14.562	2112	2121	2135	rVB2	24870	70185	1.76%	0.278%
14	15.421	2261	2267	2284	rBV	605635	1070214	26.86%	4.240%


Sum of corrected areas: 25240309

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081120\
Data File : BF121238.D
Acq On : 11 Aug 2020 14:08
Operator : JU/CG
Sample : PB130878BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130878BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

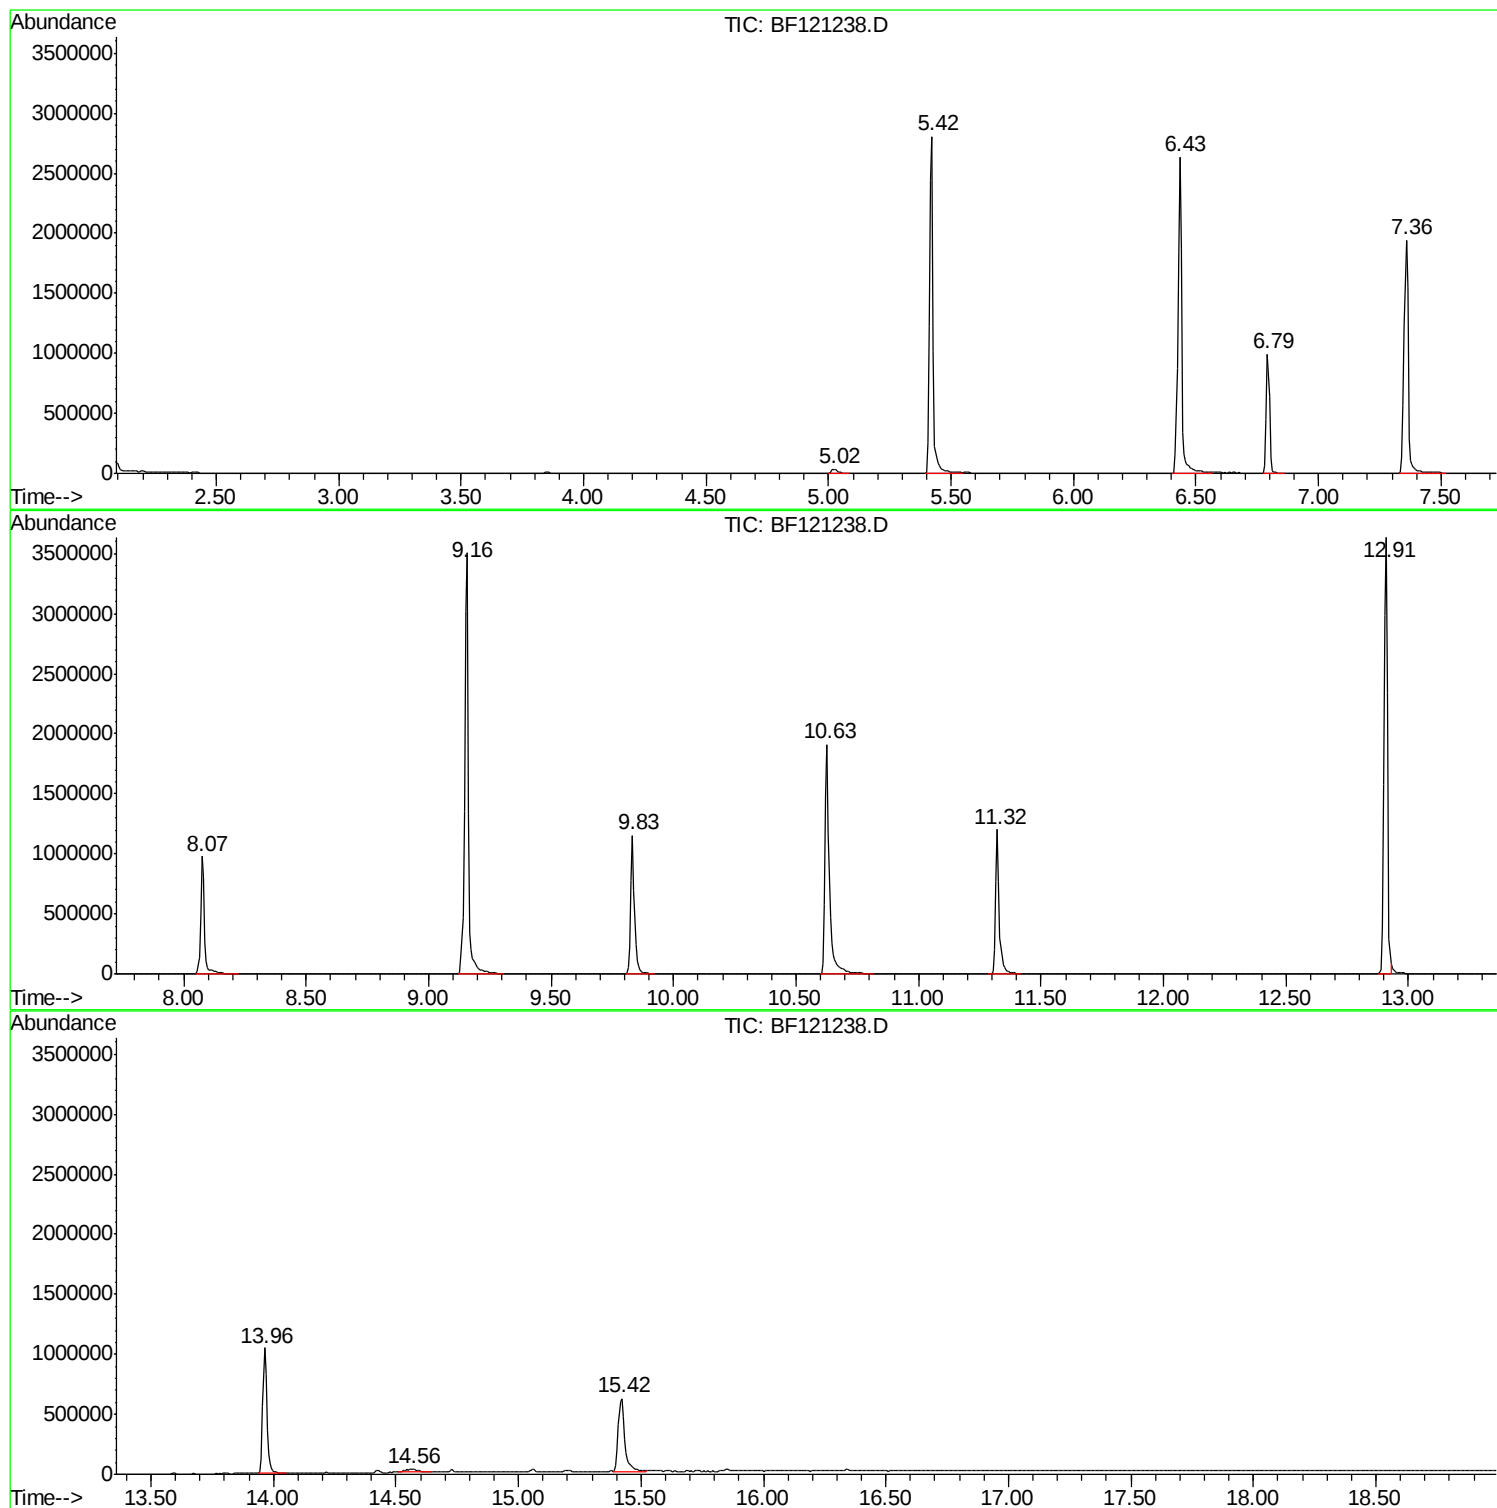

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081120\
Data File : BF121238.D
Acq On : 11 Aug 2020 14:08
Operator : JU/CG
Sample : PB130878BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130878BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081120\
Data File : BF121238.D
Acq On : 11 Aug 2020 14:08
Operator : JU/CG
Sample : PB130878BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130878BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc