

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
 Data File : BF129725.D
 Acq On : 11 Aug 2022 20:34
 Operator : CG\JU
 Sample : N4107-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 12 00:03:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 11 23:50:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.828	152	158997	20.000	ng	-0.01
21) Naphthalene-d8	8.110	136	640127	20.000	ng	-0.01
39) Acenaphthene-d10	9.869	164	330161	20.000	ng	-0.01
64) Phenanthrene-d10	11.357	188	502792	20.000	ng	#-0.01
76) Chrysene-d12	14.004	240	271033	20.000	ng	-0.02
86) Perylene-d12	15.480	264	303311	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	1200404	122.987	ng	0.00
7) Phenol-d6	6.487	99	1534332	125.065	ng	0.00
23) Nitrobenzene-d5	7.398	82	975604	83.197	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	343691	108.275	ng	-0.01
45) 2-Fluorobiphenyl	9.187	172	1780787	83.438	ng	-0.01
79) Terphenyl-d14	12.945	244	1339155	93.215	ng	-0.01
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.398	70	129943	17.496	ng	# 73
25) Isophorone	7.398	82	975592	46.413	ng	# 65
51) 2,6-Dinitrotoluene	9.869	165	43044	8.438	ng	# 25
57) 2,4-Dinitrotoluene	9.869	165	43044	6.459	ng	# 21
67) 4-Bromophenyl-phenylether	10.663	248	20994	3.813	ng	# 1
88) Benzo(b)fluoranthene	15.045	252	40253	2.001	ng	# 92
89) Benzo(k)fluoranthene	15.045	252	40253	2.042	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
Data File : BF129725.D
Acq On : 11 Aug 2022 20:34
Operator : CG\JU
Sample : N4107-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :


Quant Time: Aug 12 00:03:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 11 23:50:03 2022
Response via : Initial Calibration

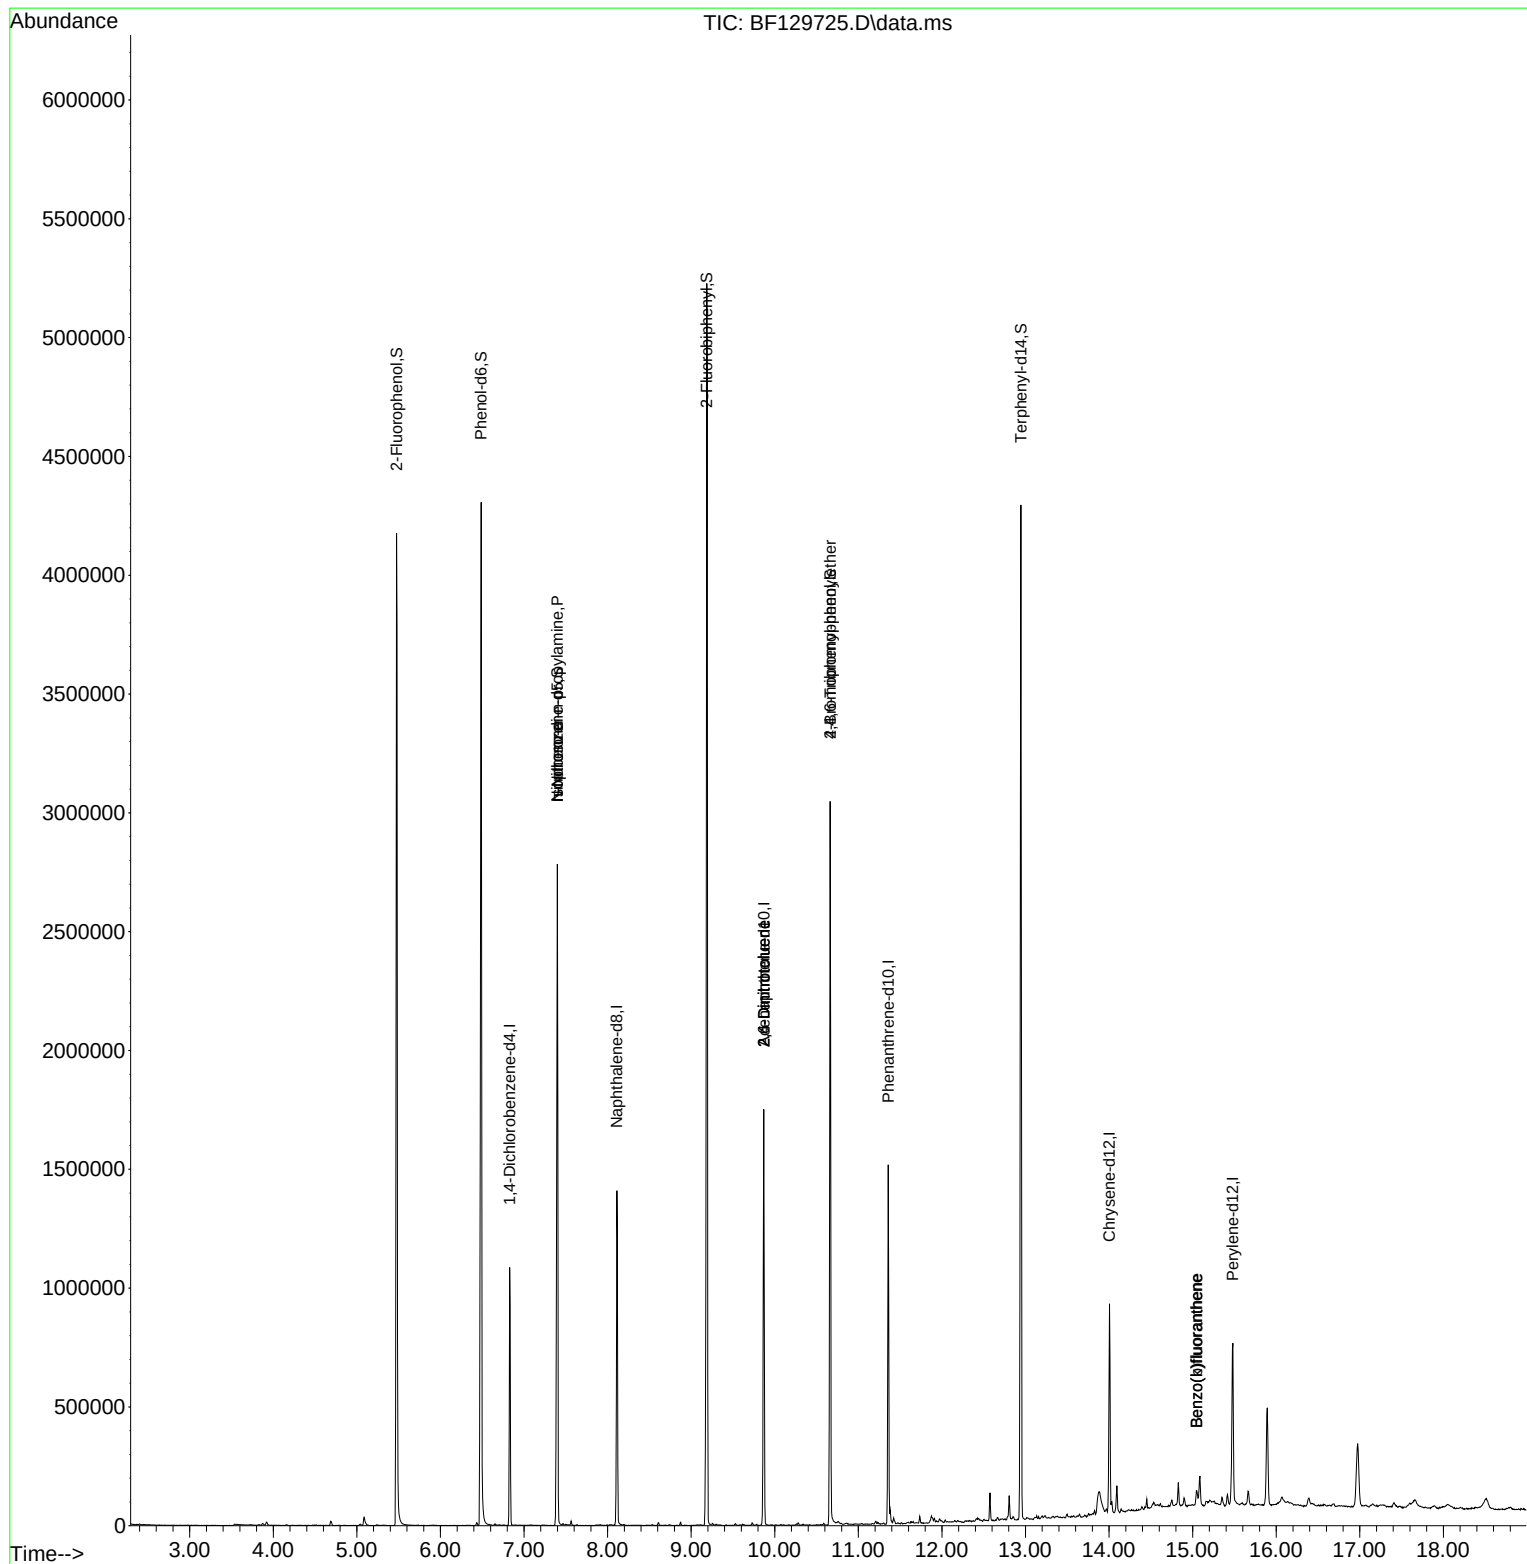






#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.828 min Scan# 71
 Delta R.T. -0.012 min
 Lab File: BF129725.D
 Acq: 11 Aug 2022 20:34

Instrument :
 BNA_F
 ClientSampleId :




Tgt Ion:152 Resp: 158997

Ion	Ratio	Lower	Upper
152	100		
150	158.0	123.7	185.5
115	64.5	49.9	74.9

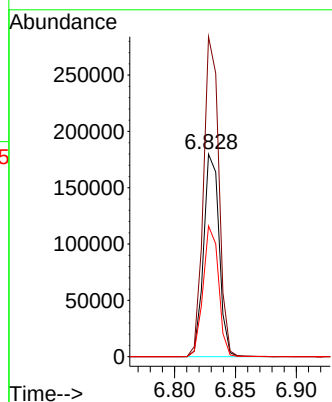




#5
 2-Fluorophenol
 Concen: 122.987 ng
 RT: 5.475 min Scan# 542
 Delta R.T. 0.006 min
 Lab File: BF129725.D
 Acq: 11 Aug 2022 20:34



Tgt Ion:112 Resp: 1200404


Ion	Ratio	Lower	Upper
112	100		
64	63.0	53.3	79.9
63	33.1	28.0	42.0

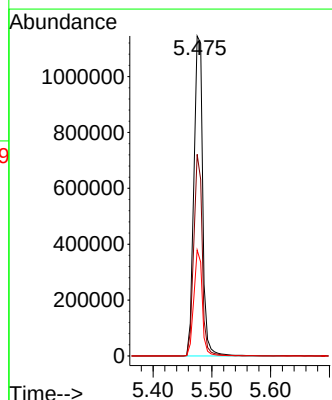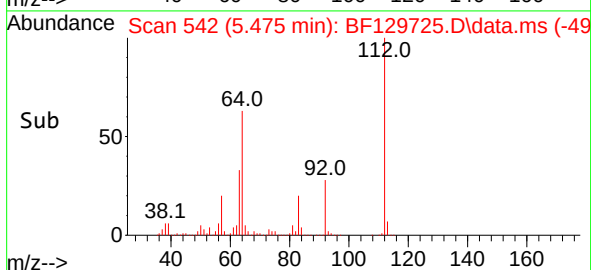






#7
Phenol-d6
Concen: 125.065 ng
RT: 6.487 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

Instrument :
BNA_F
ClientSampleId :



Tgt Ion: 99 Resp: 1534332




Ion	Ratio	Lower	Upper
99	100		
42	18.2	17.3	25.9
71	37.0	28.9	43.3

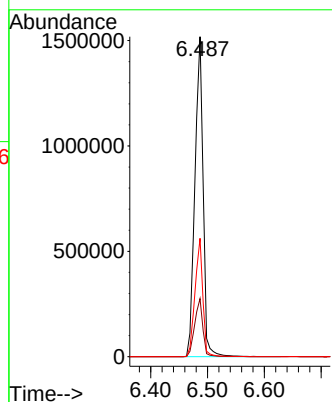


#19
n-Nitroso-di-n-propylamine
Concen: 17.496 ng
RT: 7.398 min Scan# 869
Delta R.T. 0.141 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

Tgt Ion: 70 Resp: 129943


Ion	Ratio	Lower	Upper
70	100		
42	46.8	52.3	78.5#
101	0.0	7.5	11.3#
130	2.0	16.1	24.1#

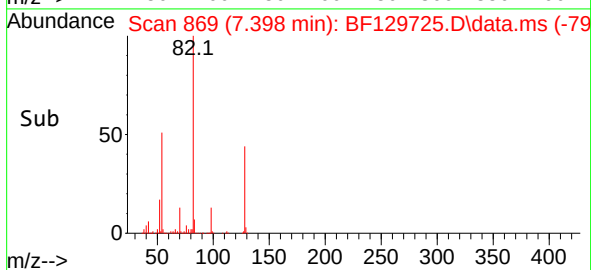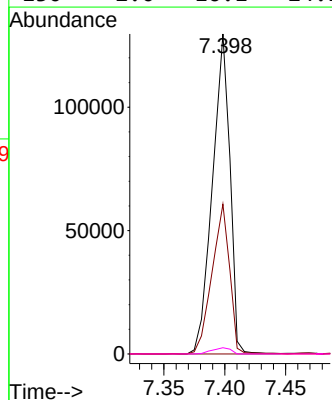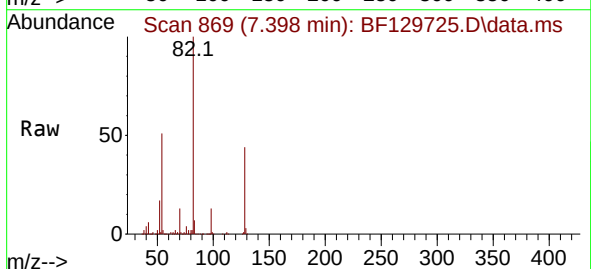






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.110 min Scan# 91
Delta R.T. -0.012 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34


Instrument :
BNA_F
ClientSampleId :





Tgt Ion:136 Resp: 640127
Ion Ratio Lower Upper
136 100
137 11.3 8.8 13.2
54 8.6 7.5 11.3
68 5.6 4.7 7.1

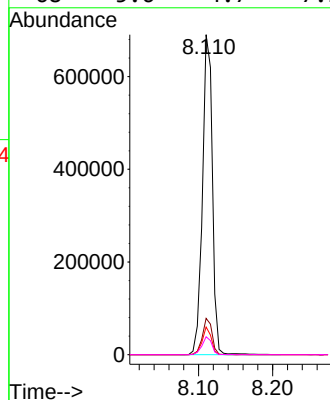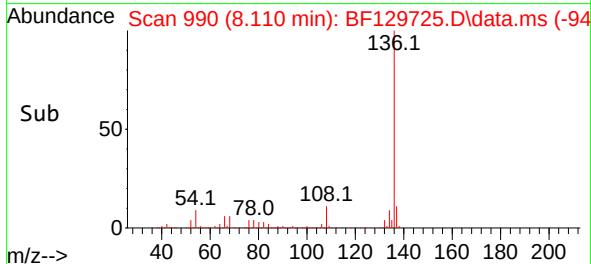


#23
Nitrobenzene-d5
Concen: 83.197 ng
RT: 7.398 min Scan# 869
Delta R.T. -0.012 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

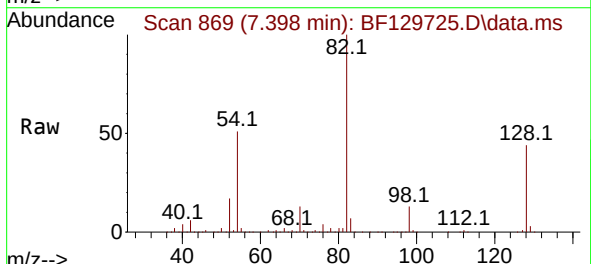

Tgt Ion: 82 Resp: 975604
Ion Ratio Lower Upper
82 100
128 43.8 34.0 51.0
54 50.5 46.9 70.3



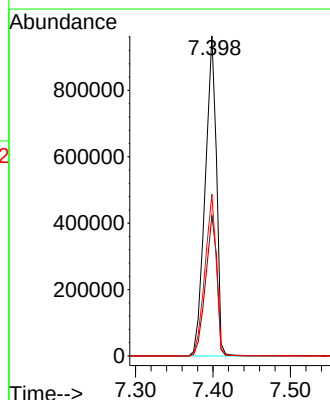





#25
Isophorone
Concen: 46.413 ng
RT: 7.398 min Scan# 80
Delta R.T. -0.265 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34




Instrument :
BNA_F
ClientSampleId :


Tgt Ion: 82 Resp: 975592
Ion Ratio Lower Upper
82 100
95 0.0 5.7 8.5#
138 0.0 14.2 21.2#

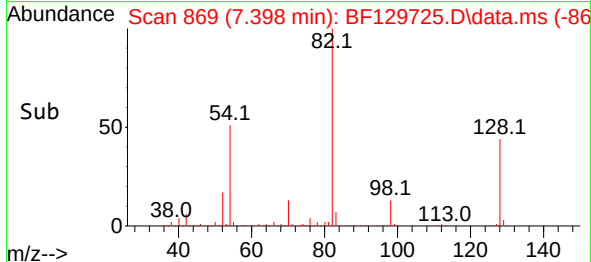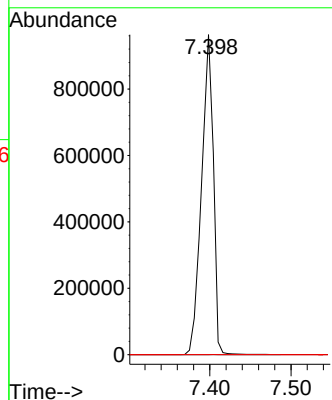

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.869 min Scan# 1289
Delta R.T. -0.012 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

Tgt Ion:164 Resp: 330161
Ion Ratio Lower Upper
164 100
162 102.6 79.5 119.3
160 43.9 34.2 51.4

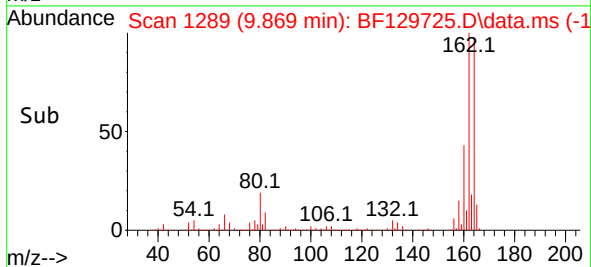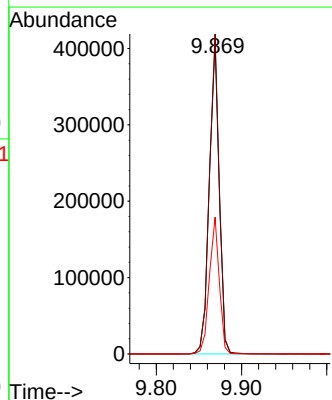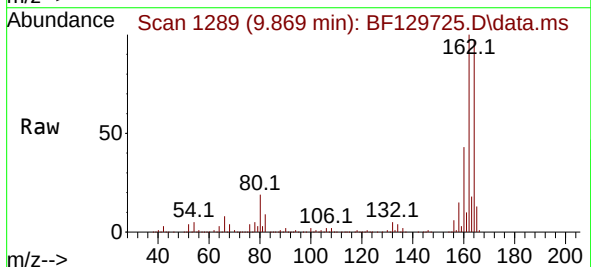



#42

2,4,6-Tribromophenol

Concen: 108.275 ng

RT: 10.663 min Scan# 1434

Delta R.T. -0.012 min


Lab File: BF129725.D

Acq: 11 Aug 2022 20:34

Instrument :

BNA_F

ClientSampleId :






Tgt Ion:330 Resp: 343691

Ion Ratio Lower Upper

330 100

332 104.0 76.8 115.2

141 35.2 28.0 42.0

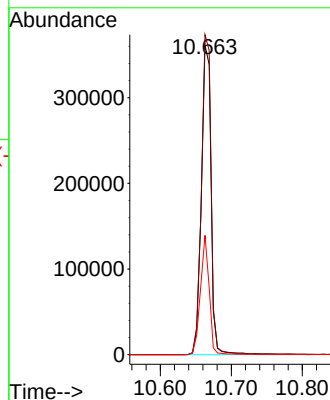

#45

2-Fluorobiphenyl

Concen: 83.438 ng

RT: 9.187 min Scan# 1173

Delta R.T. -0.012 min

Lab File: BF129725.D

Acq: 11 Aug 2022 20:34




Tgt Ion:172 Resp: 1780787


Ion Ratio Lower Upper

172 100

171 35.4 28.8 43.2

170 23.5 19.8 29.8

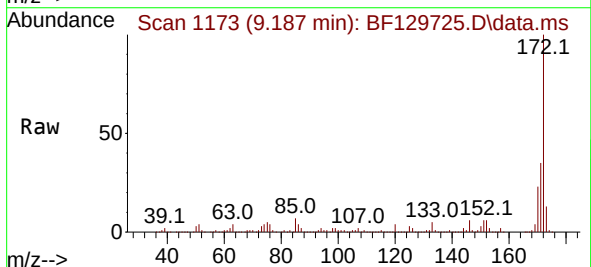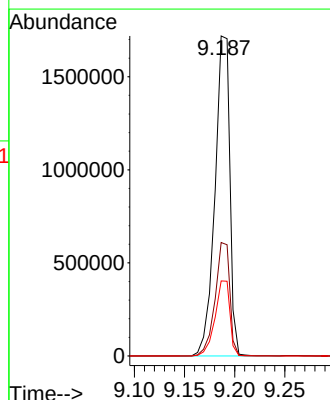



#51

2,6-Dinitrotoluene

Concen: 8.438 ng

RT: 9.869 min Scan# 1289

Delta R.T. 0.200 min

Lab File: BF129725.D

Acq: 11 Aug 2022 20:34

Instrument :

BNA_F

ClientSampleId :





Tgt Ion:165 Resp: 43044

Ion Ratio Lower Upper

165 100

63 1.1 44.9 67.3#

89 1.5 43.6 65.4#

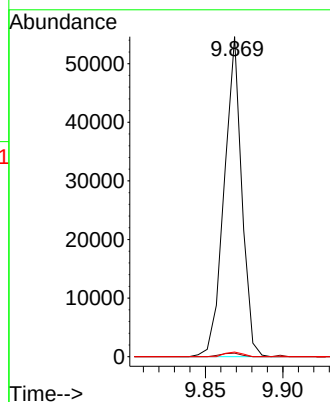

#57

2,4-Dinitrotoluene

Concen: 6.459 ng

RT: 9.869 min Scan# 1289

Delta R.T. -0.212 min

Lab File: BF129725.D

Acq: 11 Aug 2022 20:34

Tgt Ion:165 Resp: 43044




Ion Ratio Lower Upper


165 100

63 1.1 39.8 59.6#

89 1.5 60.2 90.2#

182 0.0 2.2 3.2#

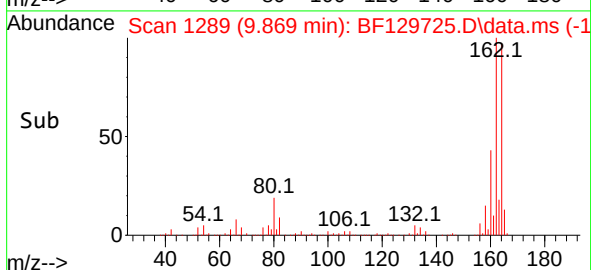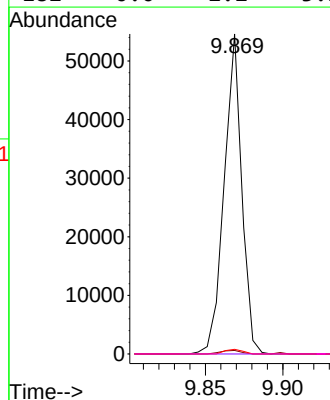



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.357 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF129725.D

Acq: 11 Aug 2022 20:34

Instrument :

BNA_F

ClientSampleId :





Tgt Ion:188 Resp: 502792

Ion Ratio Lower Upper

188 100

94 10.7 7.0 10.6#

80 11.7 7.6 11.4#

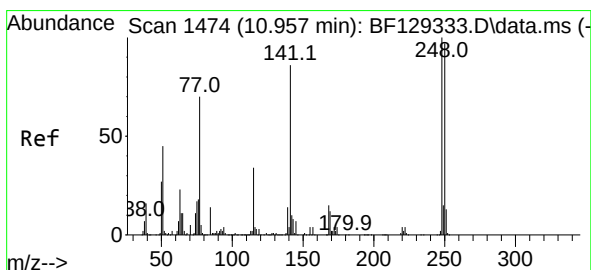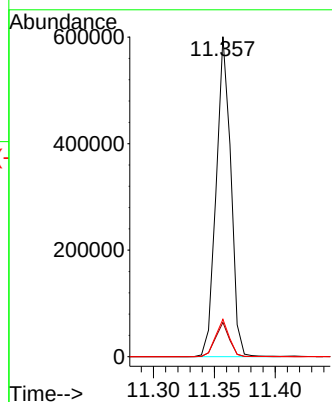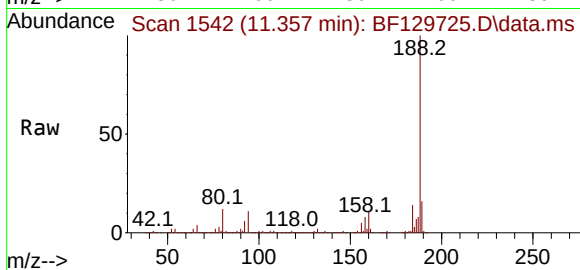

#67

4-Bromophenyl-phenylether

Concen: 3.813 ng

RT: 10.663 min Scan# 1424

Delta R.T. -0.247 min

Lab File: BF129725.D

Acq: 11 Aug 2022 20:34




Tgt Ion:248 Resp: 20994


Ion Ratio Lower Upper

248 100

250 195.0 80.6 120.8#


141 555.9 58.9 88.3#

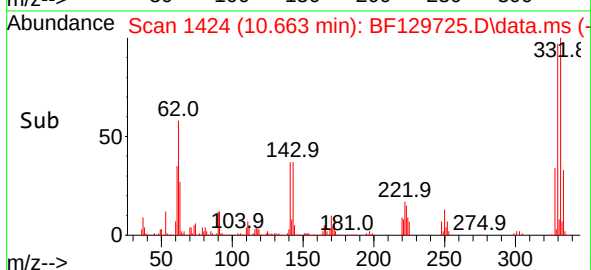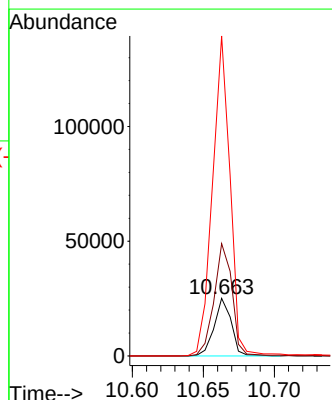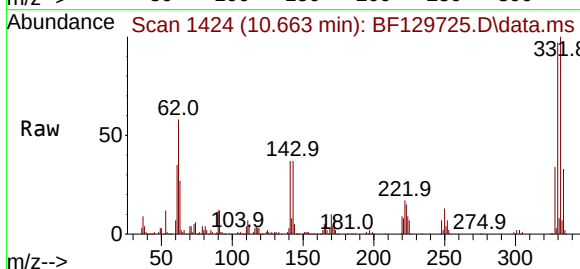






#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.004 min Scan# 1992
Delta R.T. -0.018 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34


Instrument :
BNA_F
ClientSampleId :





Tgt Ion:240 Resp: 271033
Ion Ratio Lower Upper
240 100
120 12.4 8.9 13.3
236 25.8 20.8 31.2

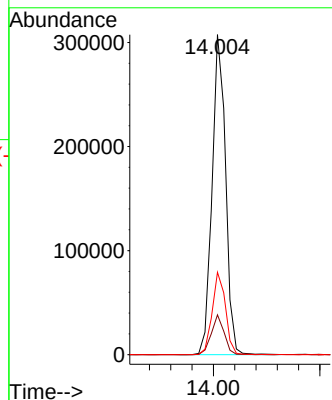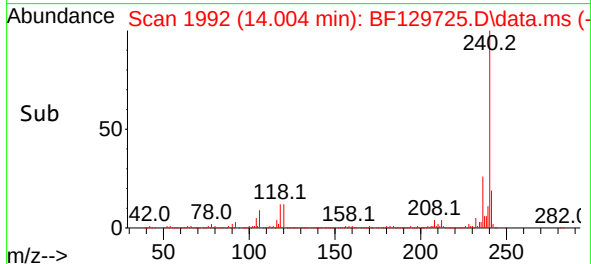


#79
Terphenyl-d14
Concen: 93.215 ng
RT: 12.945 min Scan# 1812
Delta R.T. -0.012 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

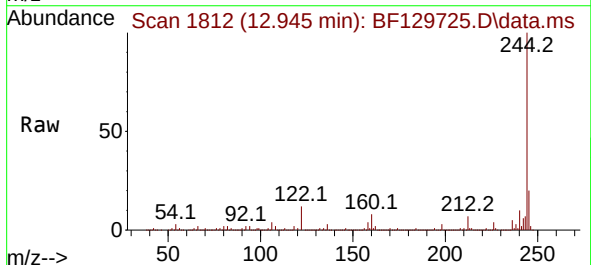


Tgt Ion:244 Resp: 1339155
Ion Ratio Lower Upper
244 100
212 7.2 6.1 9.1
122 12.2 8.8 13.2

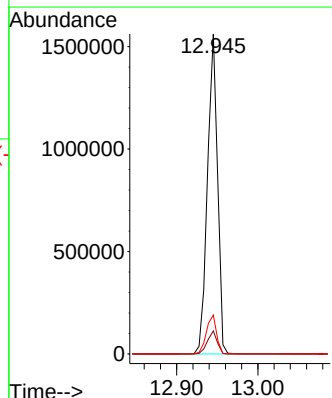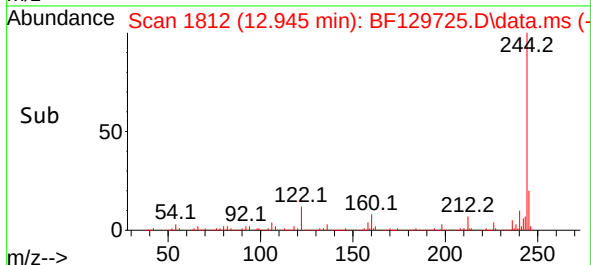






#86
Perylene-d12
Concen: 20.000 ng
RT: 15.480 min Scan# 2169
Delta R.T. -0.012 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

Instrument :
BNA_F
ClientSampleId :



Tgt Ion:264 Resp: 303311




Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.4	27.6
265	20.9	17.2	25.8

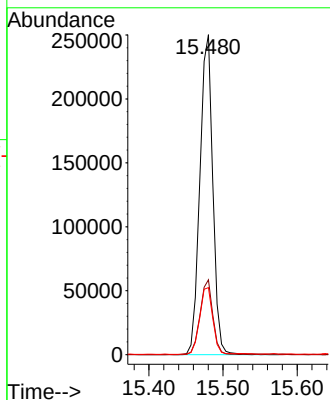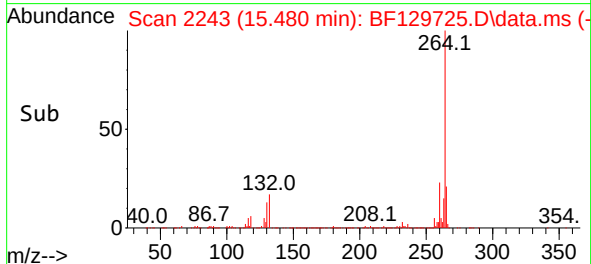


#88
Benzo(b)fluoranthene
Concen: 2.001 ng
RT: 15.045 min Scan# 2169
Delta R.T. -0.018 min
Lab File: BF129725.D
Acq: 11 Aug 2022 20:34

Tgt Ion:252 Resp: 40253

Ion	Ratio	Lower	Upper
252	100		
253	24.9	17.7	26.5
125	15.0	8.0	12.0

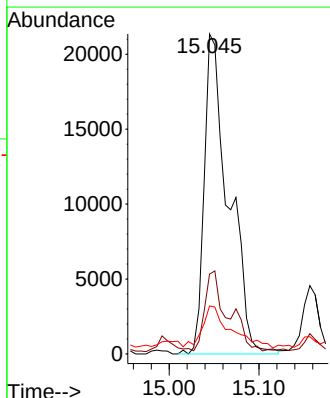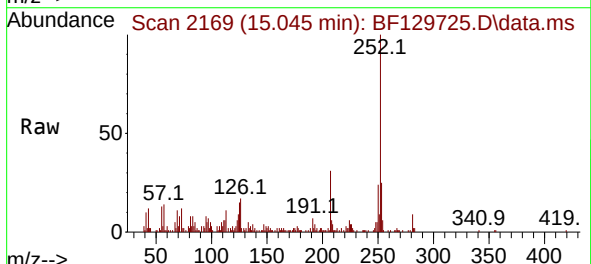



#89

Benzo(k)fluoranthene

Concen: 2.042 ng

RT: 15.045 min Scan# 21

Delta R.T. -0.047 min


Lab File: BF129725.D

Acq: 11 Aug 2022 20:34

Instrument :

BNA_F

ClientSampleId :

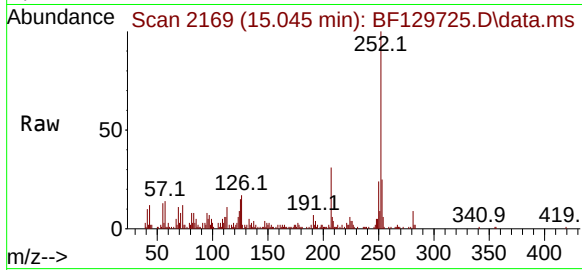

Tgt Ion:252 Resp: 40253

Ion Ratio Lower Upper

252 100

253 24.9 17.8 26.6

125 15.0 8.3 12.5#

