
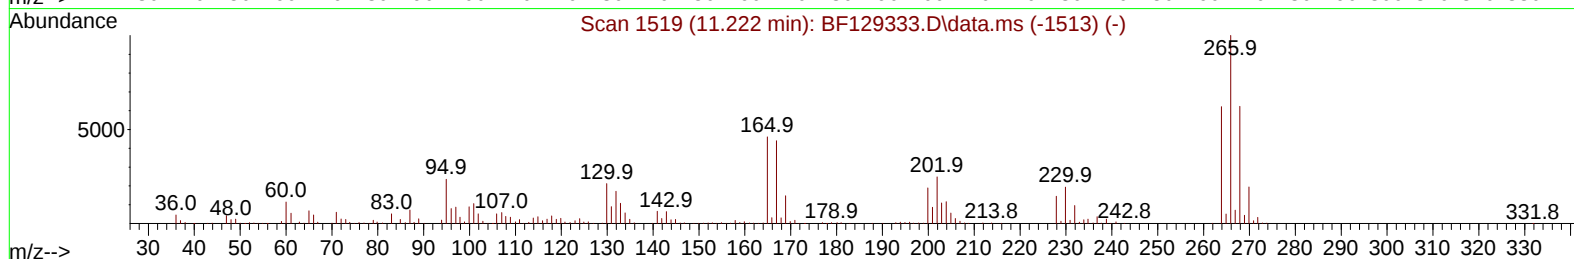
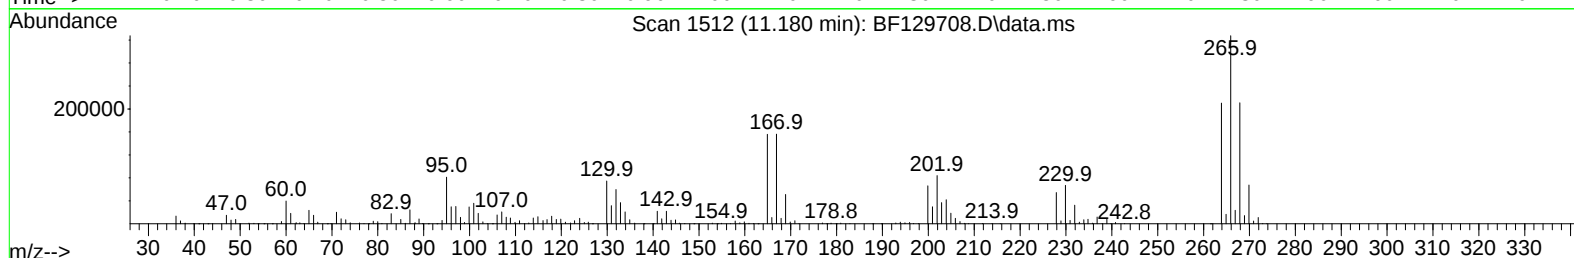


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
 Data File : BF129708.D
 Acq On : 11 Aug 2022 10:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 07:58:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 11 23:50:03 2022
 Response via : Initial Calibration

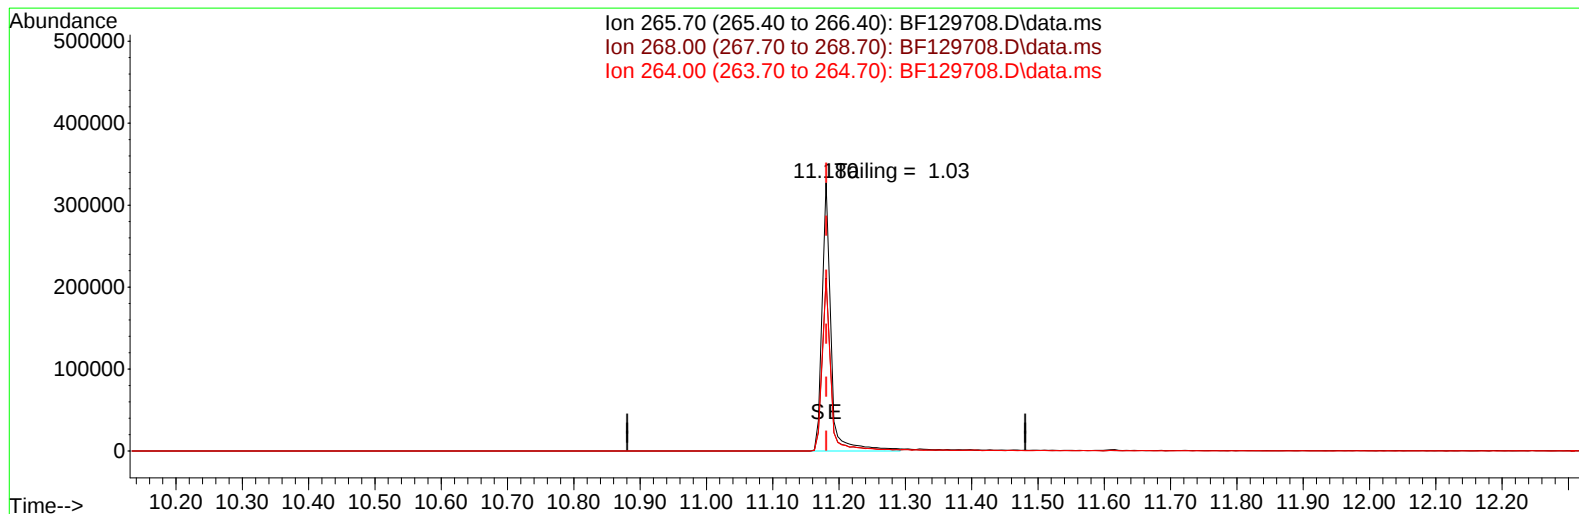

TIC: BF129708.D\data.ms

(70) Pentachlorophenol (C)




11.180min (-0.000) 112780.27 ng

response 313532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.35
264.00	61.80	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
Data File : BF129708.D
Acq On : 11 Aug 2022 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 07:58:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 11 23:50:03 2022
Response via : Initial Calibration

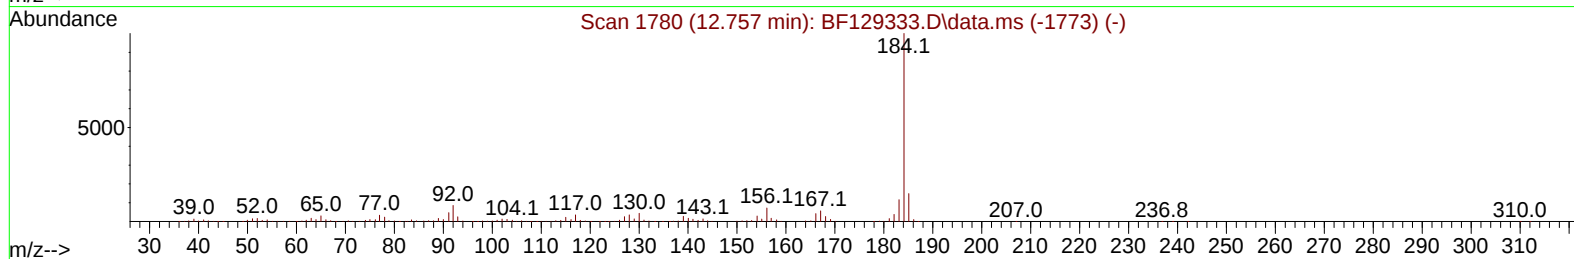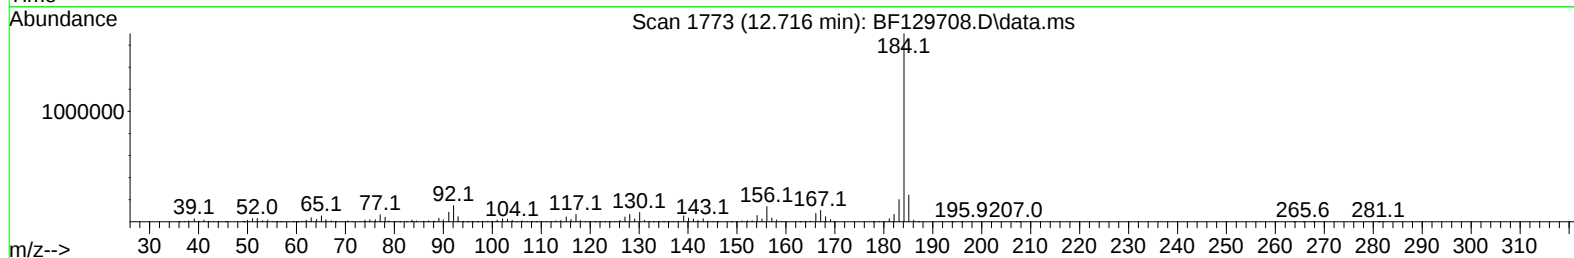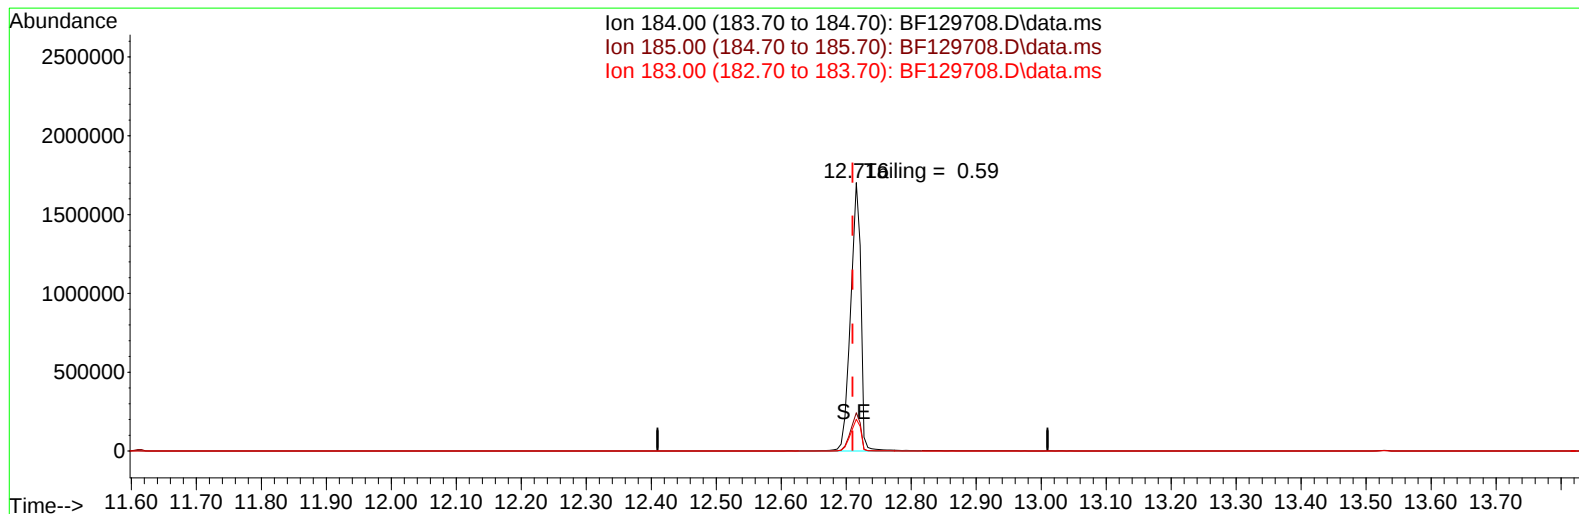

TIC: BF129708.D\data.ms

(77) Benzidine

12.716min (+ 0.006) 78717.44 ng

response 1879883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.25
183.00	11.60	11.88
0.00	0.00	0.00