
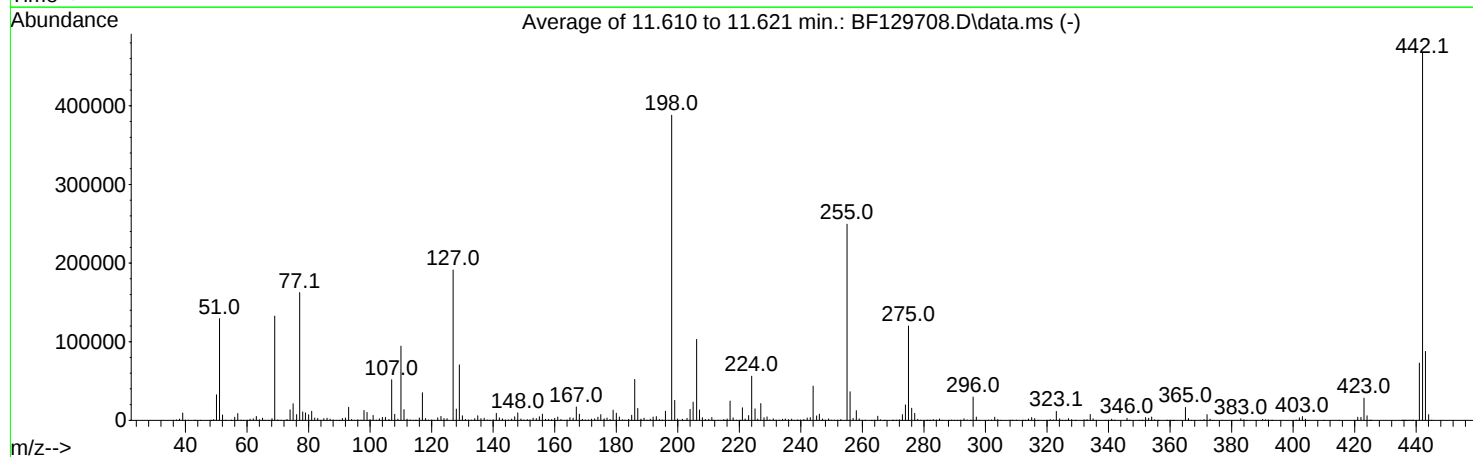


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081122\  
 Data File : BF129708.D  
 Acq On : 11 Aug 2022 10:03  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Aug 11 23:50:03 2022

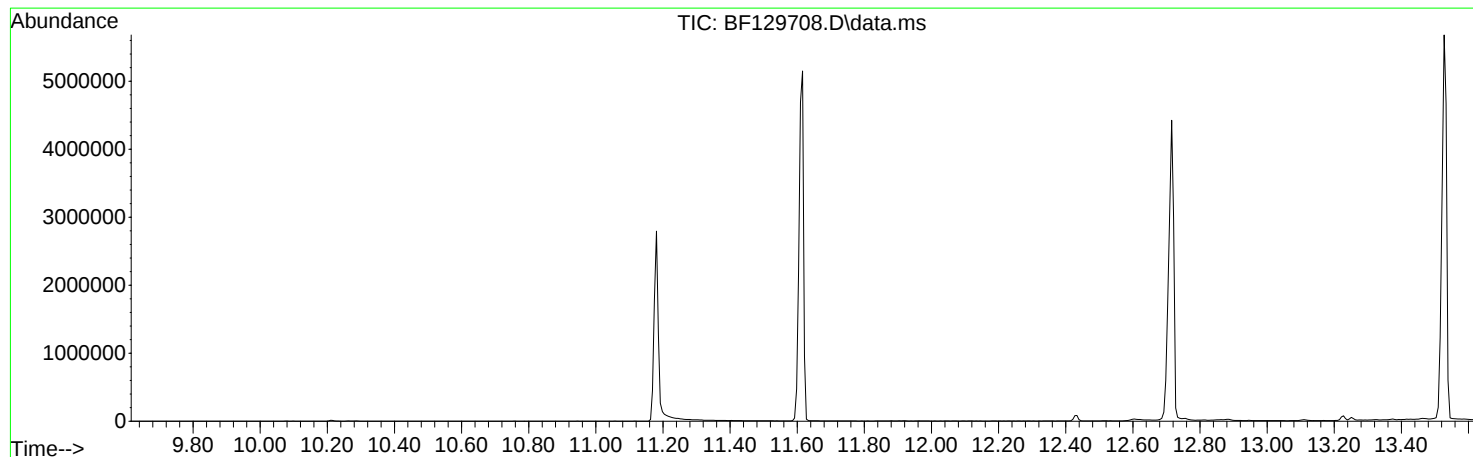




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1578

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.4         | 129461     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 2282       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.2         | 132583     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 694        | PASS                |
| 127            | 198             | 10              | 80              | 49.3         | 191333     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.1          | 224        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 388099     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 25423      | PASS                |
| 275            | 198             | 10              | 60              | 31.0         | 120128     | PASS                |
| 365            | 198             | 1               | 100             | 4.3          | 16519      | PASS                |
| 441            | 198             | 0.01            | 100             | 18.8         | 72936      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 467776     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 87797      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081122\  
 Data File : BF129708.D  
 Acq On : 11 Aug 2022 10:03  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 12 07:58:00 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Aug 11 23:50:03 2022  
 Response via : Initial Calibration

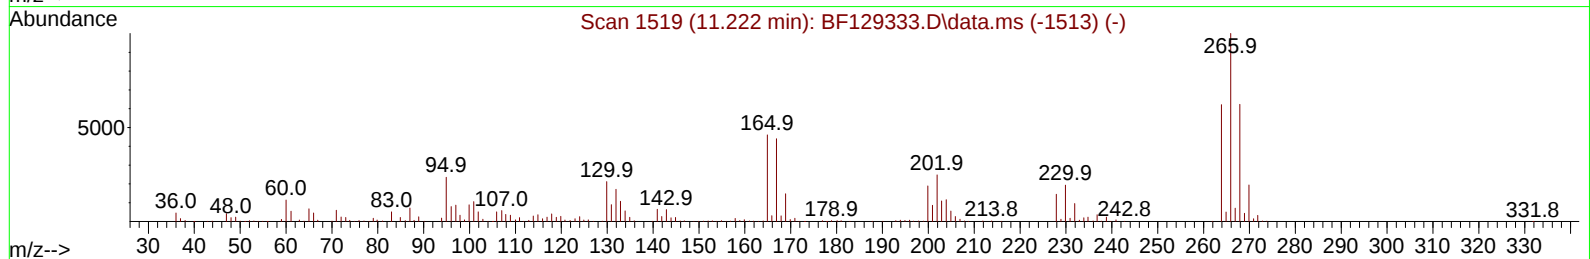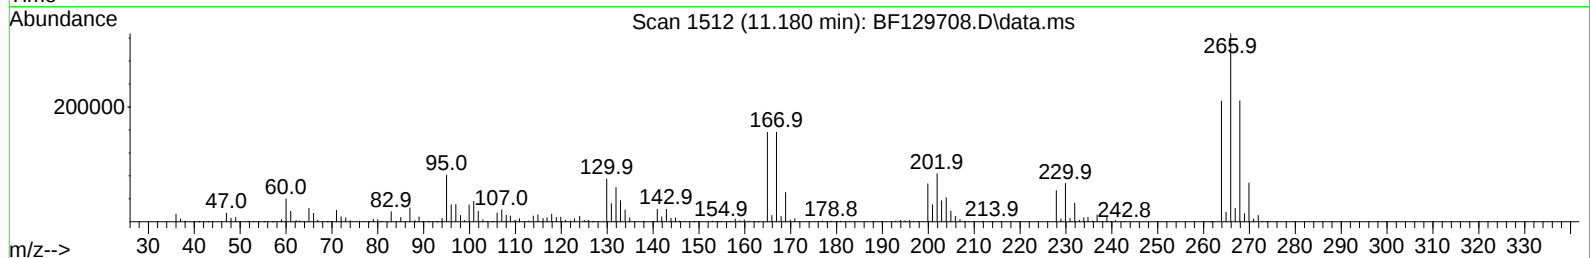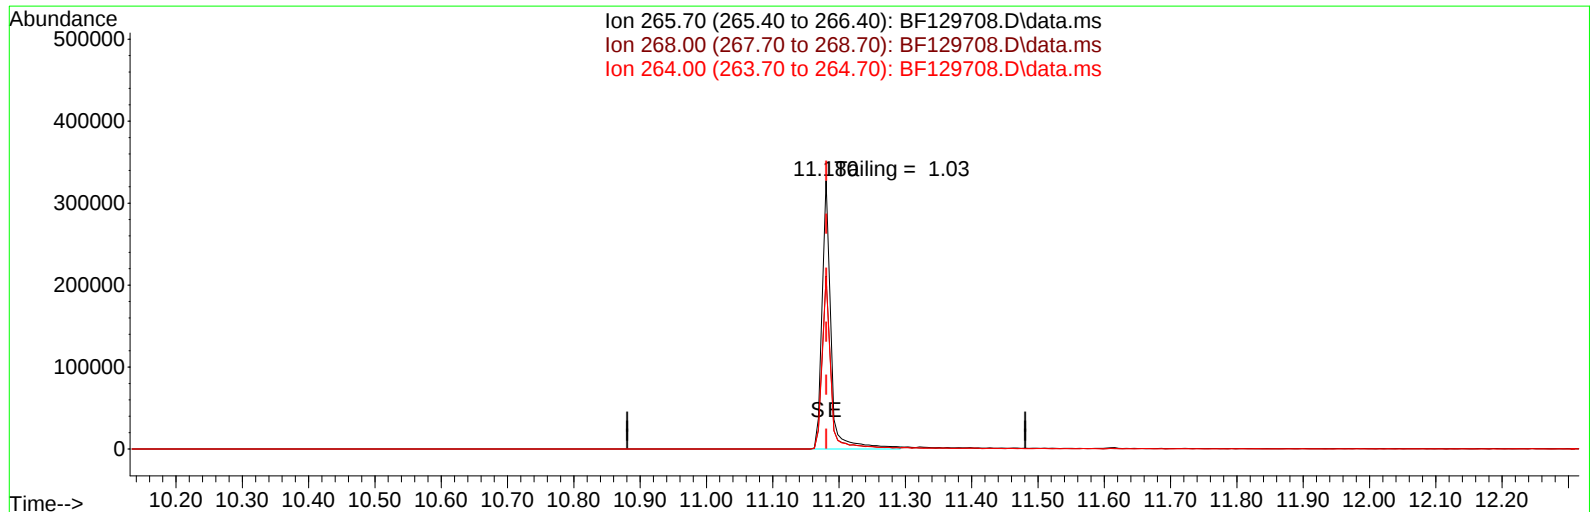

TIC: BF129708.D\data.ms

**(70) Pentachlorophenol (C)**

11.180min (-0.000) 112780.27 ng




response 313532

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.70  | 64.35  |
| 264.00 | 61.80  | 64.16  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081122\  
Data File : BF129708.D  
Acq On : 11 Aug 2022 10:03  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 12 07:58:00 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 11 23:50:03 2022  
Response via : Initial Calibration

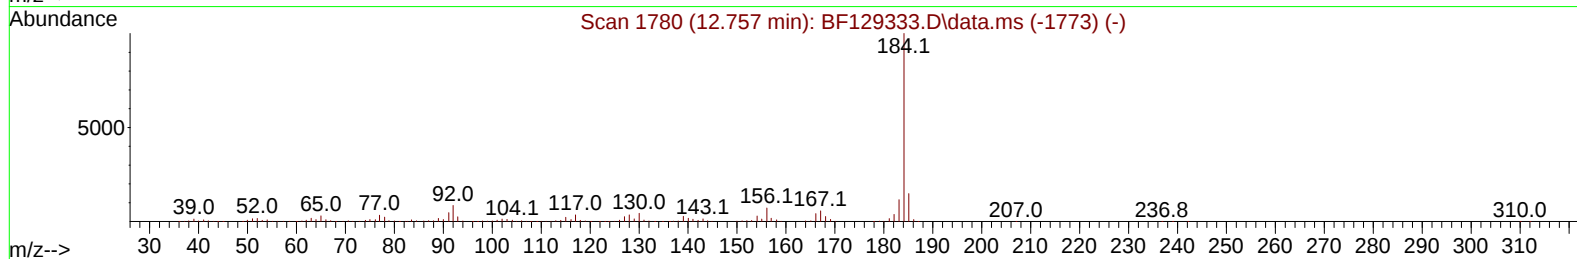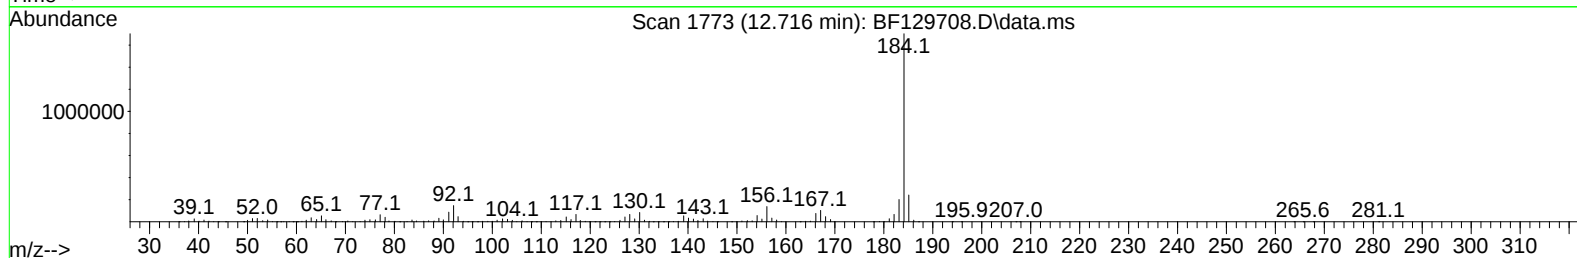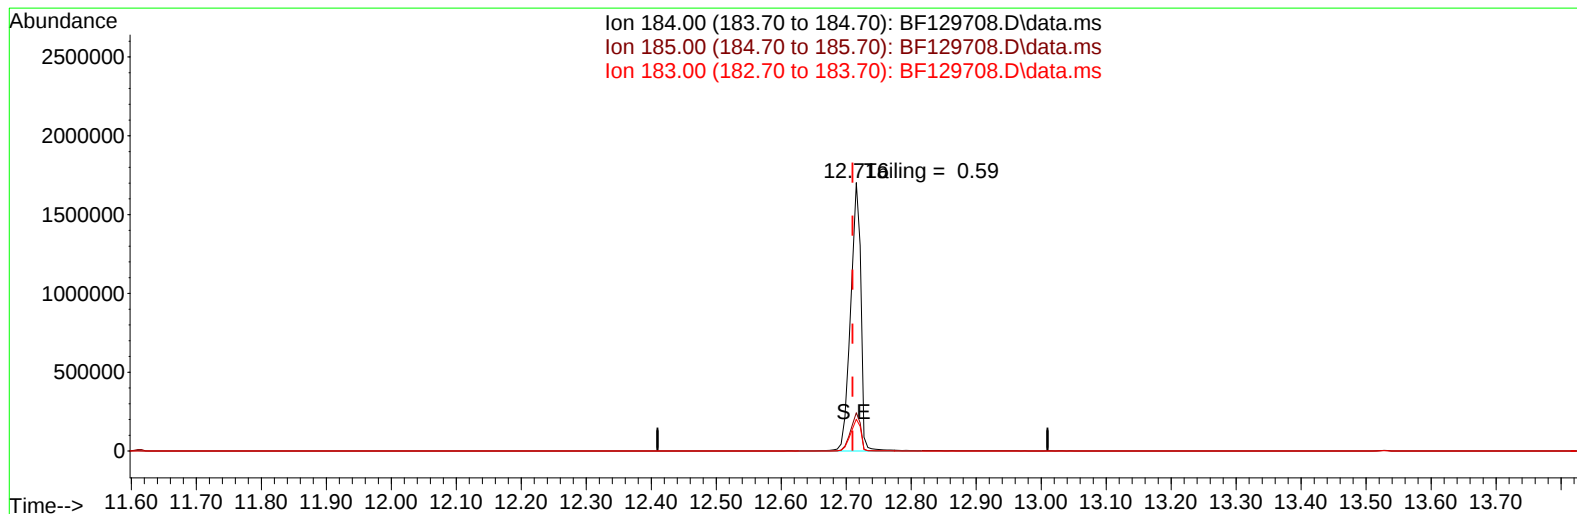

TIC: BF129708.D\data.ms

**(77) Benzidine**

**12.716min (+ 0.006) 78717.44 ng**

**response 1879883**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.25  |
| 183.00 | 11.60  | 11.88  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/11/2022     | BNA_F            | <u>BF129708.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1072058          | 13.527             |
| DDD           | 17683            | 13.27              |
| DDE           | 2262             | 12.886             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 19945         | 1092003          | 1.83               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP