
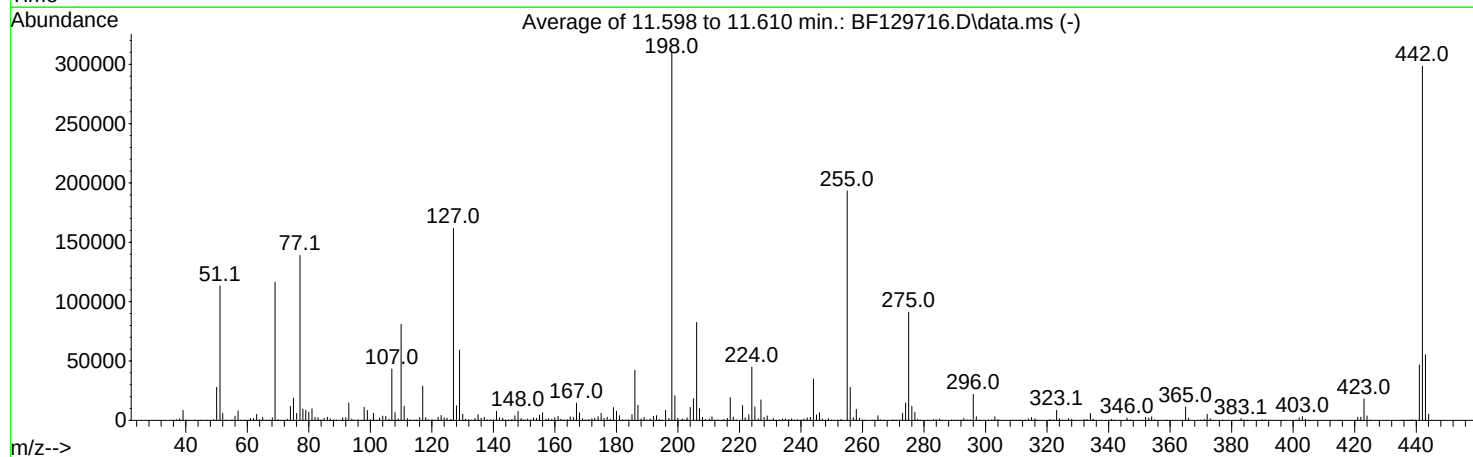


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
 Data File : BF129716.D
 Acq On : 11 Aug 2022 15:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 12 15:52:45 2022

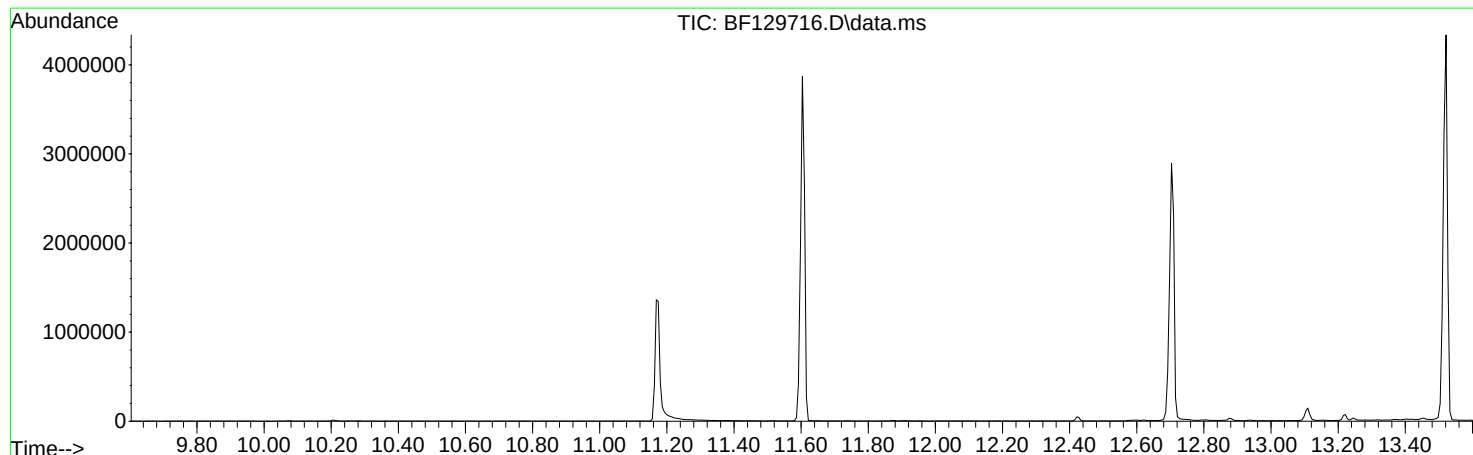




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	113264	PASS
68	69	0.00	2	1.8	2146	PASS
69	198	0.00	100	37.6	116427	PASS
70	69	0.00	2	0.5	598	PASS
127	198	10	80	52.2	161837	PASS
197	198	0.00	2	0.6	1709	PASS
198	198	100	100	100.0	309931	PASS
199	198	5	9	6.7	20732	PASS
275	198	10	60	29.4	91104	PASS
365	198	1	100	3.6	11304	PASS
441	198	0.01	100	15.0	46597	PASS
442	442	50	100	100.0	298461	PASS
443	442	15	24	18.5	55328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
Data File : BF129716.D
Acq On : 11 Aug 2022 15:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 07:59:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 11 23:50:03 2022
Response via : Initial Calibration

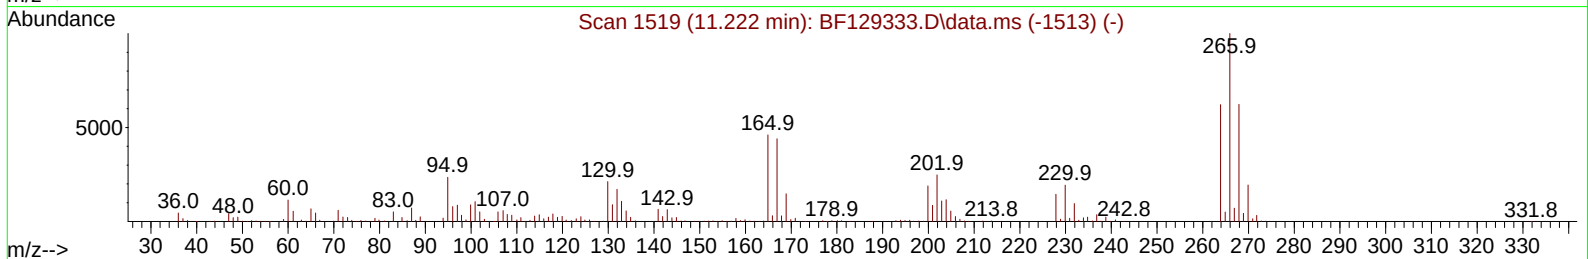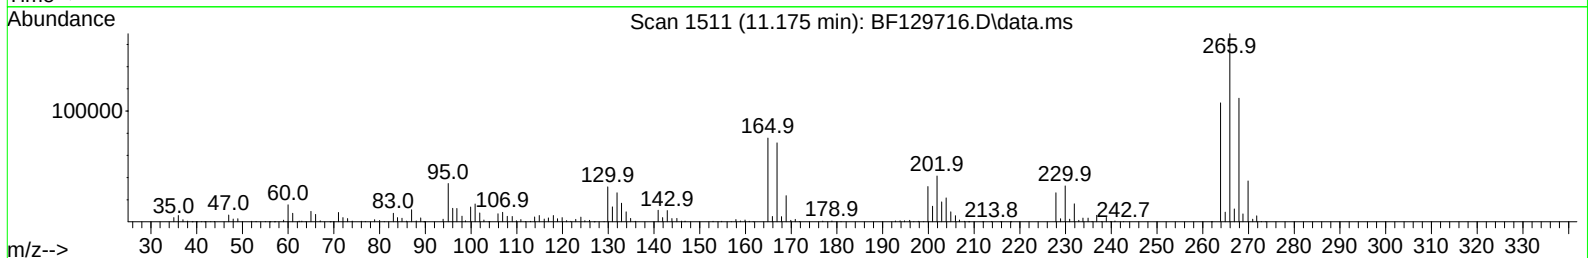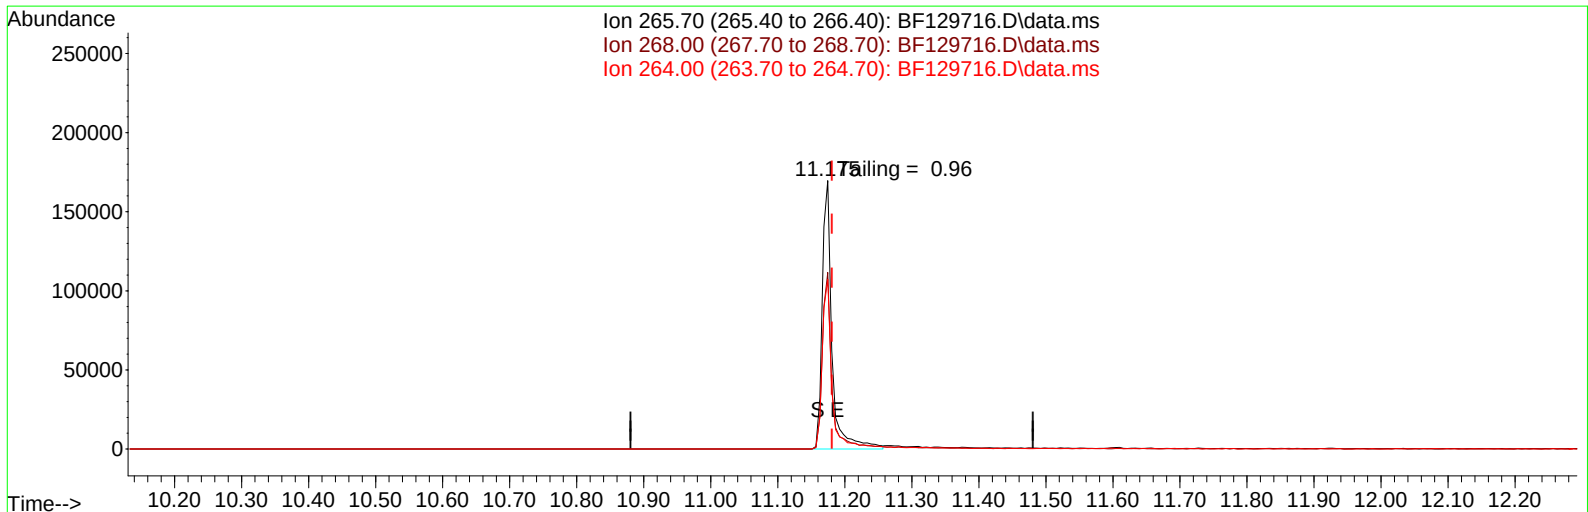

TIC: BF129716.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.006) 41716.35 ng




response 176515

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.76
264.00	61.80	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081122\
 Data File : BF129716.D
 Acq On : 11 Aug 2022 15:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 12 07:59:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 11 23:50:03 2022
 Response via : Initial Calibration

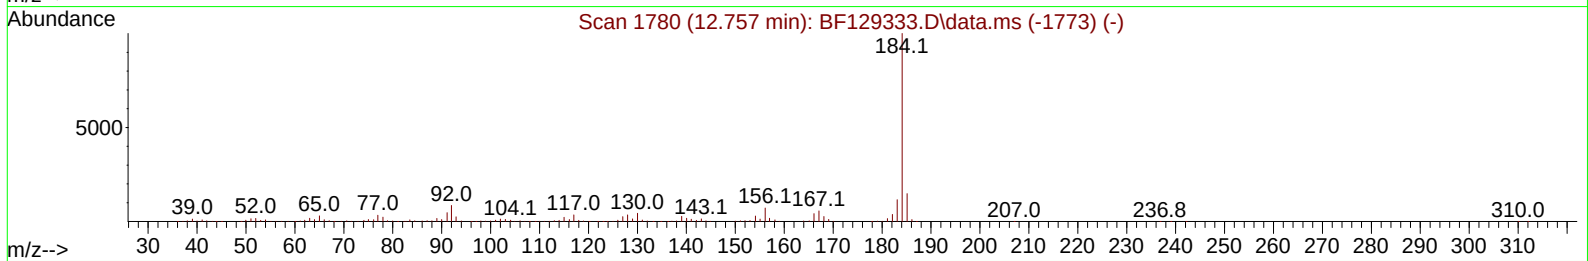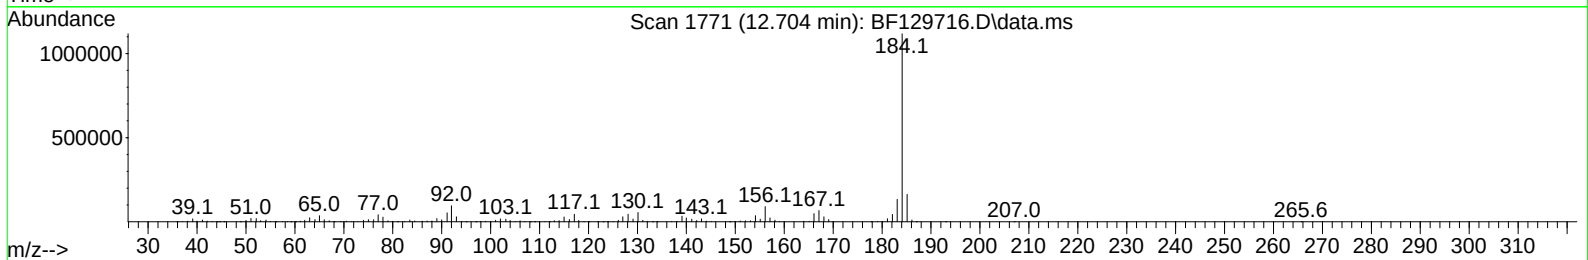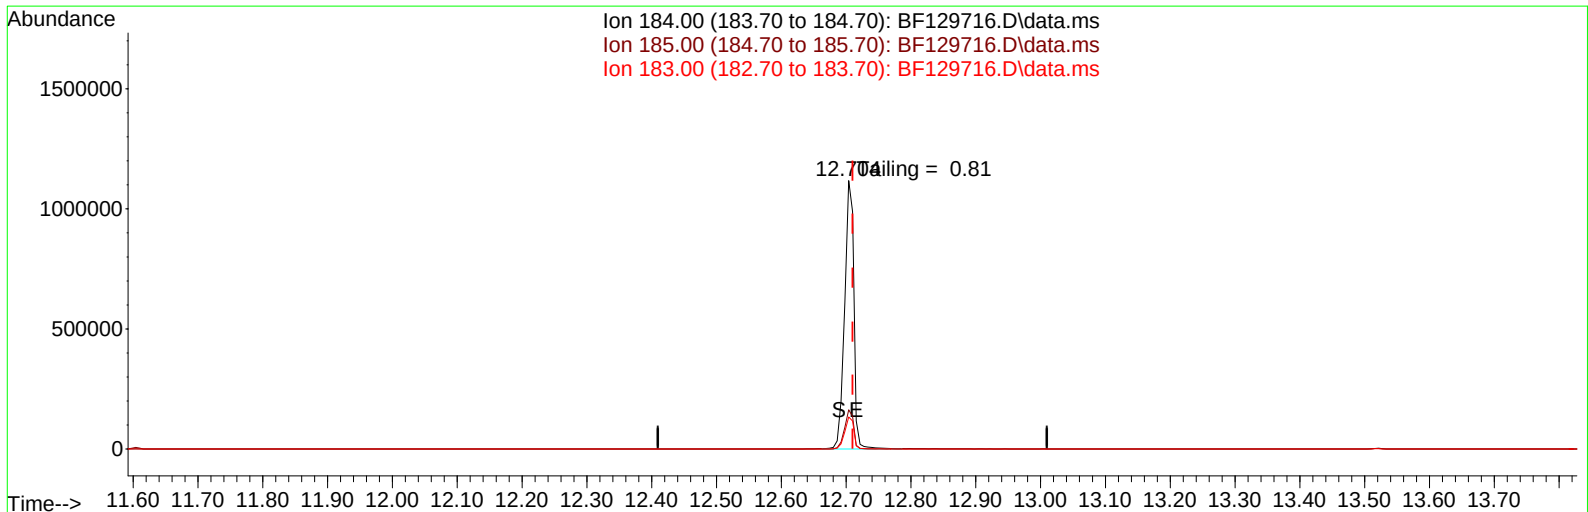

TIC: BF129716.D\data.ms

(77) Benzidine

12.704min (-0.006) 15818.07 ng

response 1118744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.61
183.00	11.60	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2022	BNA_F	<u>BF129716.D</u>
Compound Name	Response	Retention Time
DDT	716301	13.521
DDD	15342	13.221
DDE	3354	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18696	734997	2.54

Instrument :
BNA_F
ClientSampleId :
DFTPP