

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
 Data File : BF097658.D
 Acq On : 13 Aug 2017 6:14
 Operator : SJ/JU
 Sample : I4697-08DL 250X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NYSEG-PH4-ESMI-4BDL

Quant Time: Aug 14 05:26:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 15:55:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	126596	20.00	ng	0.00
21) Naphthalene-d8	9.53	136	497512	20.00	ng	0.00
38) Acenaphthene-d10	12.35	164	197220	20.00	ng	-0.02
63) Phenanthrene-d10	14.75	188	281694	20.00	ng	-0.01
75) Chrysene-d12	18.45	240	193383	20.00	ng	-0.01
86) Perylene-d12	20.12	264	181314	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	8.57	82	110	0.01	ng	0.15
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	11.32	172	3421	0.26	ng	0.00
78) Terphenyl-d14	17.10	244	1784	0.19	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
31) Naphthalene	9.56	128	1040604	41.76	ng	99
33) 4-Chloroaniline	9.56	127	137325	13.30	ng	# 36
37) 2-Methylnaphthalene	10.69	142	192829	12.30	ng	98
45) 1,1'-Biphenyl	11.46	154	64304	3.80	ng	93
48) Acenaphthylene	12.13	152	44729	2.17	ng	97
50) 2,6-Dinitrotoluene	12.35	165	25447	8.11	ng	# 31
51) Acenaphthene	12.40	154	262512	21.21	ng	99
54) Dibenzofuran	12.69	168	219681	12.68	ng	97
55) 4-Nitrophenol	12.69	139	84275	53.85	ng	# 27
57) Fluorene	13.24	166	197709	13.87	ng	99
70) Phenanthrene	14.79	178	851538	52.48	ng	99
71) Anthracene	14.87	178	242340	14.60	ng	98
72) Carbazole	15.18	167	60312	3.82	ng	98
74) Fluoranthene	16.56	202	525352	35.83	ng	98
77) Pyrene	16.86	202	429712	26.87	ng	96
80) Benzo(a)anthracene	18.48	228	115115	10.19	ng	97
82) Chrysene	18.48	228	115115	10.25	ng	99
85) Indeno(1,2,3-cd)pyrene	21.34	276	61217	7.01	ng	99
87) Benzo(b)fluoranthene	19.72	252	199315	18.31	ng	# 94
88) Benzo(k)fluoranthene	19.72	252	199315	18.18	ng	97
89) Benzo(a)pyrene	20.06	252	123616	12.37	ng	98
91) Benzo(g,h,i)perylene	21.69	276	57527	7.33	ng	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
Data File : BF097658.D
Acq On : 13 Aug 2017 6:14
Operator : SJ/JU
Sample : I4697-08DL 250X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL

Quant Time: Aug 14 05:26:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

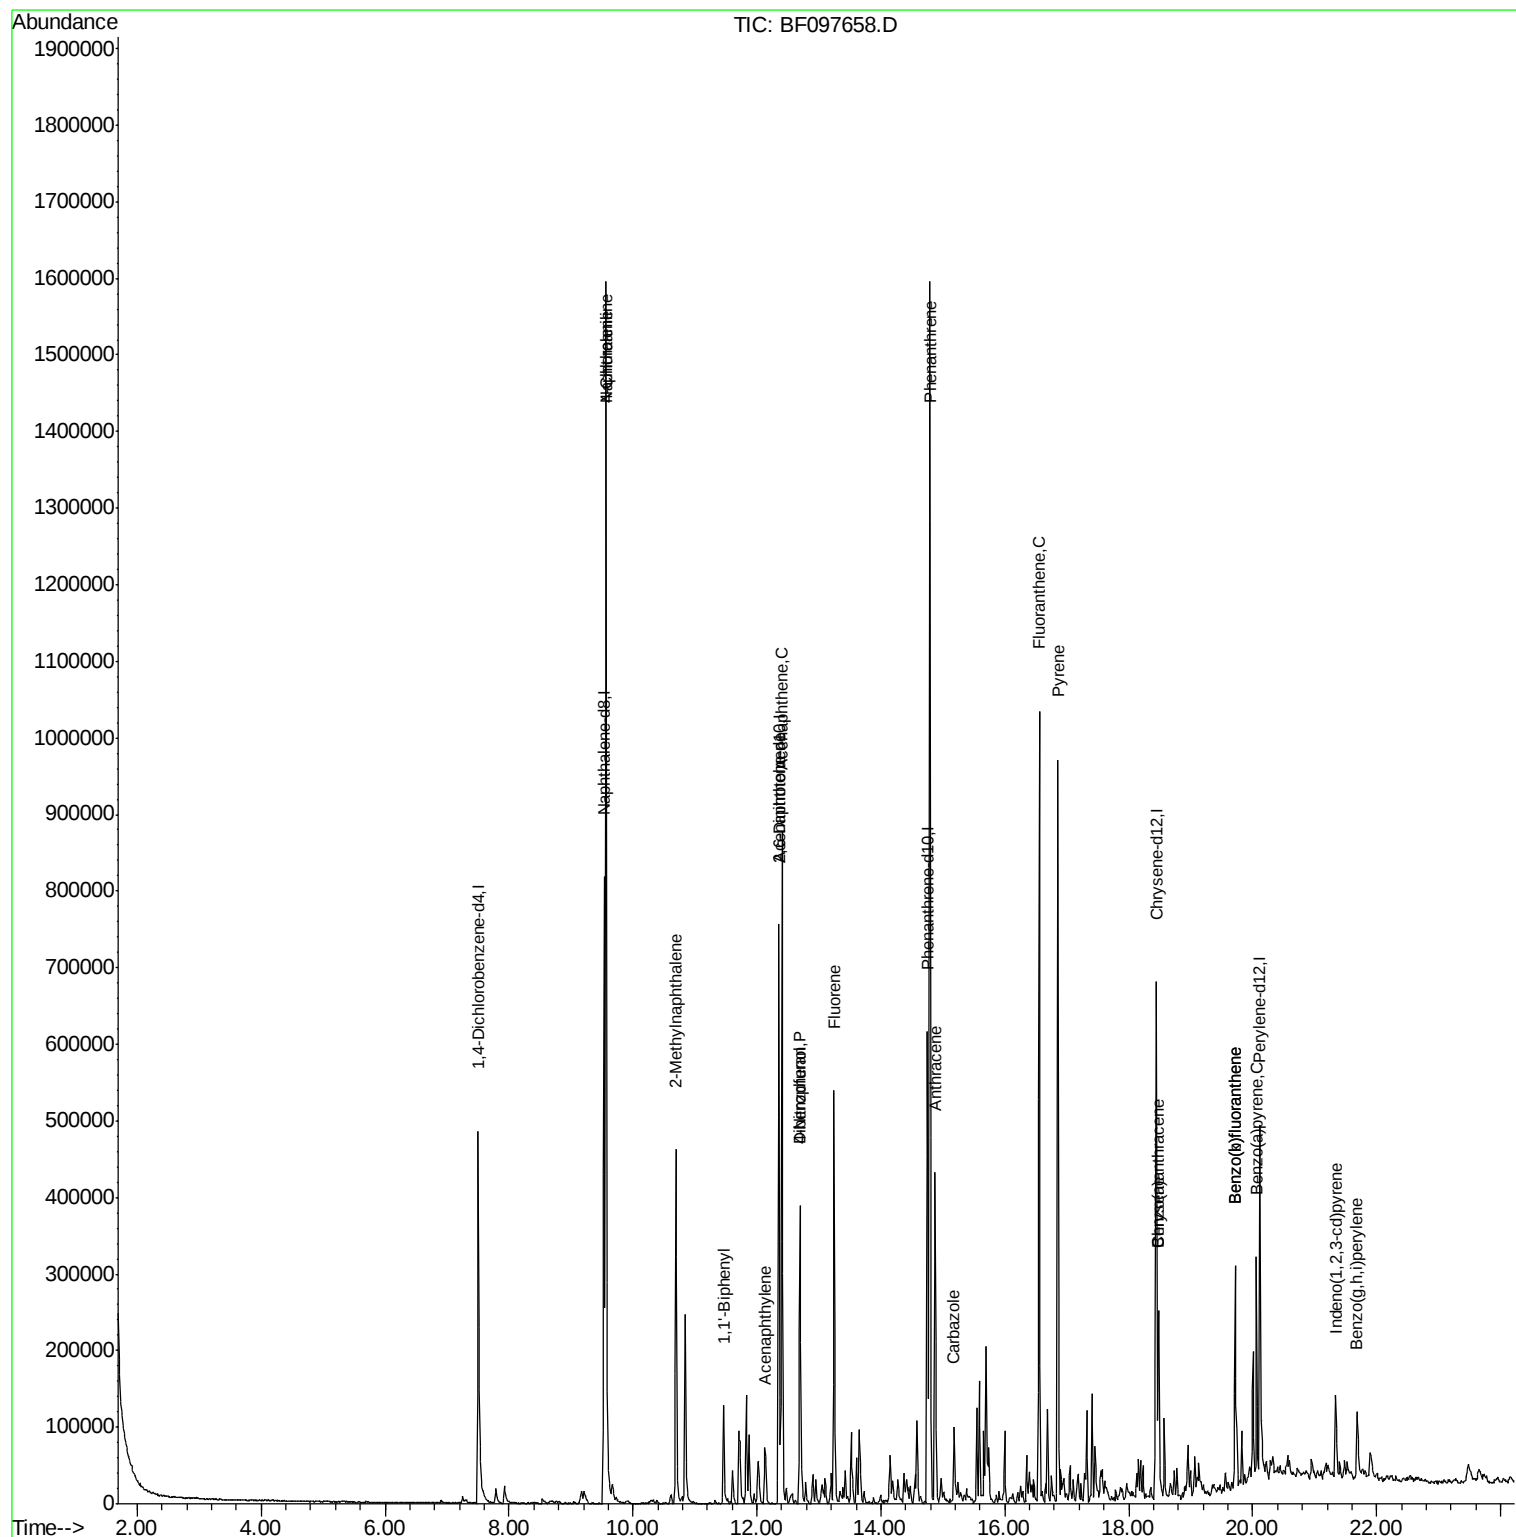

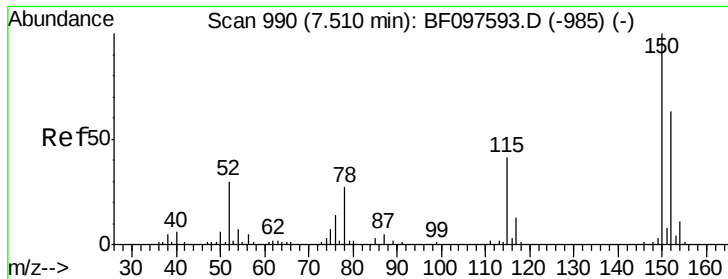


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.50 min Scan# 989
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL

Tot Ion:152 Resp: 126596
Ion Ratio Lower Upper
152 100
150 156.0 126.2 189.2
115 66.7 52.2 78.2

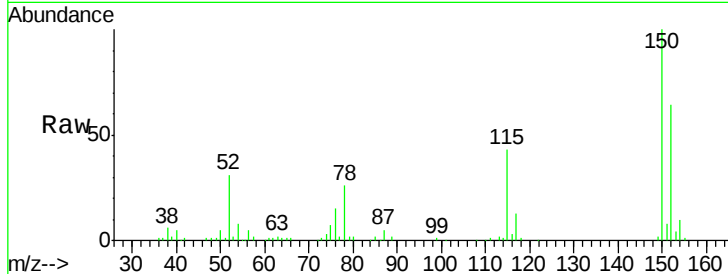

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

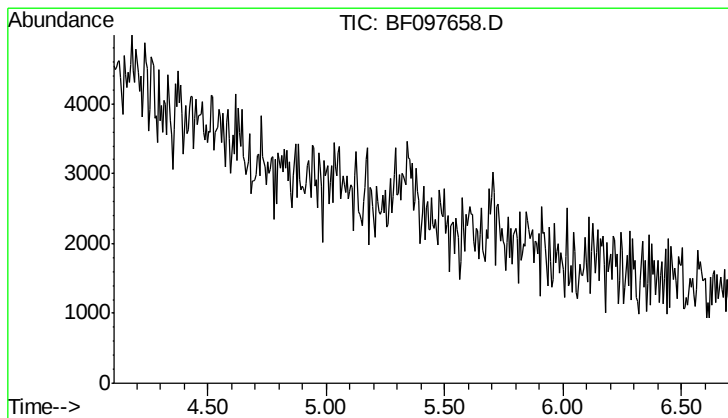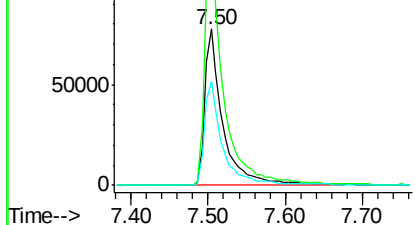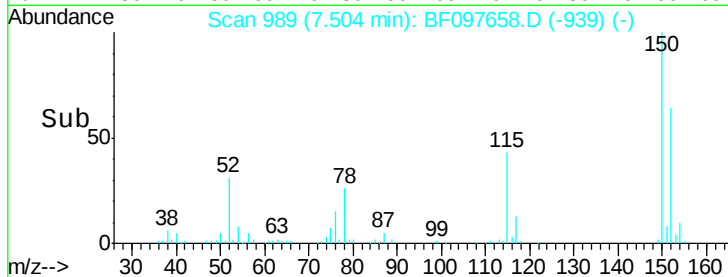



#5

2-Fluorophenol
Concen: 0.00 ng
Expected RT: 5.40 min

Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion: 112
Sig Exp Ratio
112 100
64 57.5
63 29.2

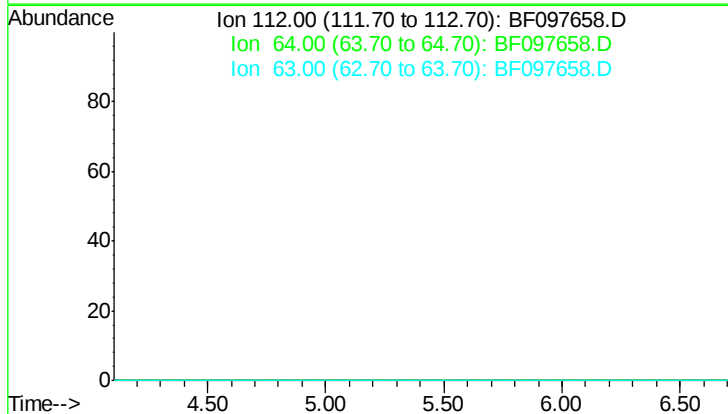

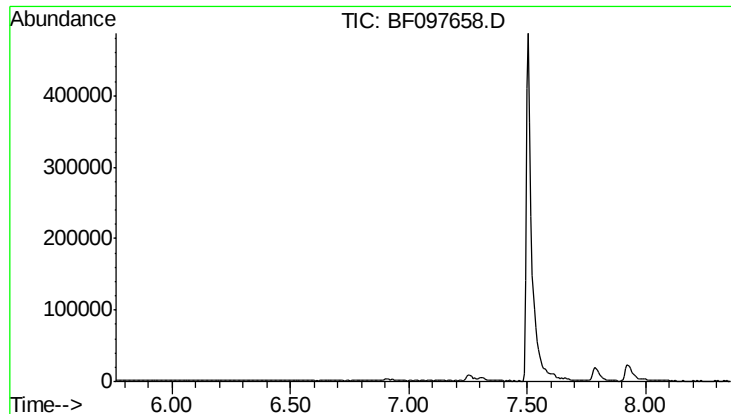

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 7.06 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL



Tot Ion: 99

Sig Exp Ratio

99 100

42 16.9

71 30.6

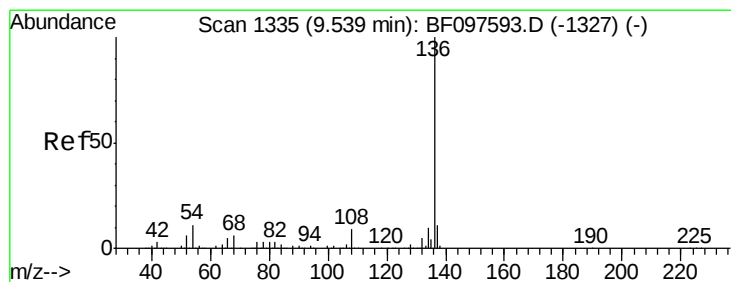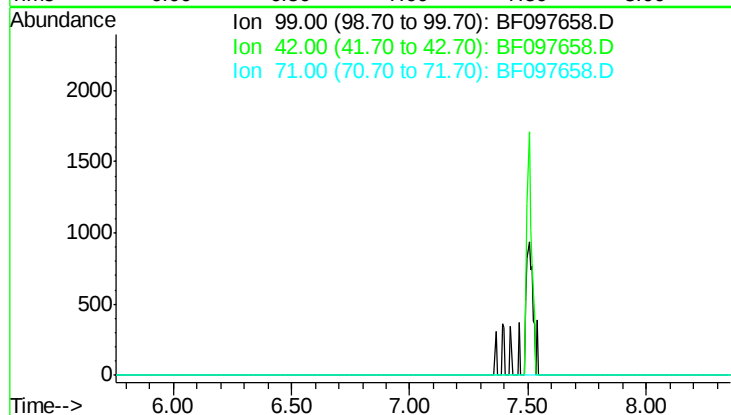

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.53 min Scan# 1334

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Tgt Ion:136 Resp: 497512




Ion Ratio Lower Upper


136 100

137 10.2 8.5 12.7

54 10.6 4.9 7.3#

68 6.3 4.1 6.1#


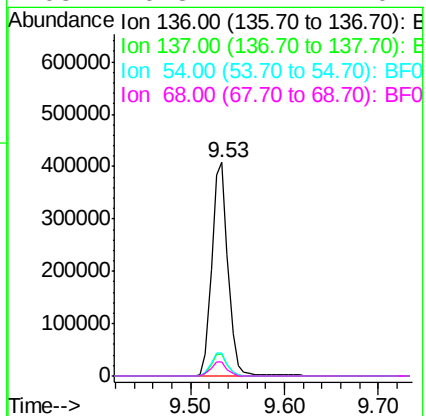

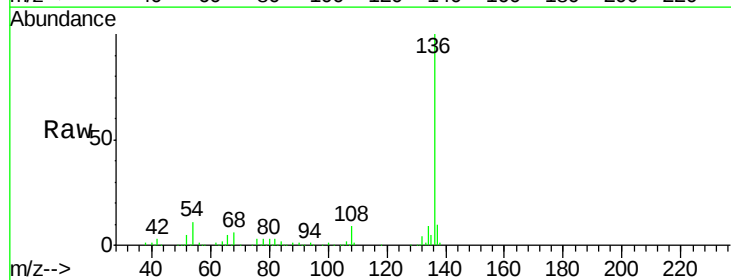




#23
 Nitrobenzene-d5
 Concen: 0.01 ng
 RT: 8.57 min Scan# 1171
 Delta R.T. 0.15 min
 Lab File: BF097658.D
 Acq: 13 Aug 2017 6:14




Instrument :
 BNA_F
 ClientSampleId :
 NYSEG-PH4-ESMI-4BDL


Tot Ion	Ratio	Lower	Upper
82	100		
128	0.0	34.0	51.0#
54	0.0	42.2	63.2#

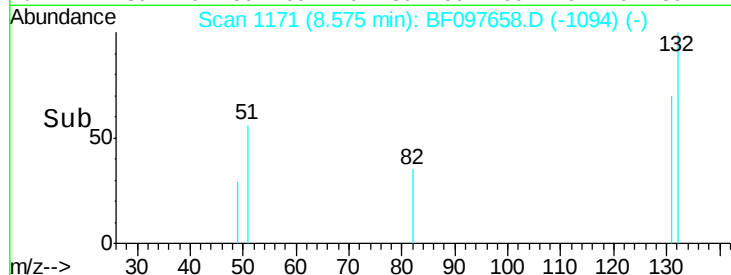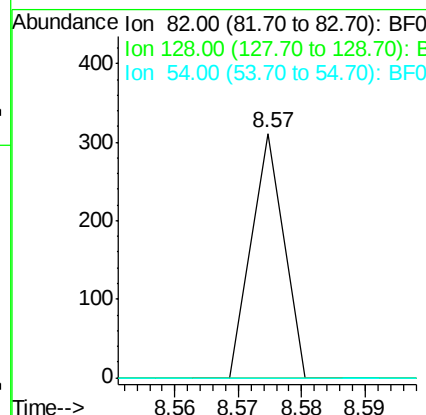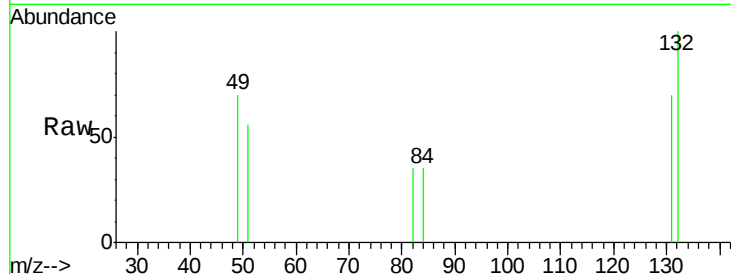

#31
 Naphthalene
 Concen: 41.76 ng
 RT: 9.56 min Scan# 1339
 Delta R.T. -0.01 min
 Lab File: BF097658.D
 Acq: 13 Aug 2017 6:14

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.8	9.0	13.6
127	13.8	10.8	16.2



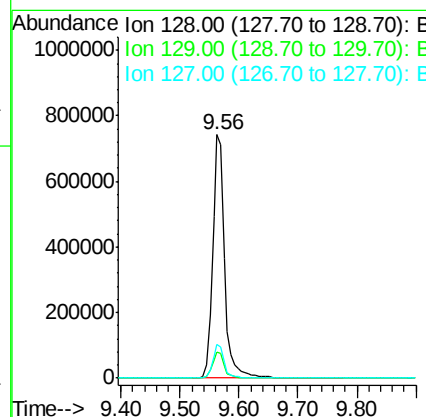





#33
4-Chloroaniline
Concen: 13.30 ng
RT: 9.56 min Scan# 1339
Delta R.T. -0.15 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14




Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL


Tot Ion:	127	Resp:	137325
Ion	Ratio	Lower	Upper
127	100		
129	78.3	26.2	39.2#
65	0.0	27.8	41.8#
92	0.0	16.8	25.2#

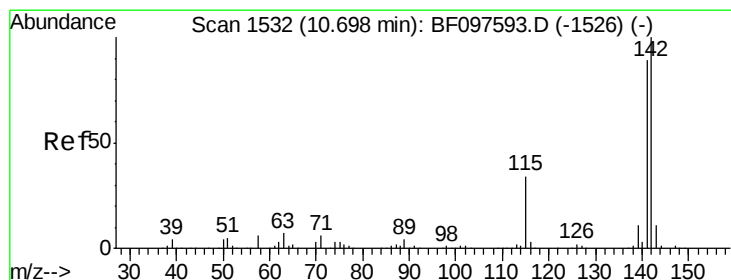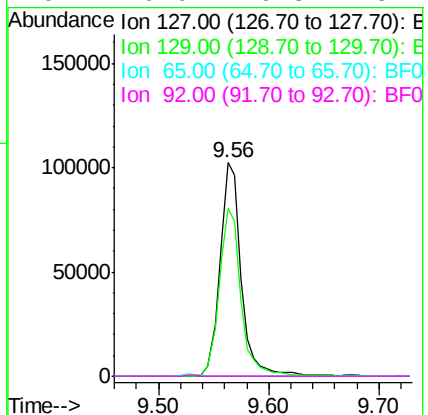

#37
2-Methylnaphthalene
Concen: 12.30 ng
RT: 10.69 min Scan# 1531
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:	142	Resp:	192829
Ion	Ratio	Lower	Upper
142	100		
141	88.3	71.3	106.9
115	31.6	27.1	40.7

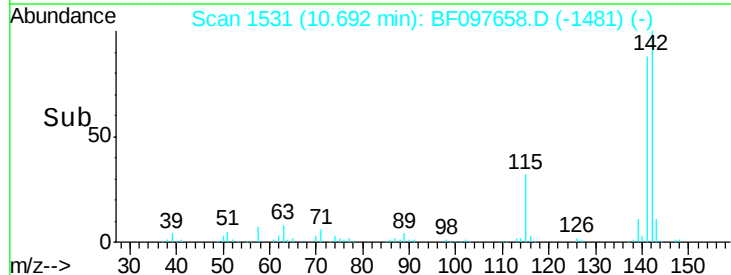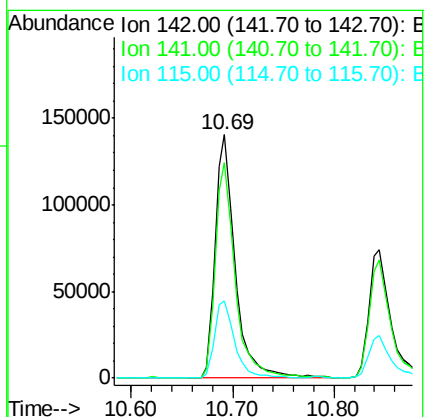



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.35 min Scan# 1813

Delta R.T. -0.02 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL


Tot Ion:164 Resp: 197220

Ion Ratio Lower Upper

164 100

162 104.3 82.6 123.8




160 45.5 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

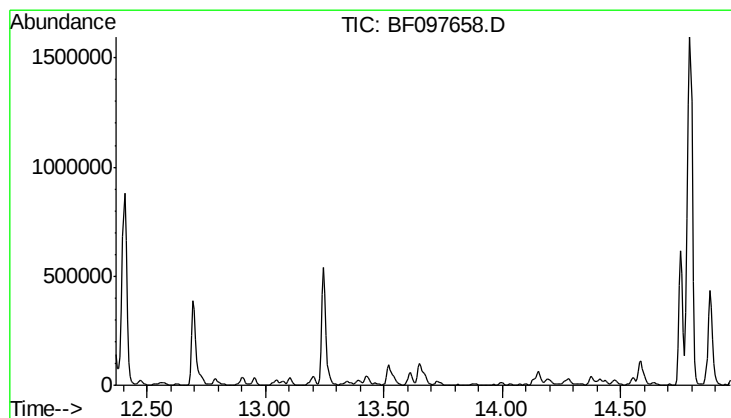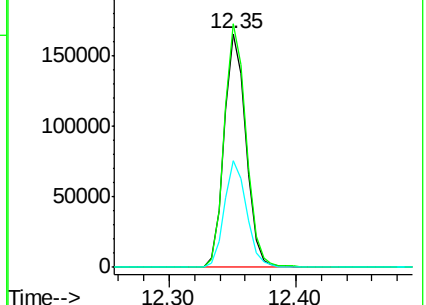

#41

2,4,6-Tribromophenol

Concen: 0.00 ng

Expected RT: 13.66 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Tgt Ion: 330


Sig Exp Ratio

330 100

332 95.8

141 39.3




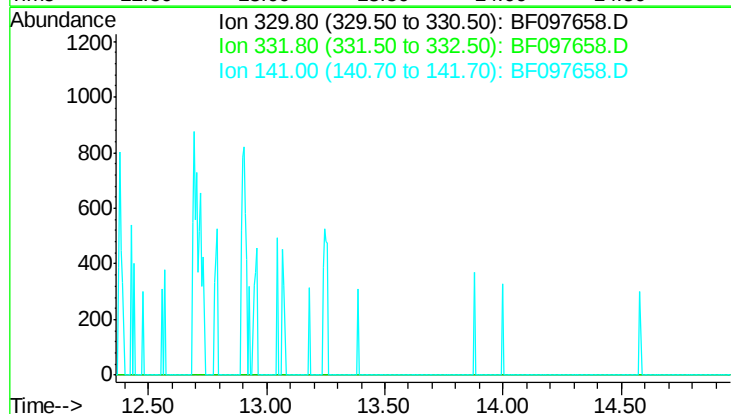


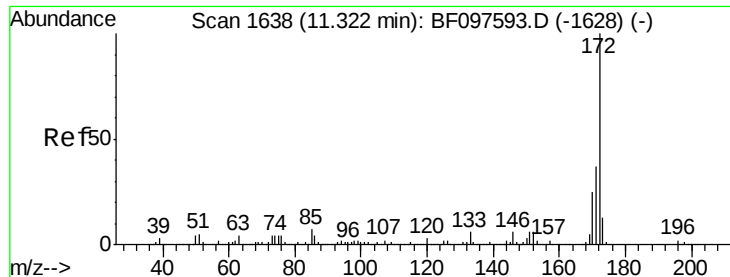

#44
2-Fluorobiphenyl
Concen: 0.26 ng
RT: 11.32 min Scan# 1638
Delta R.T. -0.00 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14




Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL


Tot Ion:172 Resp: 3421
Ion Ratio Lower Upper
172 100
171 41.3 29.6 44.4
170 21.2 19.8 29.8

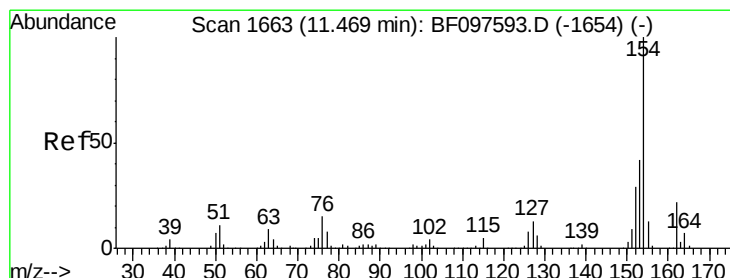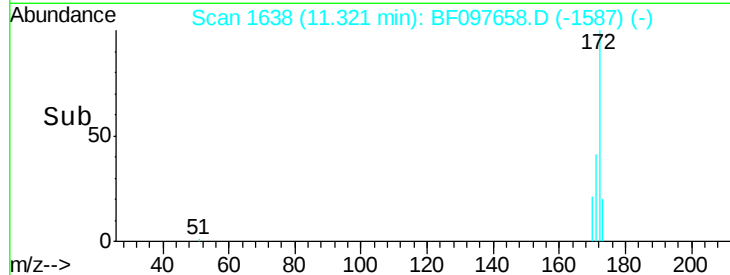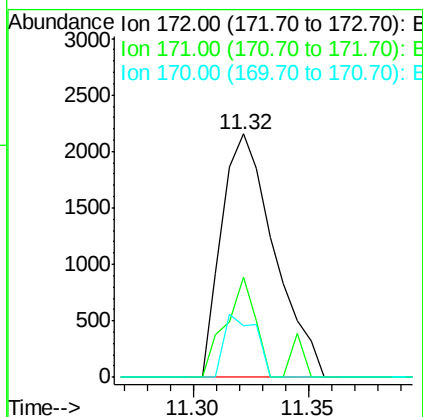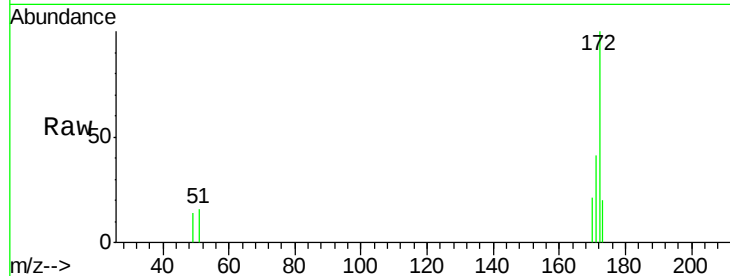

#45
1,1'-Biphenyl
Concen: 3.80 ng
RT: 11.46 min Scan# 1662
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:154 Resp: 64304
Ion Ratio Lower Upper
154 100
153 38.0 21.2 61.2
76 15.6 0.0 29.9

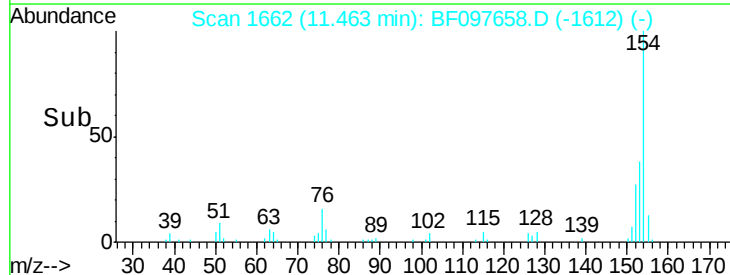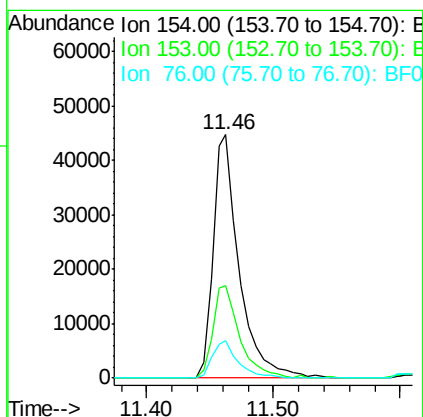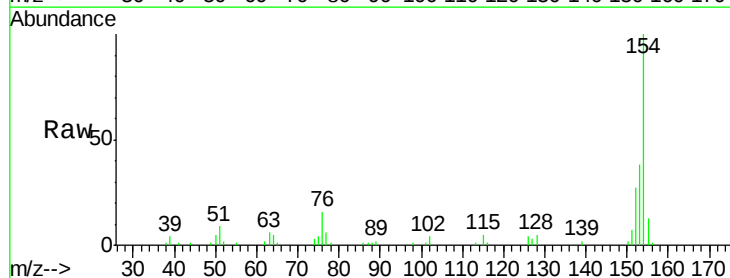



#48

Acenaphthylene

Concen: 2.17 ng

RT: 12.13 min Scan# 1775

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL


Tot Ion:152 Resp: 44729

Ion Ratio Lower Upper

152 100

151 19.7 16.8 25.2




153 14.6 10.8 16.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

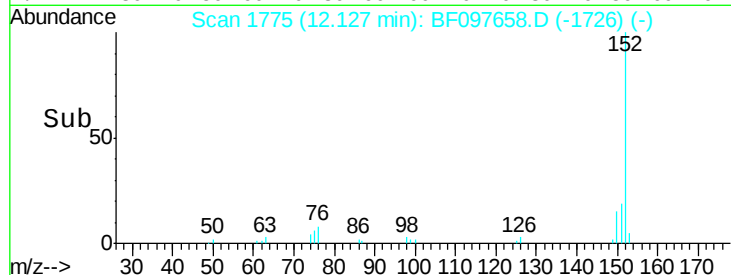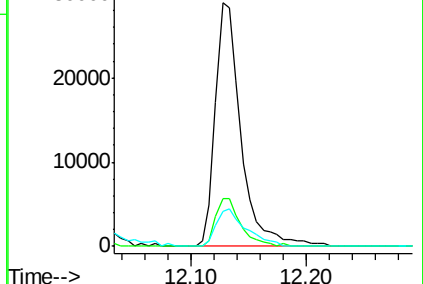

#50

2,6-Dinitrotoluene

Concen: 8.11 ng

RT: 12.35 min Scan# 1813

Delta R.T. 0.24 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Tgt Ion:165 Resp: 25447

Ion Ratio Lower Upper

165 100

63 0.0 34.3 51.5#



89 0.0 37.1 55.7#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0




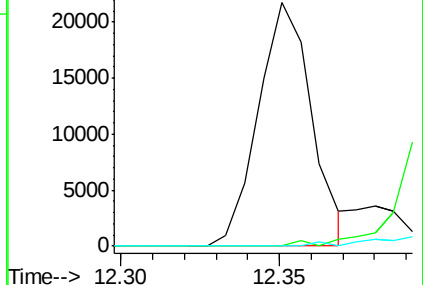




#51
Acenaphthene
Concen: 21.21 ng
RT: 12.40 min Scan# 1822
Delta R.T. -0.02 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14




Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL


Tot Ion:154 Resp: 262512
Ion Ratio Lower Upper
154 100
153 111.8 90.5 135.7
152 54.9 43.6 65.4

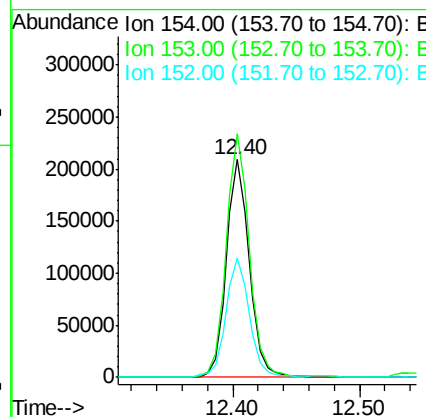

#54
Dibenzofuran
Concen: 12.68 ng
RT: 12.69 min Scan# 1871
Delta R.T. -0.02 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:168 Resp: 219681
Ion Ratio Lower Upper
168 100
139 40.7 30.6 45.8
169 13.4 10.8 16.2



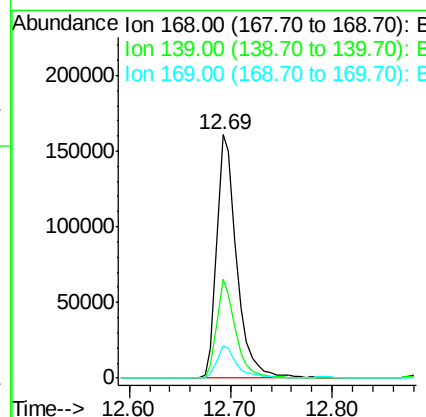





#55
4-Nitrophenol
Concen: 53.85 ng
RT: 12.69 min Scan# 1871
Delta R.T. -0.08 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14




Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL


Tot Ion:139 Resp: 84275
Ion Ratio Lower Upper
139 100
109 1.0 34.1 74.1#
65 1.4 31.4 71.4#

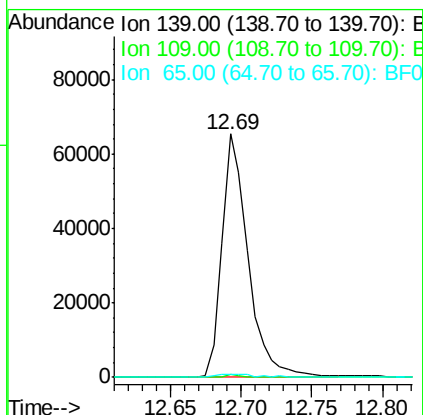

#57
Fluorene
Concen: 13.87 ng
RT: 13.24 min Scan# 1965
Delta R.T. -0.02 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:166 Resp: 197709
Ion Ratio Lower Upper
166 100
165 99.1 78.8 118.2
167 13.4 10.6 16.0

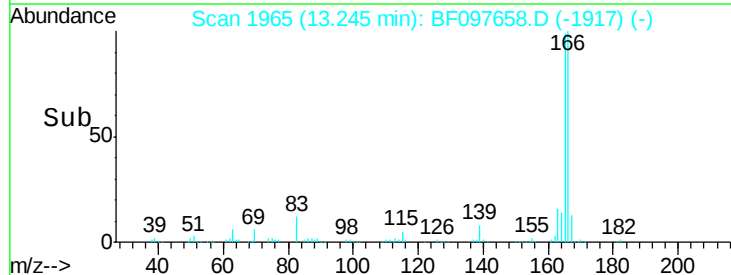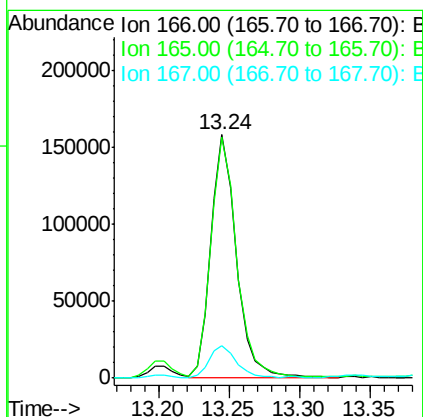



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.75 min Scan# 2221

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL


Tot Ion:188 Resp: 281694

Ion Ratio Lower Upper

188 100

94 13.4 9.4 14.2




80 13.9 10.2 15.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

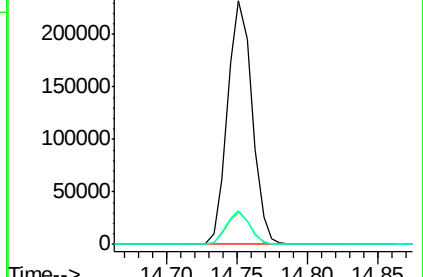

#70

Phenanthrene

Concen: 52.48 ng

RT: 14.79 min Scan# 2228

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Tgt Ion:178 Resp: 851538

Ion Ratio Lower Upper

178 100

176 19.9 16.2 24.4



179 15.4 12.6 19.0




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E




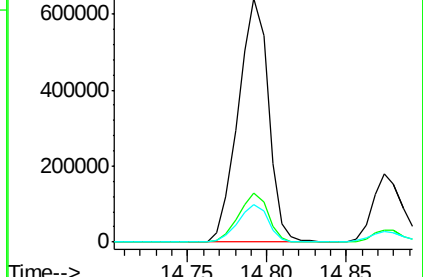




#71
 Anthracene
 Concen: 14.60 ng
 RT: 14.87 min Scan# 2242
 Delta R.T. -0.01 min
 Lab File: BF097658.D
 Acq: 13 Aug 2017 6:14




Instrument :
 BNA_F
 ClientSampleId :
 NYSEG-PH4-ESMI-4BDL


Tot Ion:178 Resp: 242340
 Ion Ratio Lower Upper
 178 100
 176 18.5 15.8 23.8
 179 15.8 12.7 19.1

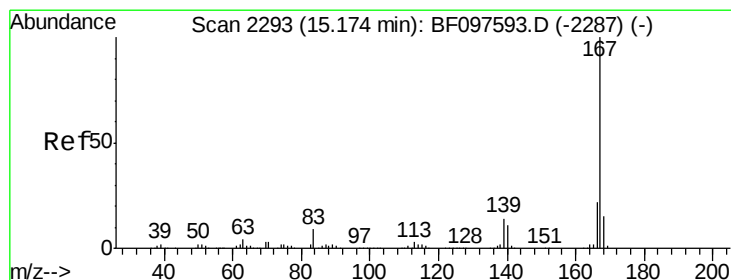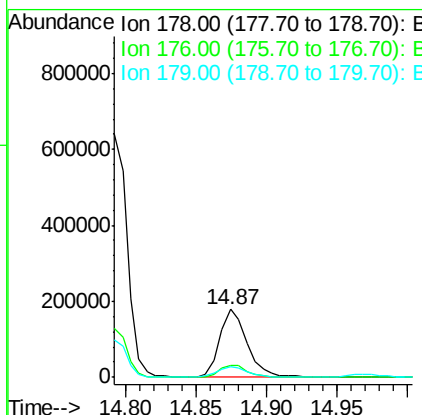

#72
 Carbazole
 Concen: 3.82 ng
 RT: 15.18 min Scan# 2294
 Delta R.T. 0.01 min
 Lab File: BF097658.D
 Acq: 13 Aug 2017 6:14

Tgt Ion:167 Resp: 60312
 Ion Ratio Lower Upper
 167 100
 166 21.1 18.1 27.1
 139 15.2 11.7 17.5

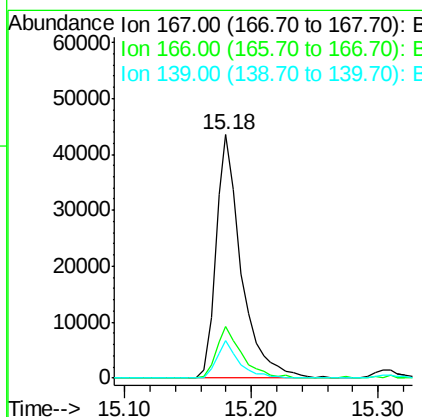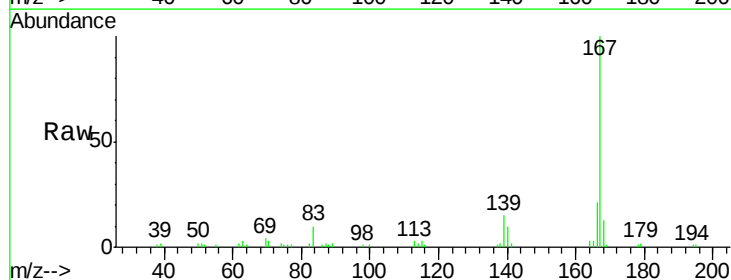



#74

Fluoranthene

Concen: 35.83 ng

RT: 16.56 min Scan# 2528

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL


Tot Ion:202 Resp: 525352

Ion Ratio Lower Upper

202 100

101 13.9 0.0 33.2




203 16.9 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

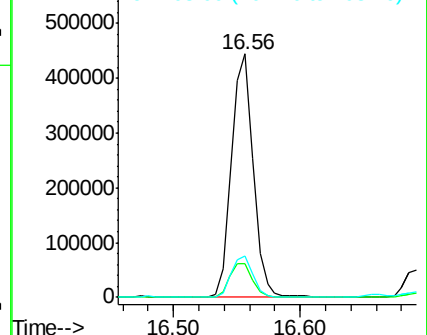

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.45 min Scan# 2850

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Tgt Ion:240 Resp: 193383

Ion Ratio Lower Upper

240 100

120 15.4 5.8 8.8#



236 25.6 20.5 30.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

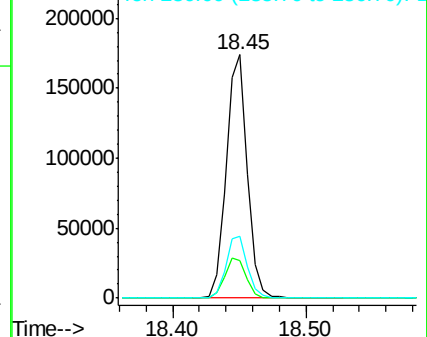



#77

Pvrene

Concen: 26.87 ng

RT: 16.86 min Scan# 2579

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14

Instrument :

BNA_F

ClientSampleId :

NYSEG-PH4-ESMI-4BDL


Tot Ion:202 Resp: 429712

Ion Ratio Lower Upper

202 100

200 20.9 17.6 26.4




203 20.3 14.4 21.6



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

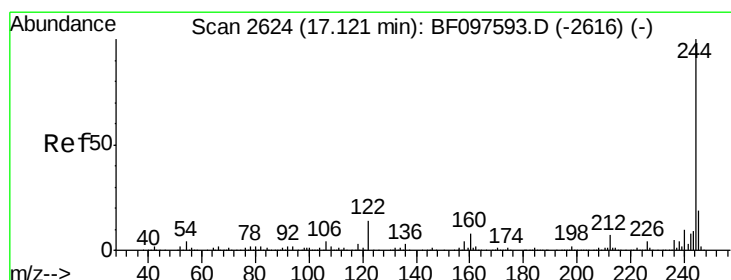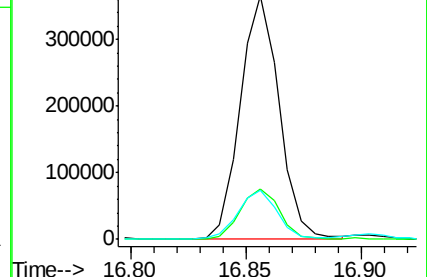

#78

Terphenyl-d14

Concen: 0.19 ng

RT: 17.10 min Scan# 2621

Delta R.T. -0.02 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Tgt Ion:244 Resp: 1784

Ion Ratio Lower Upper

244 100

212 0.0 6.0 9.0#



122 18.8 10.3 15.5#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

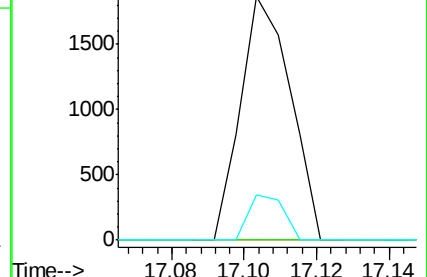







#80
Benzo(a)anthracene
Concen: 10.19 ng
RT: 18.48 min Scan# 2855
Delta R.T. 0.03 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL

Tot Ion:228 Resp: 115115
Ion Ratio Lower Upper
228 100
226 30.5 22.6 33.8
229 19.8 16.3 24.5




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

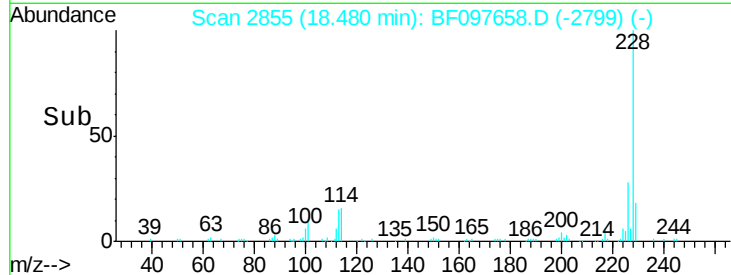
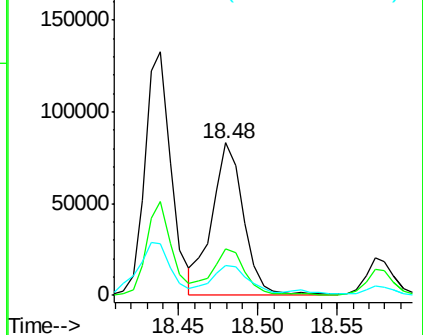



#82
Chrysene
Concen: 10.25 ng
RT: 18.48 min Scan# 2855
Delta R.T. -0.02 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:228 Resp: 115115
Ion Ratio Lower Upper
228 100
226 30.5 24.9 37.3
229 19.8 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E




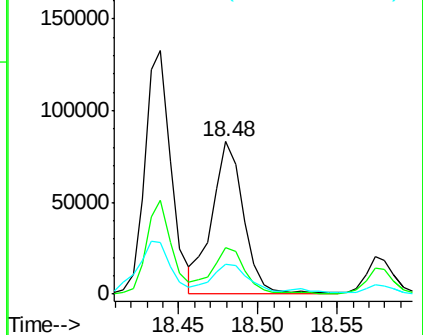




#85
Indeno(1,2,3-cd)pyrene
Concen: 7.01 ng
RT: 21.34 min Scan# 3341
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14




Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL


Tot Ion	Ratio	Lower	Upper
276	100		
138	33.8	27.8	41.6
277	24.7	20.2	30.4

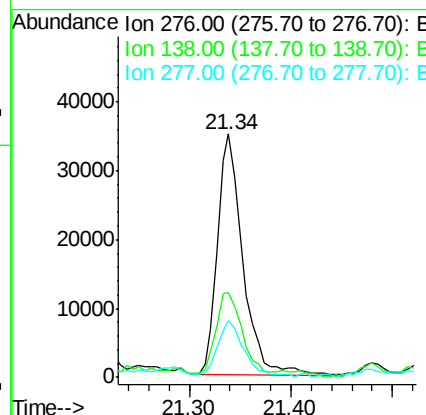

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.12 min Scan# 3133
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.5	29.3
265	20.7	17.2	25.8

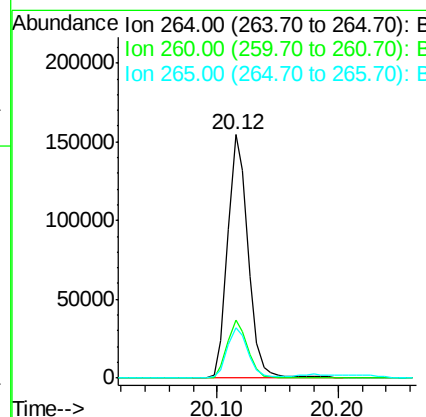



#87

Benzo(b)fluoranthene

Concen: 18.31 ng

RT: 19.72 min Scan# 3065

Delta R.T. -0.01 min

Lab File: BF097658.D

Acq: 13 Aug 2017 6:14


Instrument :

BNA_F




ClientSampleId :

NYSEG-PH4-ESMI-4BDL

Tot Ion:252	Resp:	199315
Ion Ratio	Lower	Upper
252	100	
253	20.6	18.1 27.1
125	16.2	9.8 14.8#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

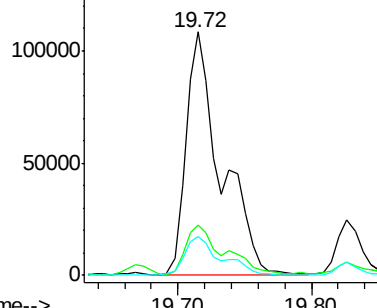

#88

Benzo(k)fluoranthene

Concen: 18.18 ng


RT: 19.72 min Scan# 3065

Delta R.T. -0.04 min



Lab File: BF097658.D


Acq: 13 Aug 2017 6:14

Tgt Ion:252	Resp:	199315
Ion Ratio	Lower	Upper
252	100	
253	20.6	18.4 27.6
125	16.2	13.1 19.7



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E




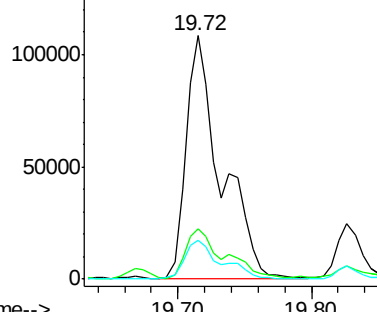




#89
Benzo(a)pyrene
Concen: 12.37 ng
RT: 20.06 min Scan# 3124
Delta R.T. -0.01 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Instrument :
BNA_F
ClientSampleId :
NYSEG-PH4-ESMI-4BDL

Tot Ion:252	Resp:	123616
Ion Ratio	Lower	Upper
252	100	
253	22.0	17.5 26.3
125	15.7	11.0 16.4

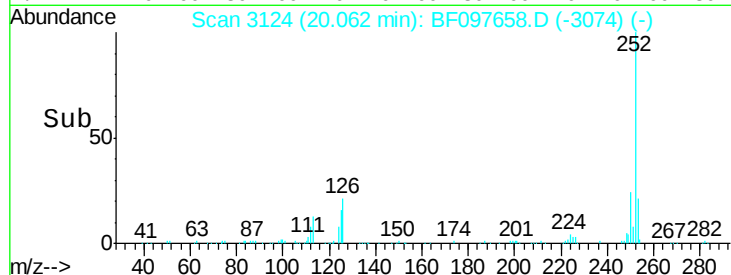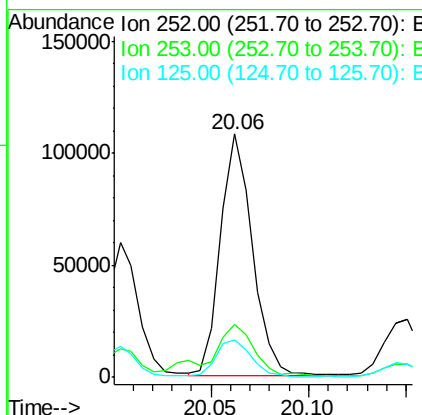

#91
Benzo(g,h,i)perylene
Concen: 7.33 ng
RT: 21.69 min Scan# 3400
Delta R.T. 0.00 min
Lab File: BF097658.D
Acq: 13 Aug 2017 6:14

Tgt Ion:276	Resp:	57527
Ion Ratio	Lower	Upper
276	100	
277	26.6	18.6 28.0
138	42.1	25.4 38.0#

