
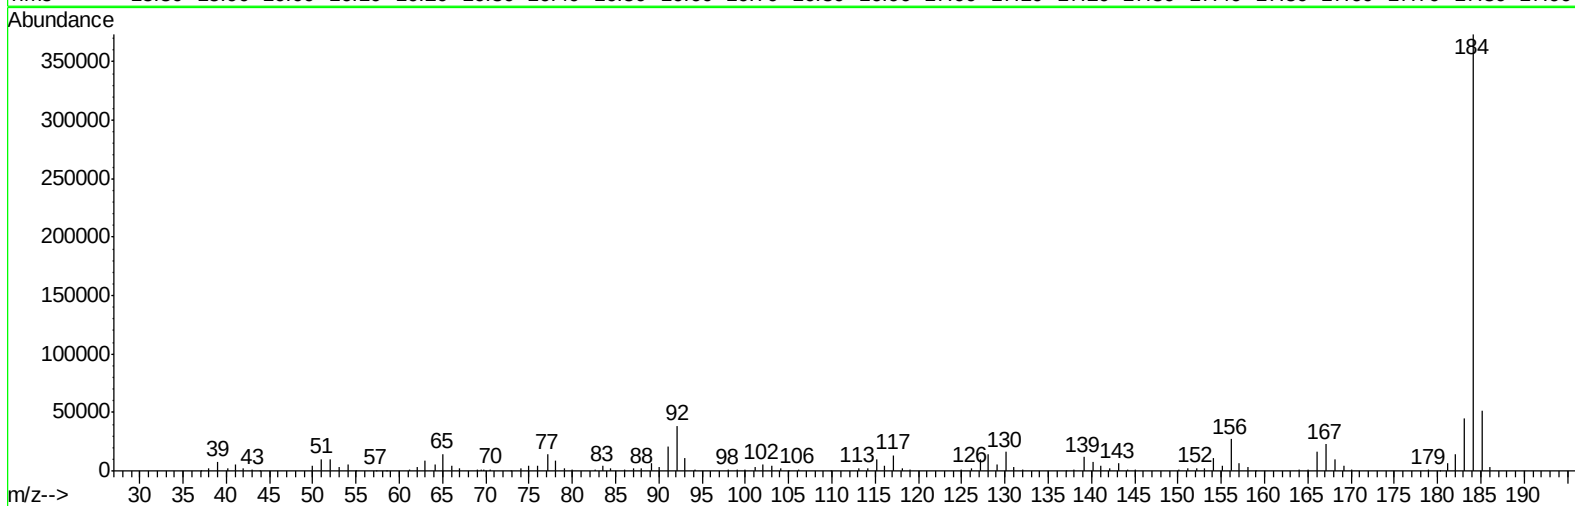


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
Data File : BF097632.D
Acq On : 12 Aug 2017 13:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 09:13:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

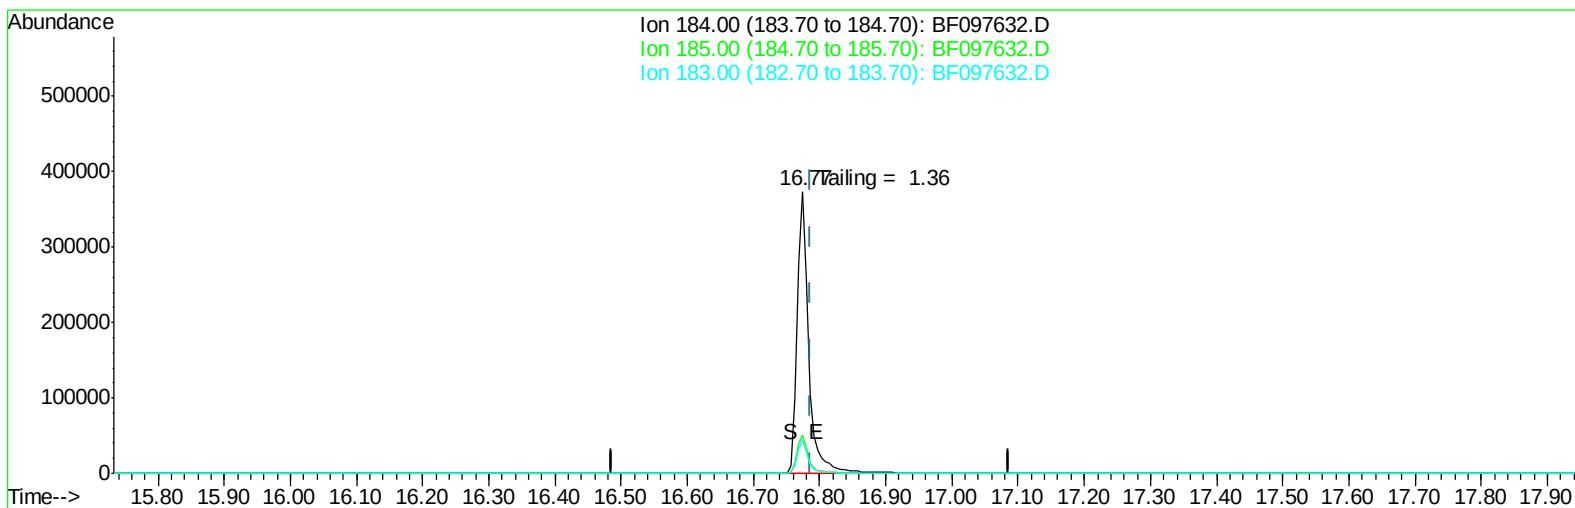

TIC: BF097632.D

(76) Benzidine



16.774min (-0.012) 0.00ng

response 461465

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.87#
183.00	12.20	11.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
Data File : BF097632.D
Acq On : 12 Aug 2017 13:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 09:13:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

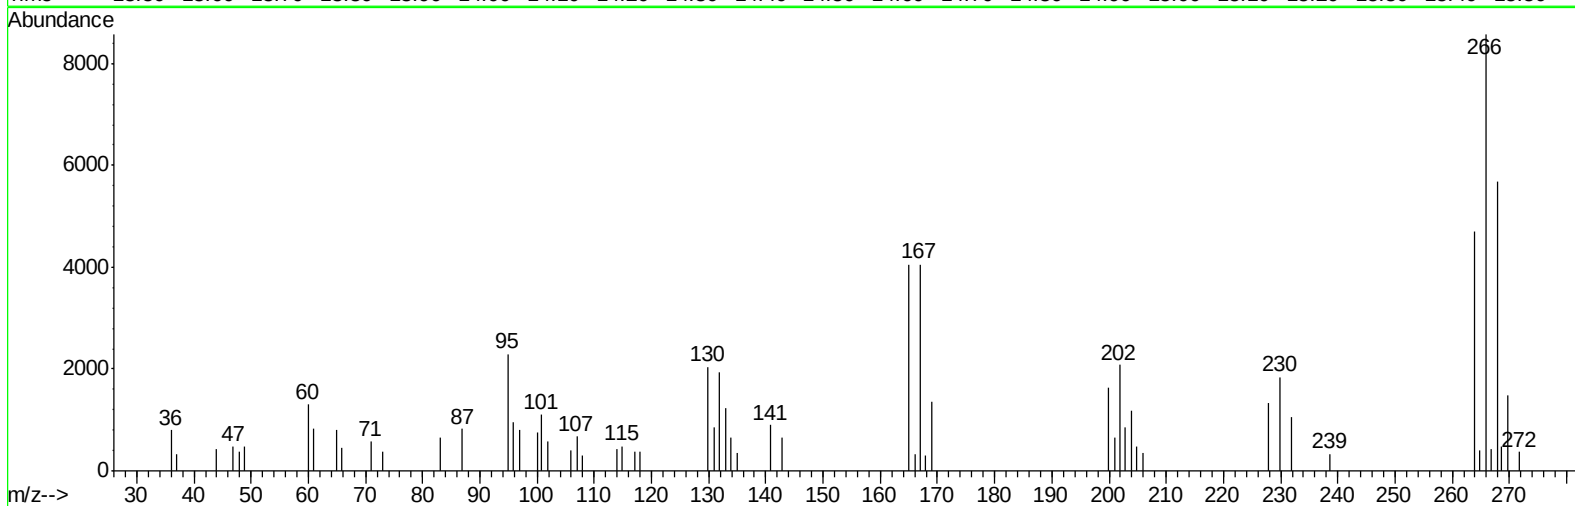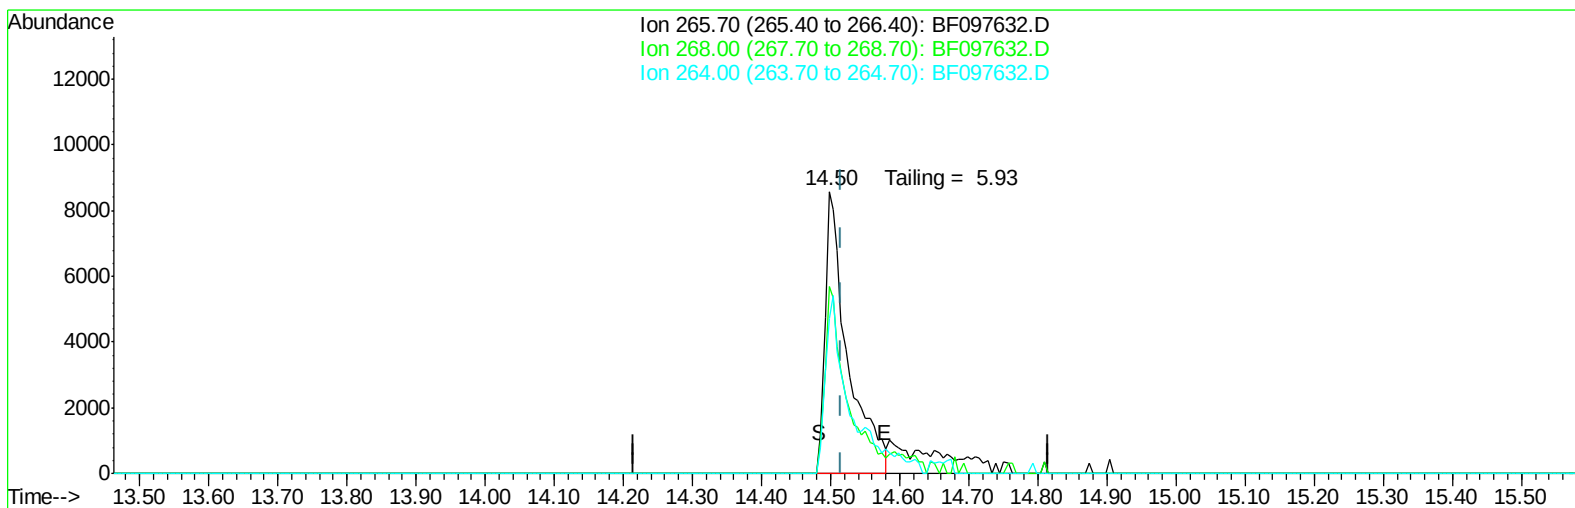

TIC: BF097632.D

(69) Pentachlorophenol (C)

14.498min (-0.017) 0.00ng

response 19331

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	71.83
264.00	64.60	54.93
0.00	0.00	0.00