
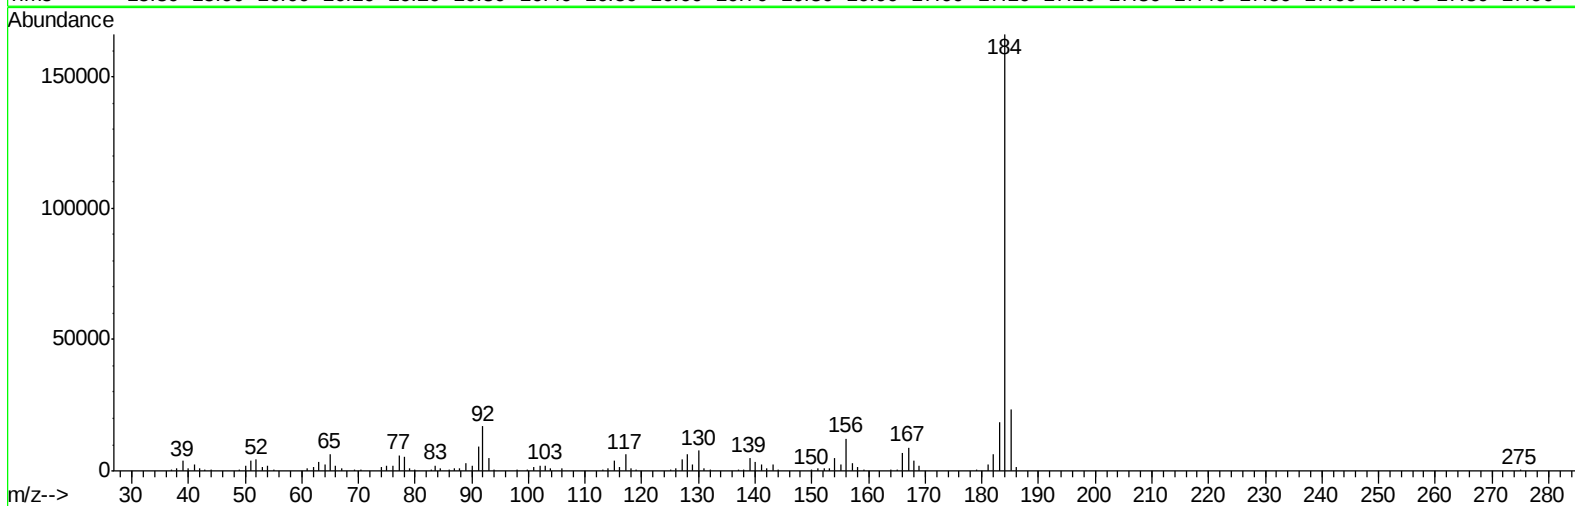


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
Data File : BF097653.D
Acq On : 13 Aug 2017 2:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 09:14:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

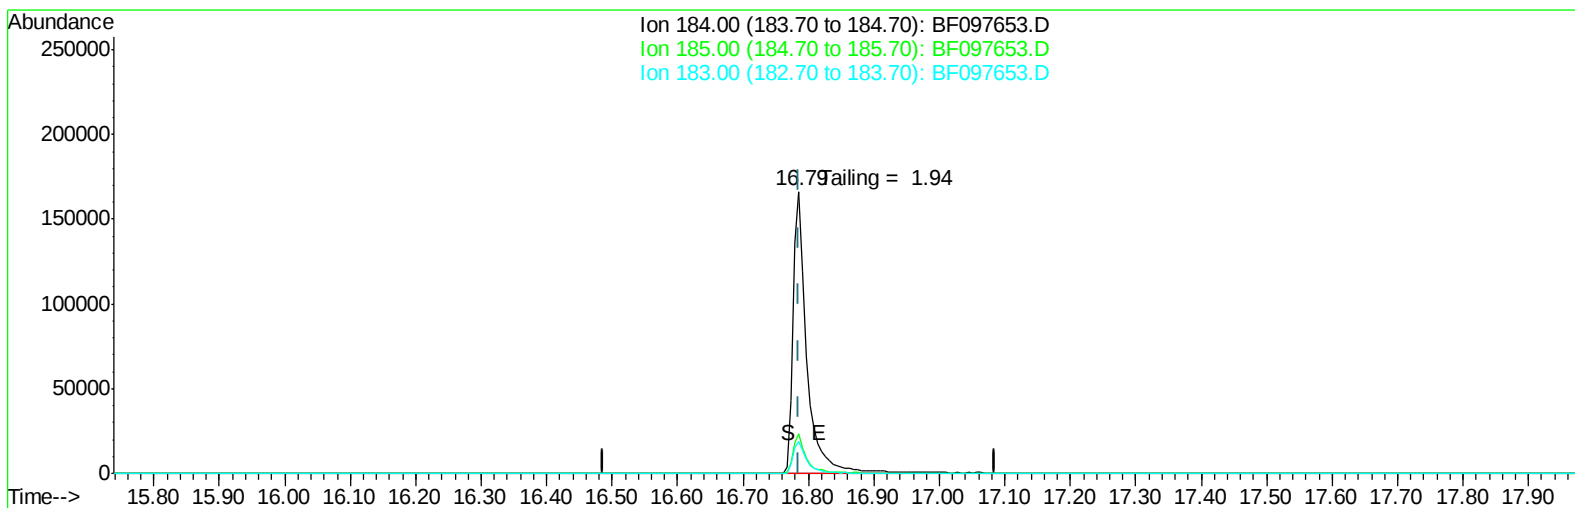

TIC: BF097653.D

(76) Benzidine



16.786min (-0.000) 0.00ng

response 245365

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.97#
183.00	12.20	11.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081217\
Data File : BF097653.D
Acq On : 13 Aug 2017 2:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 09:14:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 15:55:57 2017
Response via : Initial Calibration

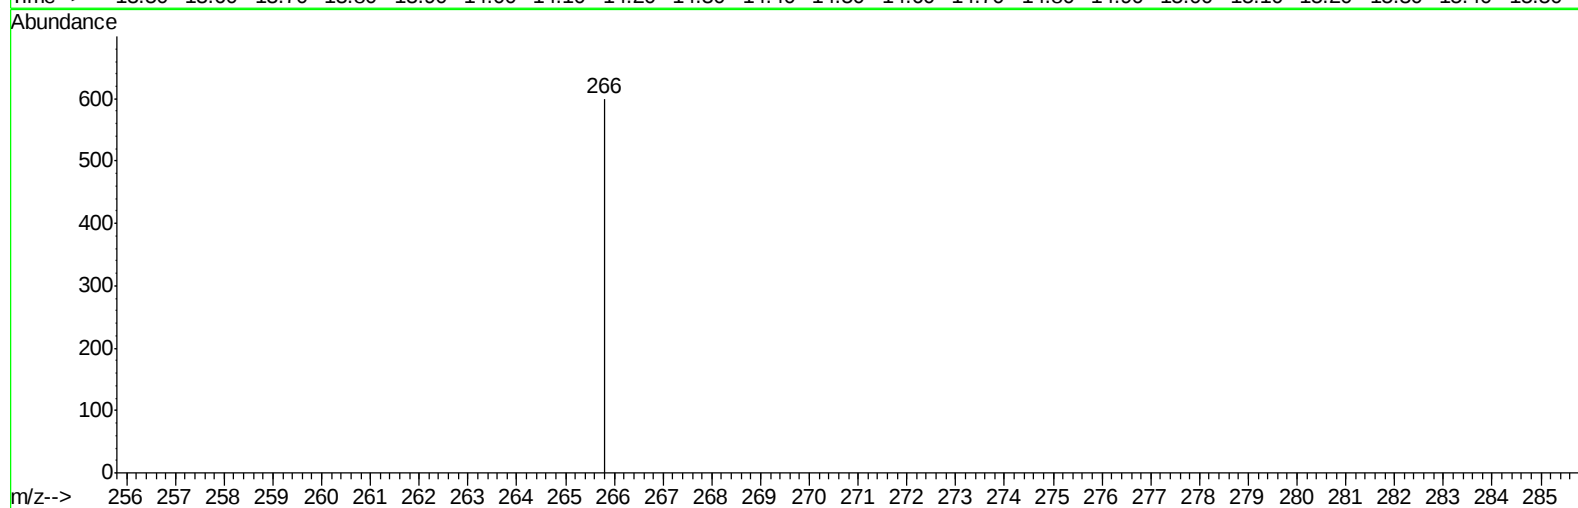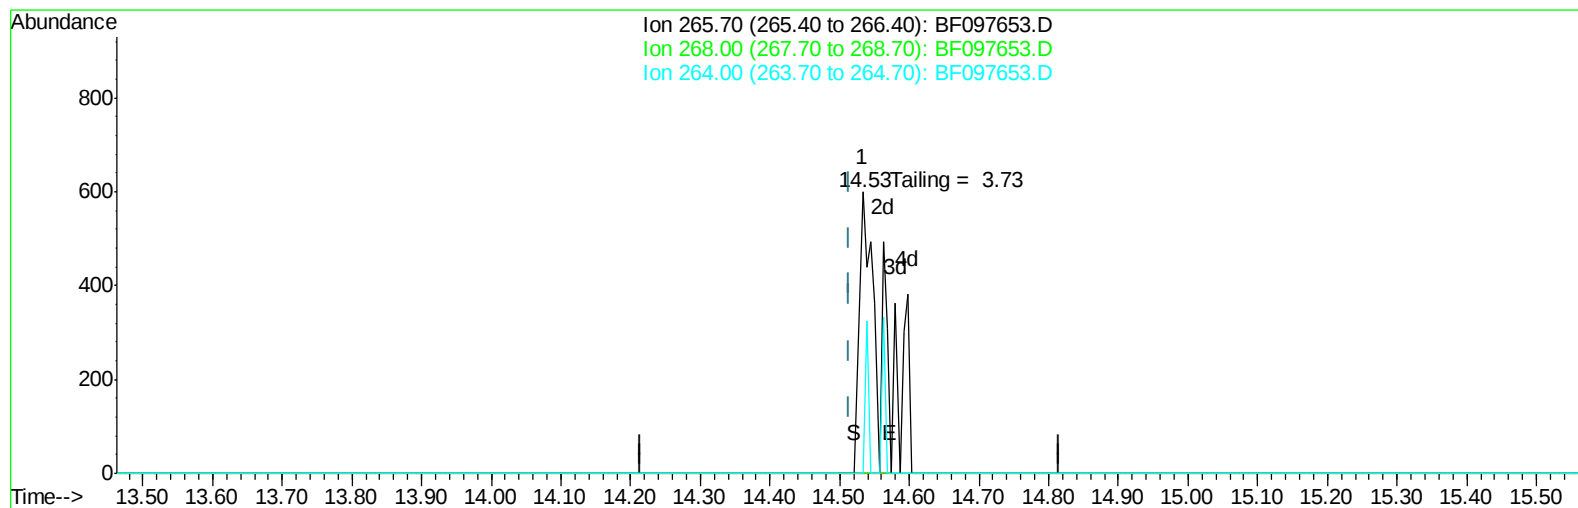

TIC: BF097653.D

(69) Pentachlorophenol (C)

14.533min (+0.018) 0.00ng

response 790

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	0.00#
264.00	64.60	0.00#
0.00	0.00	0.00