


Data Path : Z:\HPCHEM1\BNA F\Data\BF081217\
 Data File : BF097632.D
 Acq On : 12 Aug 2017 13:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 11 15:55:57 2017

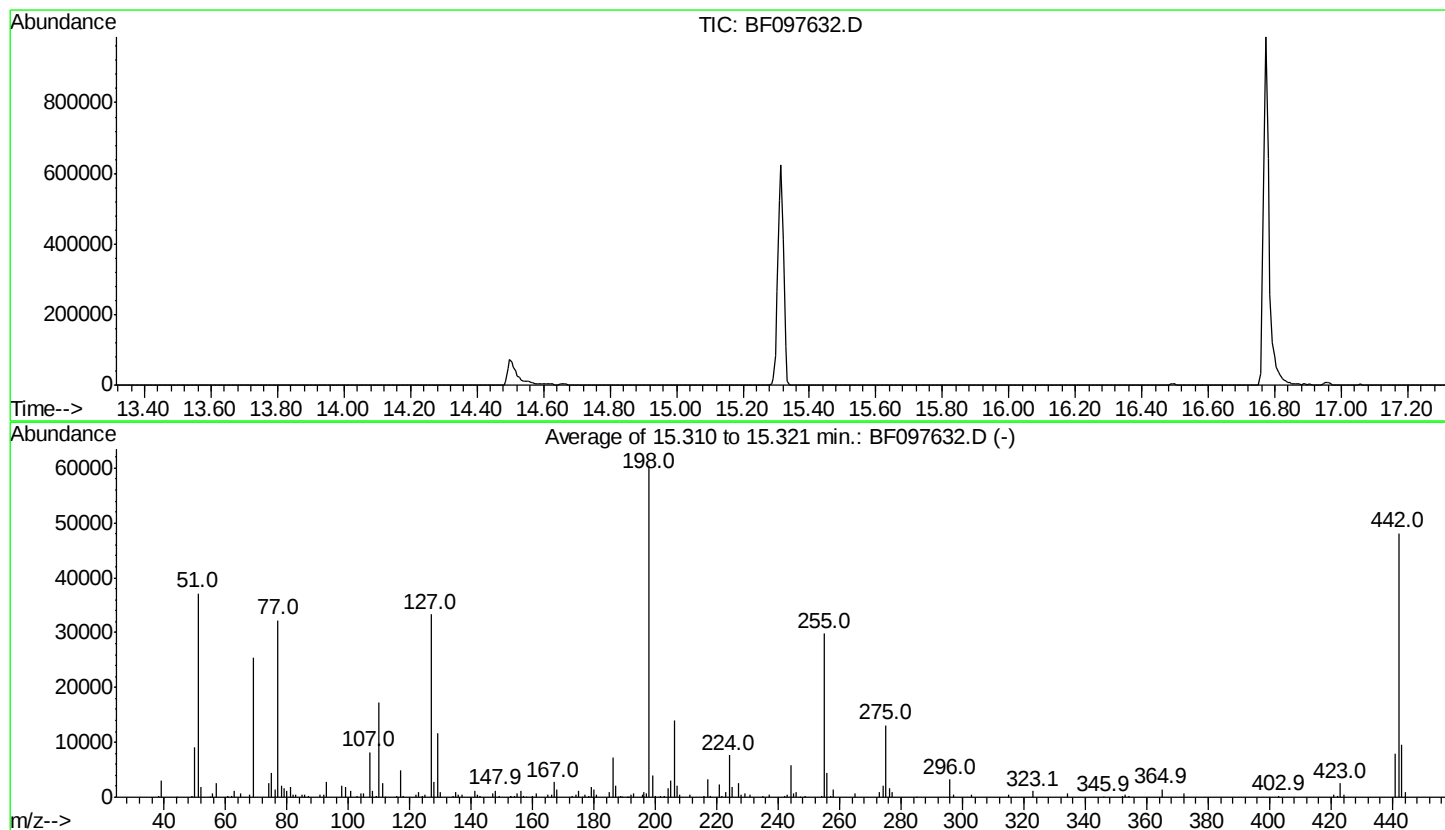

AutoFind: Scans 2316, 2317, 2318; Background Corrected with Scan 2309

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.4	37101	PASS
68	69	0.00	2	1.7	430	PASS
69	198	0.00	100	42.1	25466	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.2	33357	PASS
197	198	0.00	2	1.0	599	PASS
198	198	100	100	100.0	60442	PASS
199	198	5	9	6.7	4037	PASS
275	198	10	60	21.7	13101	PASS
365	198	1	100	2.4	1441	PASS
441	442	0.01	24	16.5	7961	PASS
442	198	50	100	79.6	48104	PASS
443	442	15	24	19.9	9576	PASS