


Data Path : Z:\HPCHEM1\BNA F\Data\BF081217\
 Data File : BF097653.D
 Acq On : 13 Aug 2017 2:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 11 15:55:57 2017

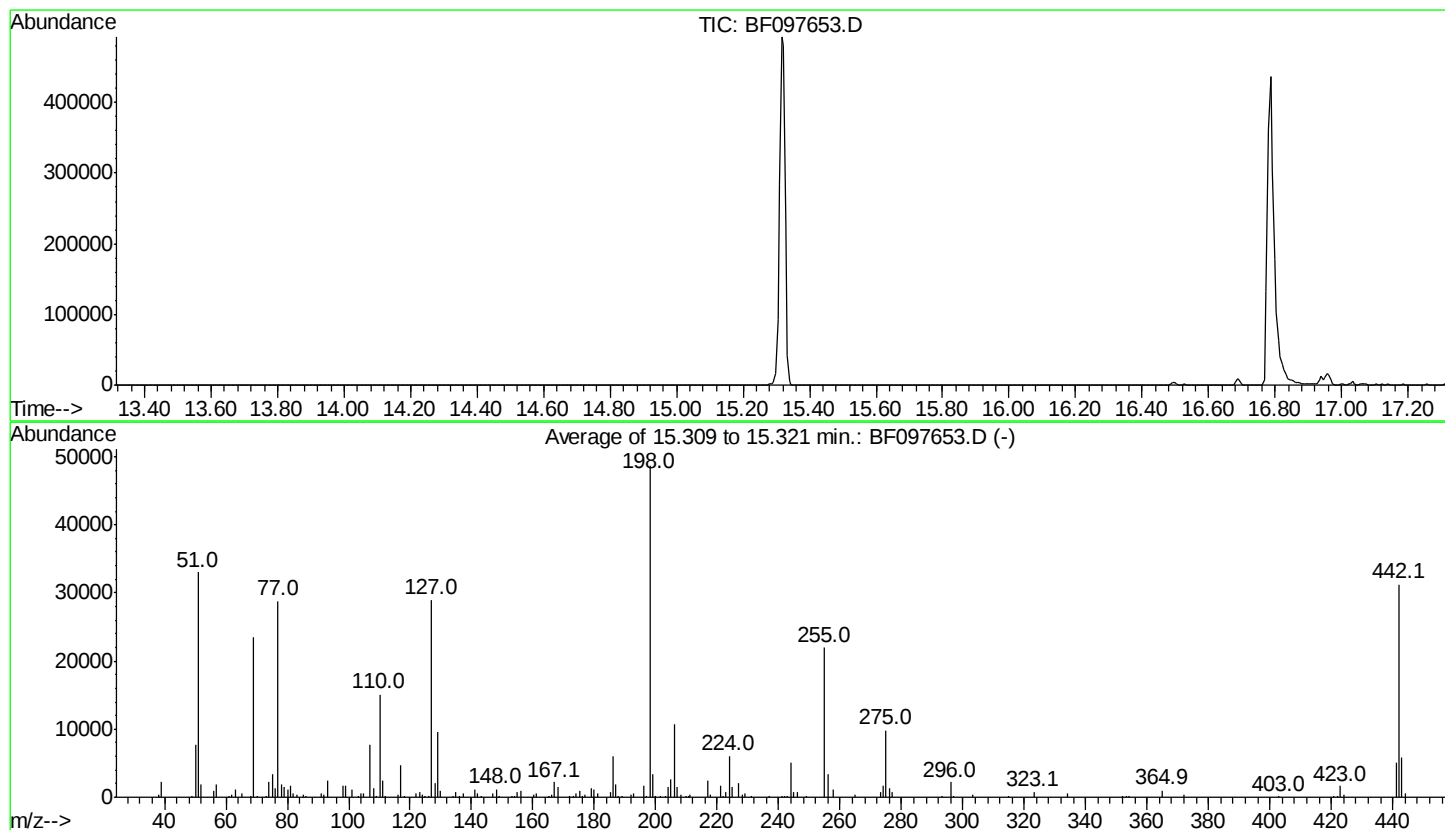

AutoFind: Scans 2316, 2317, 2318; Background Corrected with Scan 2310

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.9	33056	PASS
68	69	0.00	2	0.6	141	PASS
69	198	0.00	100	48.1	23405	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	59.6	28992	PASS
197	198	0.00	2	0.5	245	PASS
198	198	100	100	100.0	48685	PASS
199	198	5	9	6.9	3342	PASS
275	198	10	60	20.1	9809	PASS
365	198	1	100	2.0	970	PASS
441	442	0.01	24	16.3	5081	PASS
442	198	50	100	64.2	31253	PASS
443	442	15	24	18.4	5753	PASS