

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
 Data File : BF138929.D
 Acq On : 12 Aug 2024 12:41
 Operator : RC/JU
 Sample : P3520-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-CF-10-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	499	504	521	rVB	54413	85424	12.10%	1.654%
2	5.469	569	574	599	rBV	420065	597503	84.60%	11.571%
3	6.481	741	746	762	rBV	453291	629394	89.12%	12.188%
4	6.839	802	807	814	rBB	214885	261702	37.05%	5.068%
5	7.404	898	903	919	rBV	321406	408476	57.84%	7.910%
6	8.122	1020	1025	1043	rBV	264210	337222	47.75%	6.530%
7	9.192	1202	1207	1221	rBV	582424	706256	100.00%	13.677%
8	9.874	1318	1323	1333	rVB	298429	379454	53.73%	7.348%
9	9.963	1333	1338	1344	rVB	10805	15201	2.15%	0.294%
10	10.663	1452	1457	1472	rBV	298098	396306	56.11%	7.674%
11	11.357	1570	1575	1590	rBV	290360	376302	53.28%	7.287%
12	11.880	1660	1664	1674	rBV4	4775	10534	1.49%	0.204%
13	12.939	1839	1844	1851	rBV	465102	571415	80.91%	11.065%
14	13.845	1991	1998	2009	rVB4	5308	14301	2.02%	0.277%
15	13.998	2019	2024	2034	rBV	137643	185922	26.33%	3.600%
16	15.468	2268	2274	2287	rBV	108708	188594	26.70%	3.652%




Sum of corrected areas: 5164006

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138929.D
Acq On : 12 Aug 2024 12:41
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

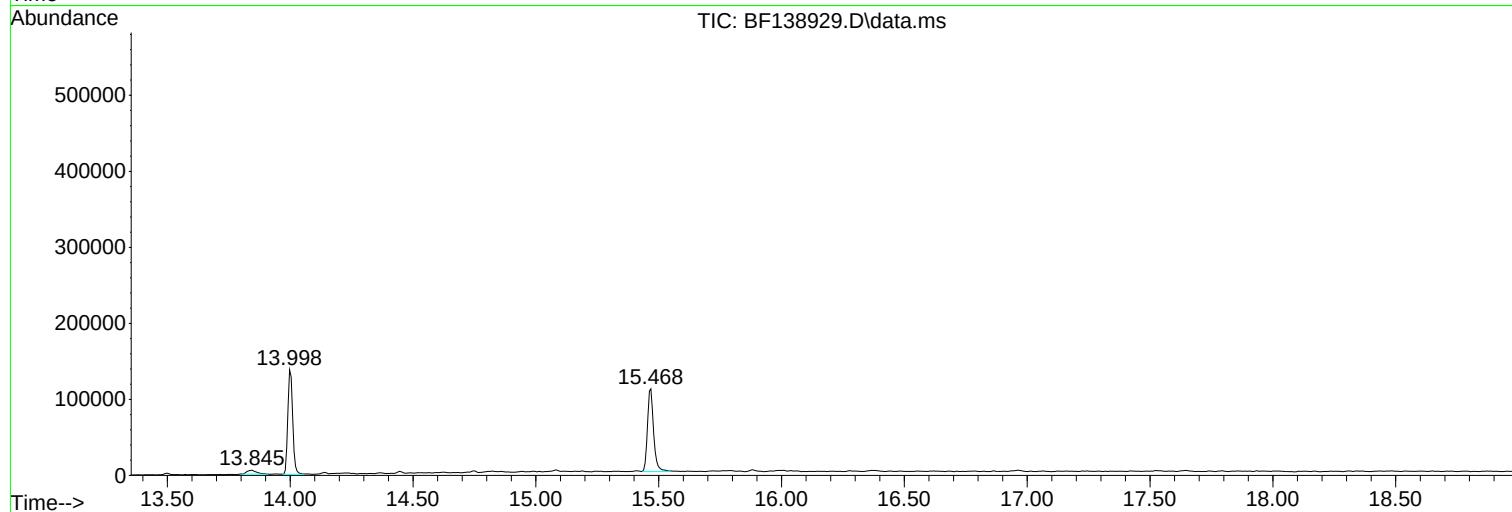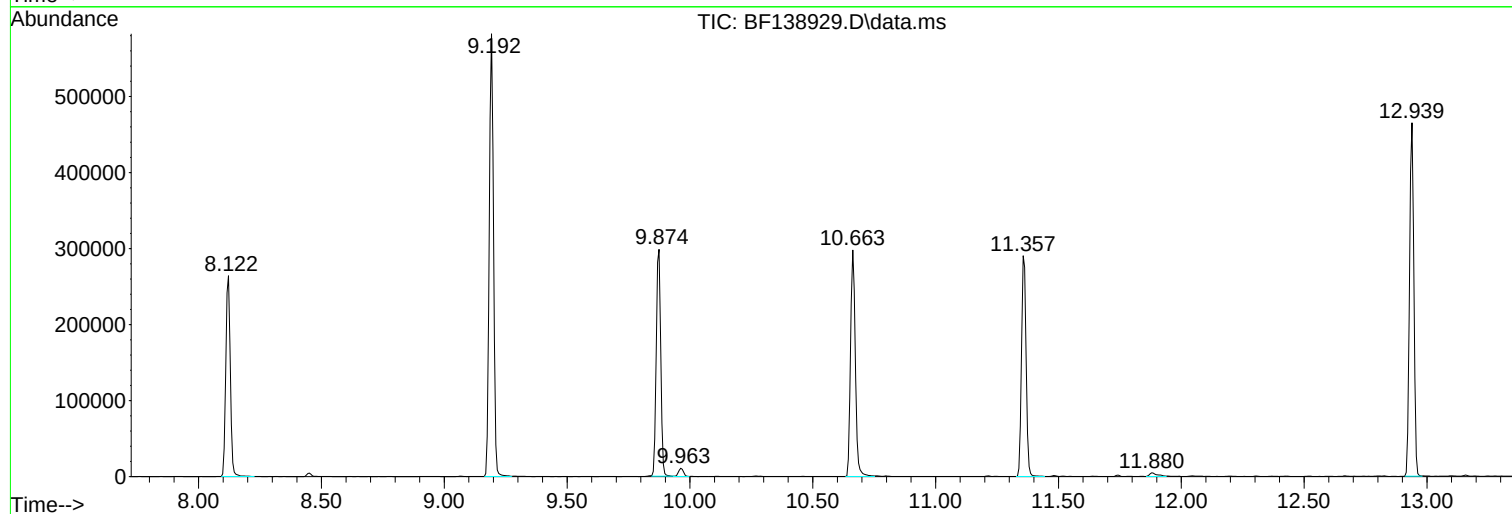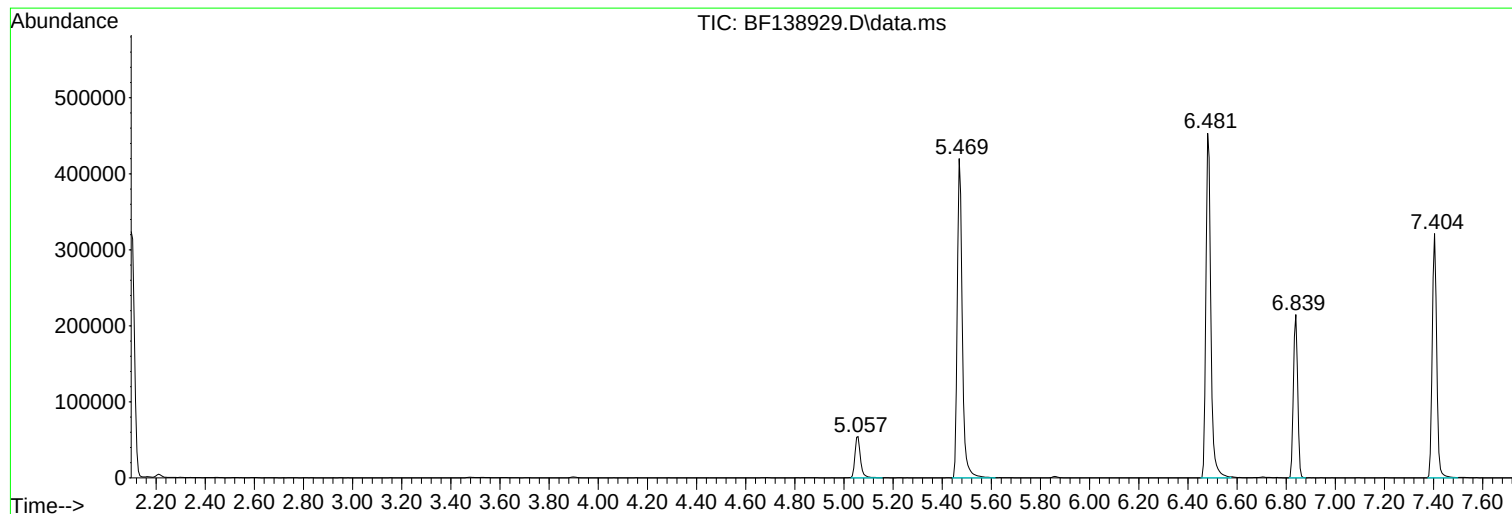

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138929.D
Acq On : 12 Aug 2024 12:41
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138929.D
Acq On : 12 Aug 2024 12:41
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------