

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
 Data File : BF138931.D
 Acq On : 12 Aug 2024 13:43
 Operator : RC/JU
 Sample : P3520-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-CF-09-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	498	504	518	rBV	61417	96752	13.23%	1.842%
2	5.469	569	574	602	rBV	464727	653118	89.34%	12.433%
3	6.481	741	746	771	rBV	514840	693355	94.84%	13.199%
4	6.840	802	807	814	rVB	197326	246236	33.68%	4.688%
5	7.404	898	903	916	rBV	339630	442780	60.57%	8.429%
6	8.116	1019	1024	1033	rBV	245980	321341	43.95%	6.117%
7	8.445	1076	1080	1094	rBB	6690	10896	1.49%	0.207%
8	9.192	1201	1207	1228	rBV	562971	731069	100.00%	13.917%
9	9.869	1317	1322	1333	rBV	279058	354737	48.52%	6.753%
10	9.963	1333	1338	1343	rVB	12681	18563	2.54%	0.353%
11	10.663	1452	1457	1473	rBV	302447	410438	56.14%	7.813%
12	11.357	1570	1575	1592	rBV	265186	338365	46.28%	6.441%
13	12.933	1838	1843	1854	rBV	436723	561668	76.83%	10.692%
14	13.839	1990	1997	2008	rBV6	6827	20441	2.80%	0.389%
15	13.998	2019	2024	2038	rVB	122839	166051	22.71%	3.161%
16	15.463	2267	2273	2291	rVB	106492	187208	25.61%	3.564%




Sum of corrected areas: 5253018

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138931.D
Acq On : 12 Aug 2024 13:43
Operator : RC/JU
Sample : P3520-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-09-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

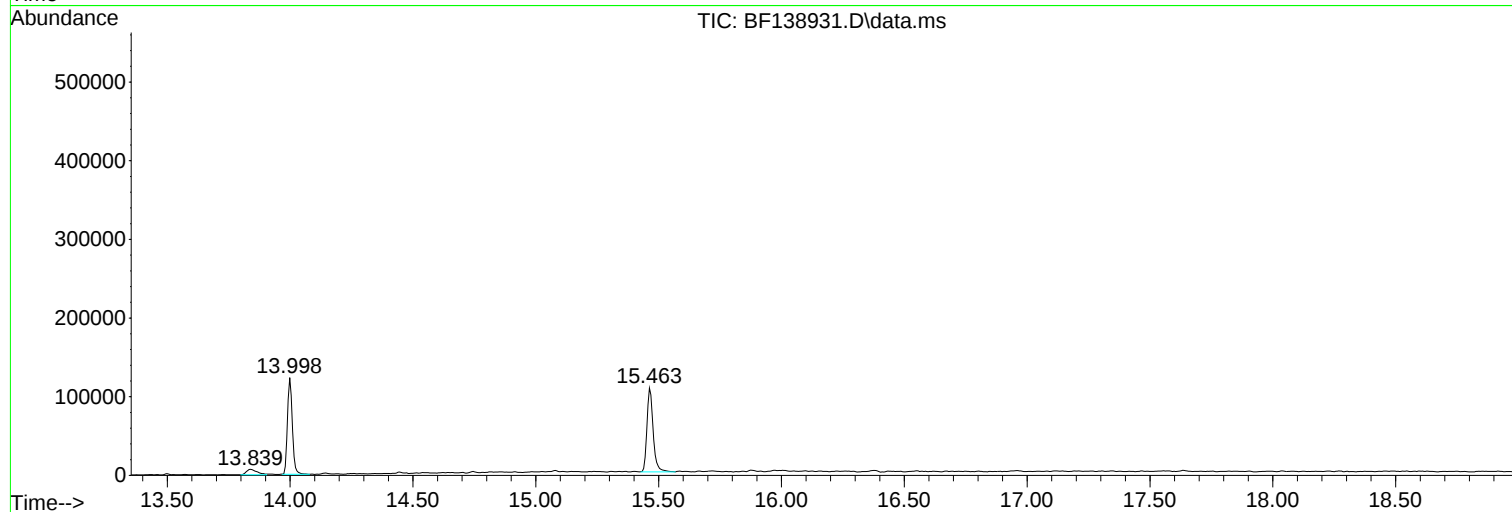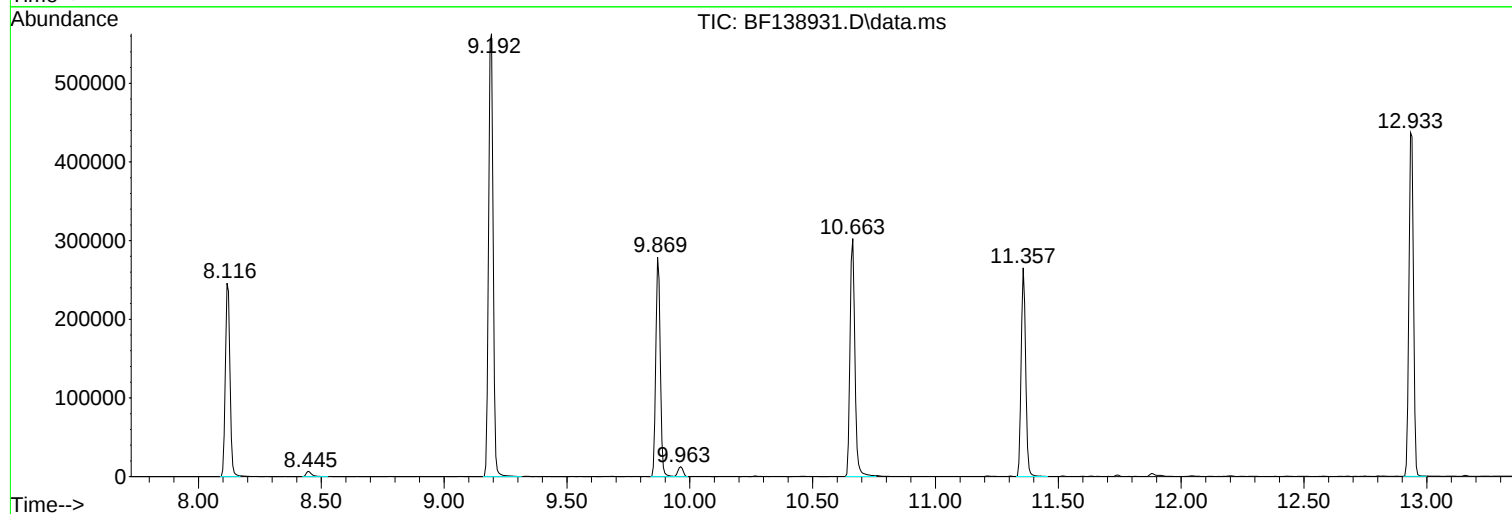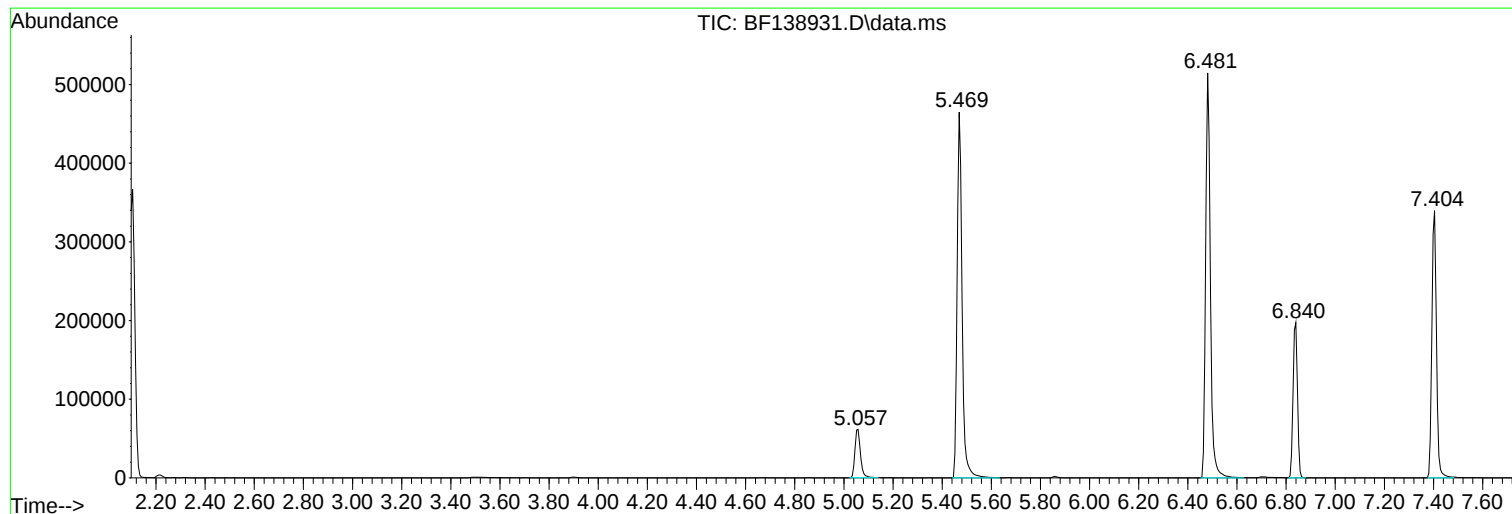

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138931.D
Acq On : 12 Aug 2024 13:43
Operator : RC/JU
Sample : P3520-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-09-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138931.D
Acq On : 12 Aug 2024 13:43
Operator : RC/JU
Sample : P3520-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-09-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------