

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
 Data File : BF138932.D
 Acq On : 12 Aug 2024 14:13
 Operator : RC/JU
 Sample : P3520-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-CF-08-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	499	504	520	rBV	82886	125743	12.85%	2.003%
2	5.469	569	574	602	rBV	561310	808776	82.64%	12.880%
3	6.481	741	746	773	rBV	617479	843765	86.22%	13.437%
4	6.839	802	807	814	rBB	194734	242306	24.76%	3.859%
5	7.404	898	903	926	rBV	428431	551850	56.39%	8.788%
6	8.116	1019	1024	1033	rBV	241852	317029	32.40%	5.049%
7	8.445	1076	1080	1094	rBB	7309	11488	1.17%	0.183%
8	9.192	1201	1207	1228	rBV	779744	978624	100.00%	15.585%
9	9.869	1317	1322	1333	rBV	287322	360614	36.85%	5.743%
10	9.963	1333	1338	1345	rVB	14392	21059	2.15%	0.335%
11	10.663	1452	1457	1472	rBV	399830	530319	54.19%	8.446%
12	11.357	1570	1575	1590	rBV	271358	344740	35.23%	5.490%
13	12.939	1838	1844	1849	rBV	606091	775427	79.24%	12.349%
14	13.833	1991	1996	2006	rBV5	6970	20676	2.11%	0.329%
15	13.998	2019	2024	2033	rBV	125113	167291	17.09%	2.664%
16	15.462	2267	2273	2286	rBV	103891	179582	18.35%	2.860%




Sum of corrected areas: 6279289

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138932.D
Acq On : 12 Aug 2024 14:13
Operator : RC/JU
Sample : P3520-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-08-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

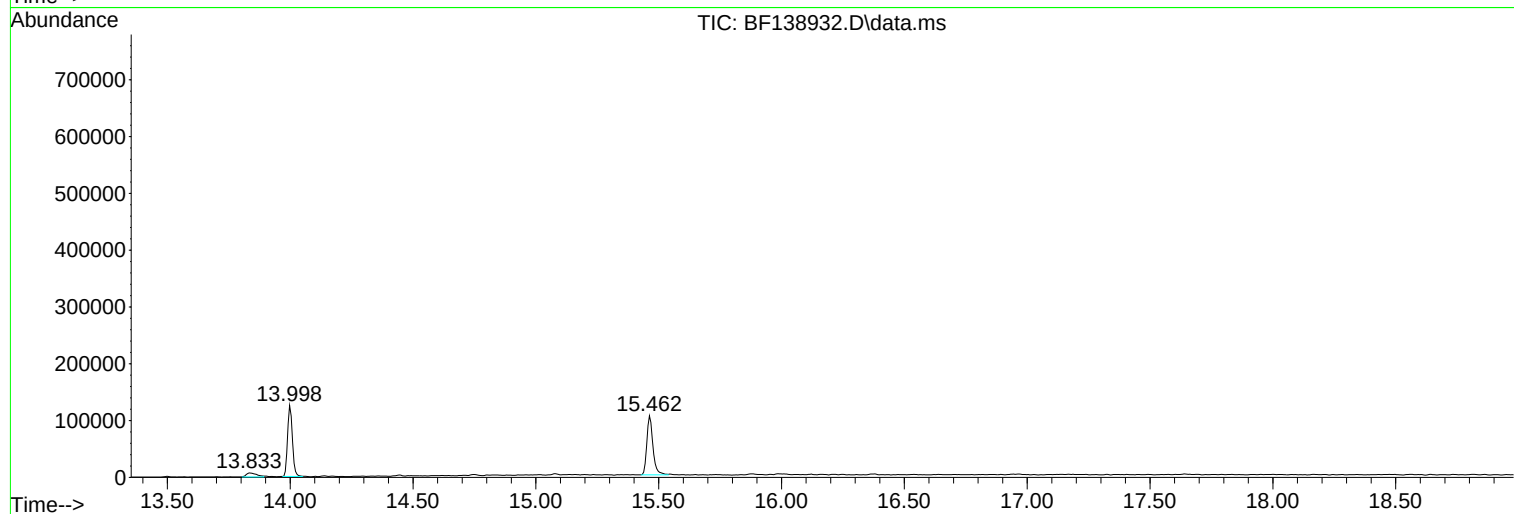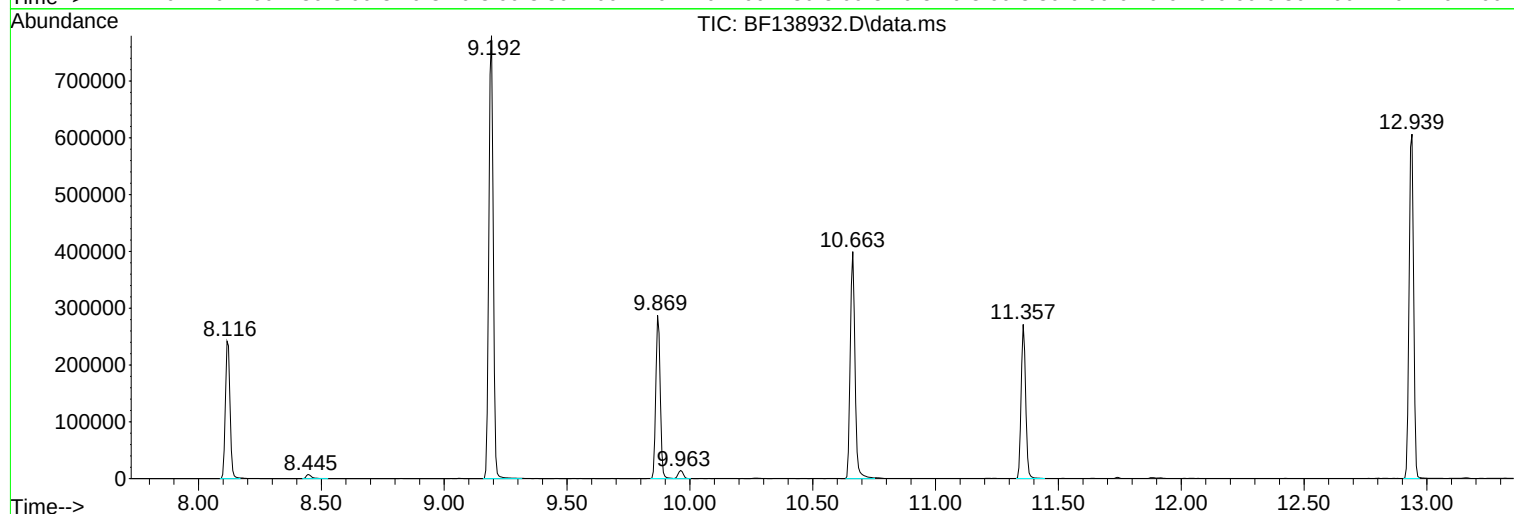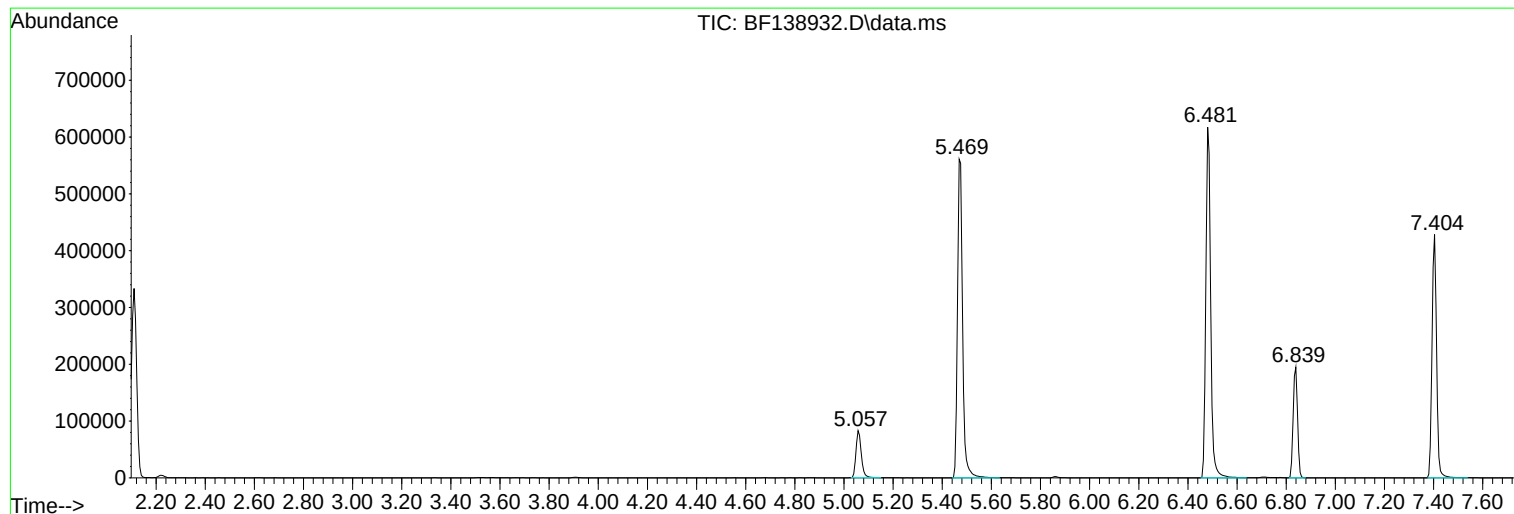

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138932.D
Acq On : 12 Aug 2024 14:13
Operator : RC/JU
Sample : P3520-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-08-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138932.D
Acq On : 12 Aug 2024 14:13
Operator : RC/JU
Sample : P3520-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-08-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------