
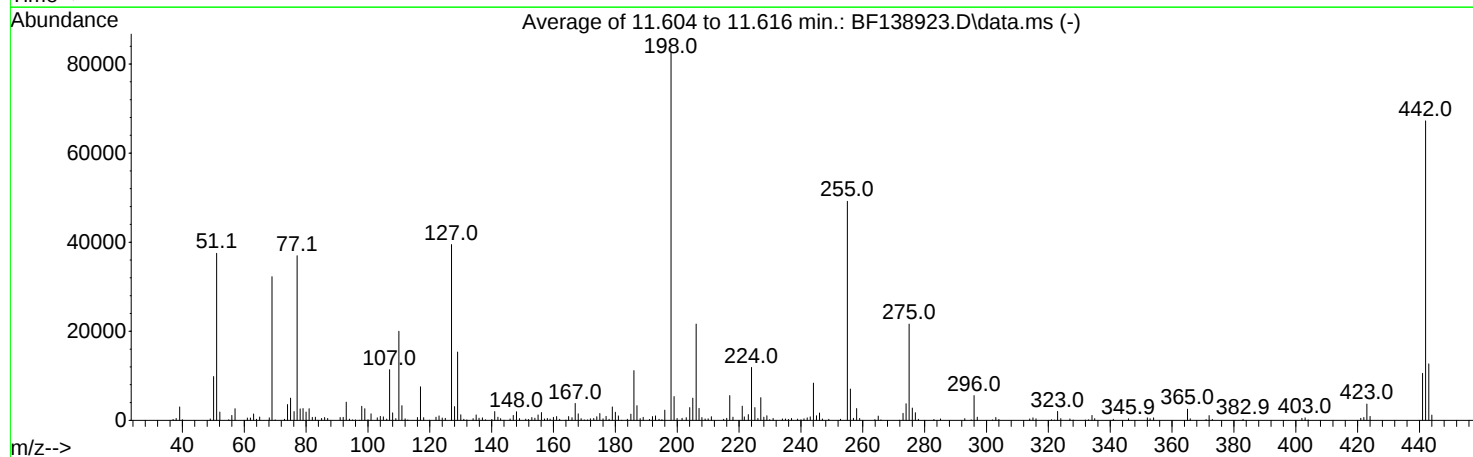


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138923.D
Acq On : 12 Aug 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

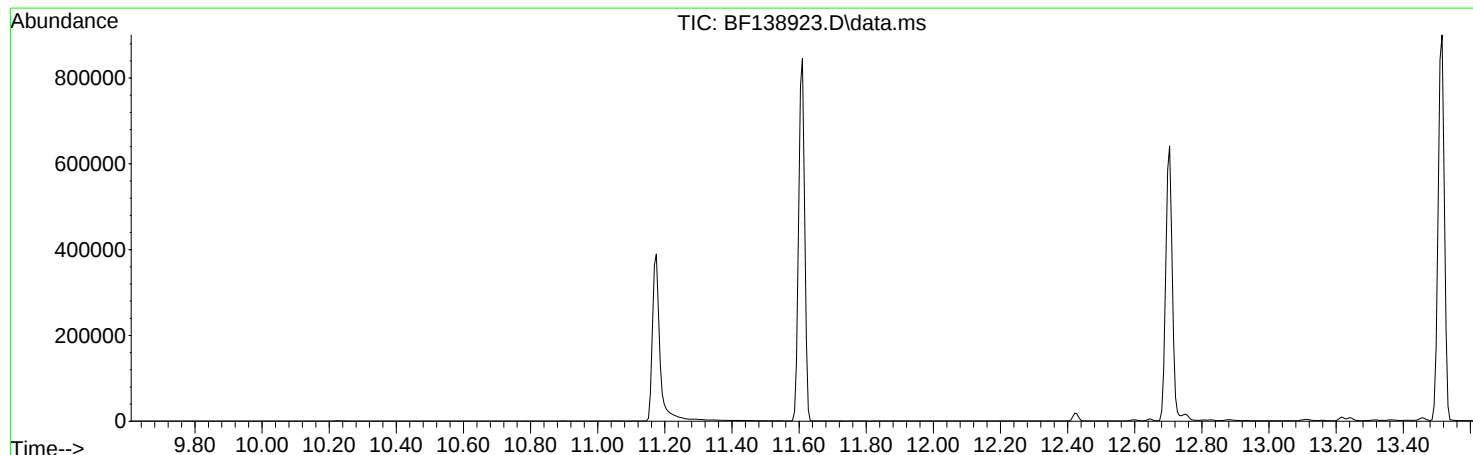

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	37515	PASS
68	69	0.00	2	1.8	591	PASS
69	198	0.00	100	39.0	32245	PASS
70	69	0.00	2	0.4	126	PASS
127	198	10	80	47.8	39469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82587	PASS
199	198	5	9	6.5	5338	PASS
275	198	10	60	26.2	21640	PASS
365	198	1	100	3.0	2506	PASS
441	198	0.01	100	12.8	10551	PASS
442	442	50	100	100.0	67245	PASS
443	442	15	24	18.8	12671	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2024	BNA_F	<u>BF138923.D</u>
Compound Name	Response	Retention Time
DDT	221063	13.516
DDD	5217	13.239
DDE	1319	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6536	227599	2.87

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138923.D
Acq On : 12 Aug 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:13:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

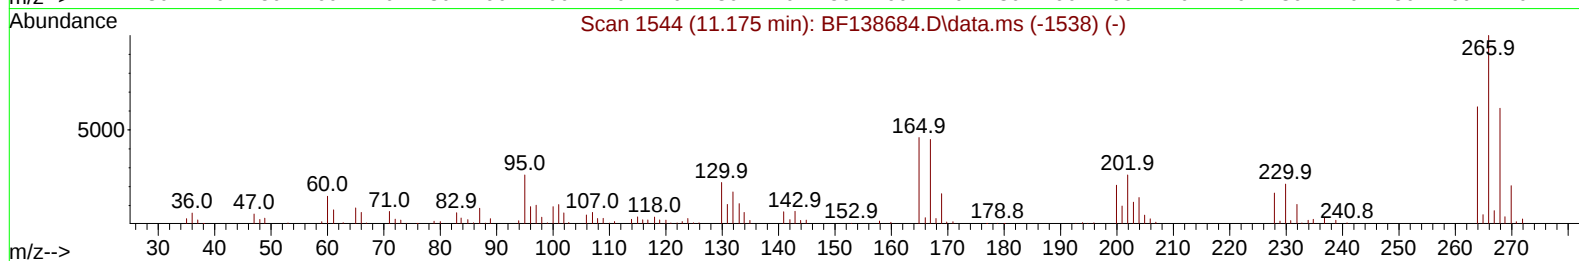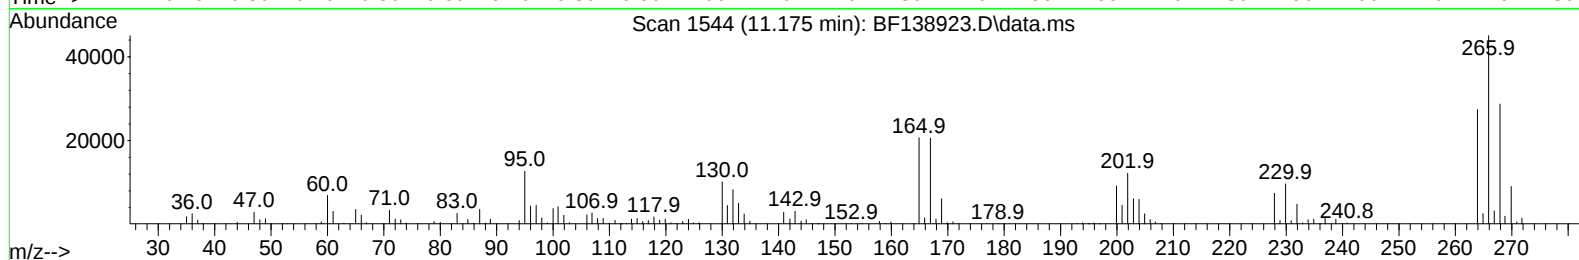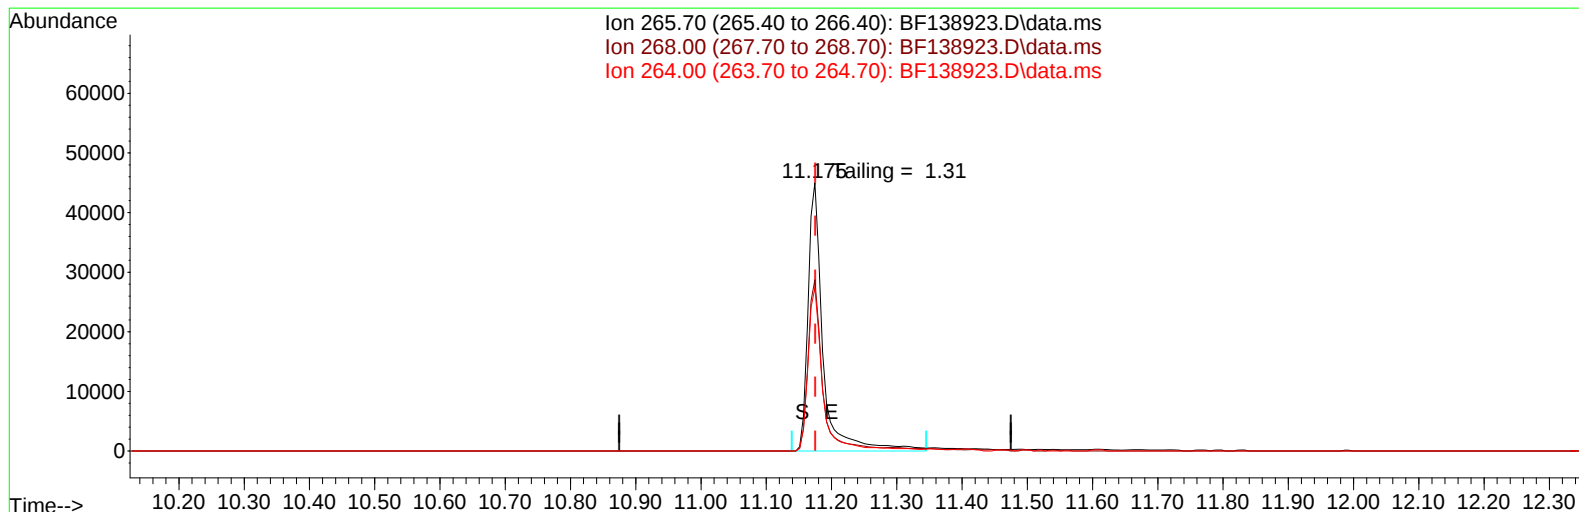

TIC: BF138923.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 27548.63 ng




response 72876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.81
264.00	62.20	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138923.D
Acq On : 12 Aug 2024 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:13:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

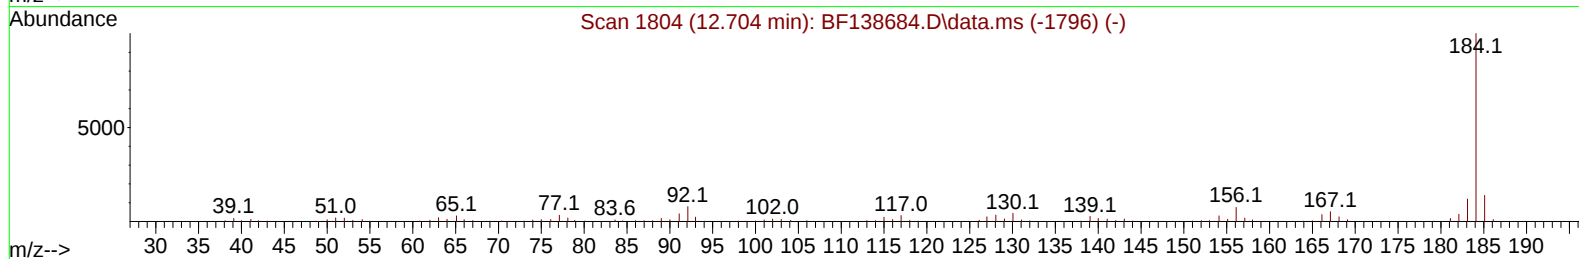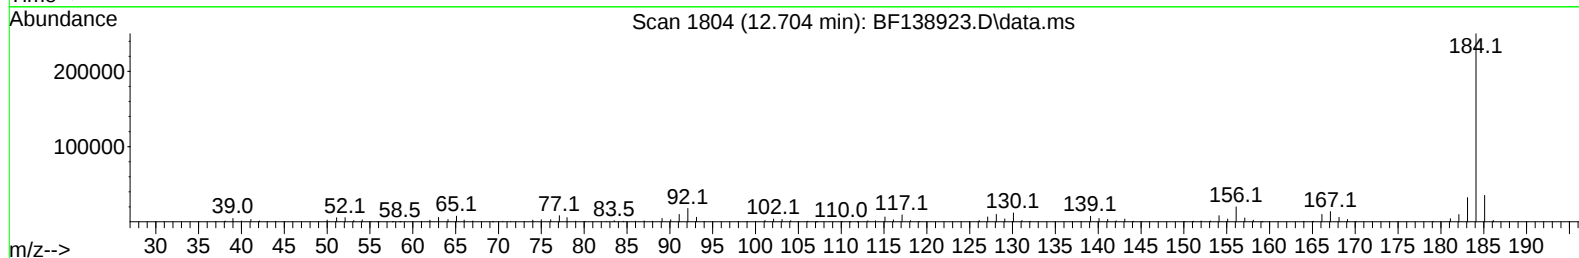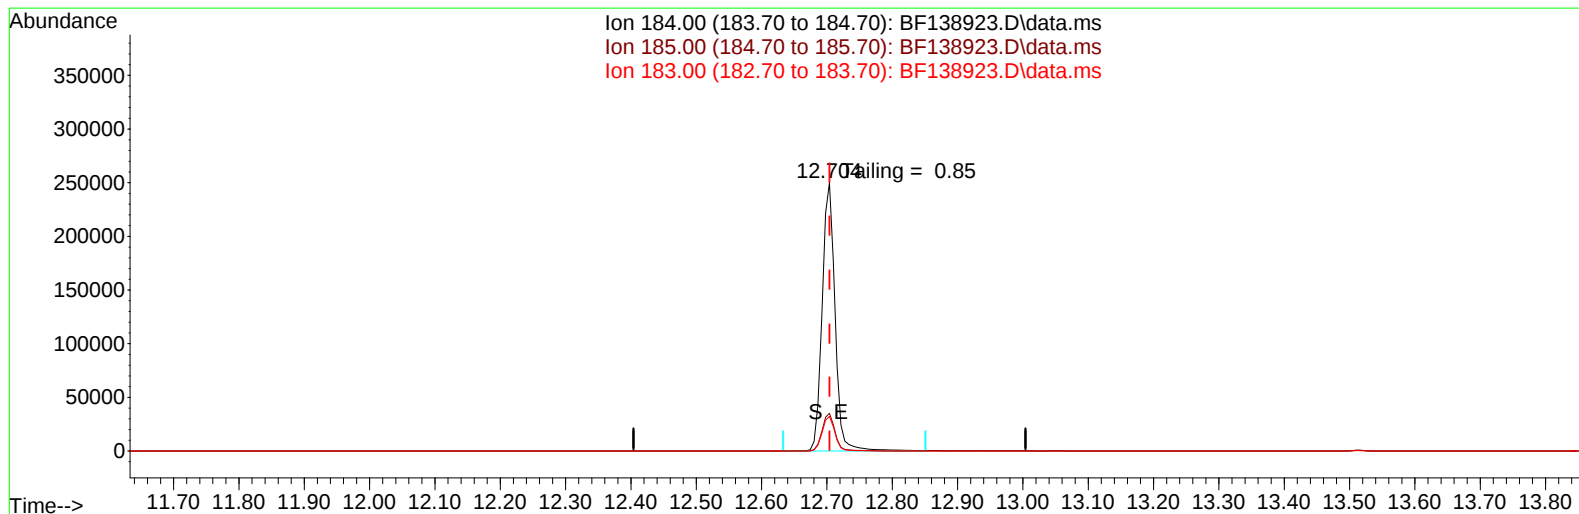

TIC: BF138923.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 343998

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.06
183.00	12.00	12.88
0.00	0.00	0.00