
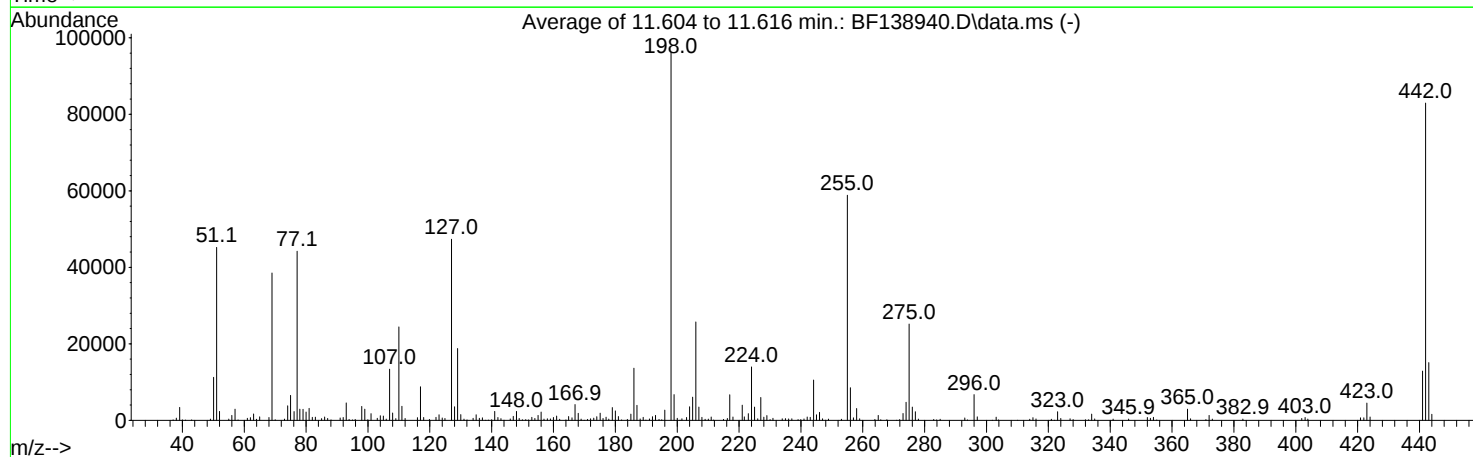


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138940.D
Acq On : 12 Aug 2024 18:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

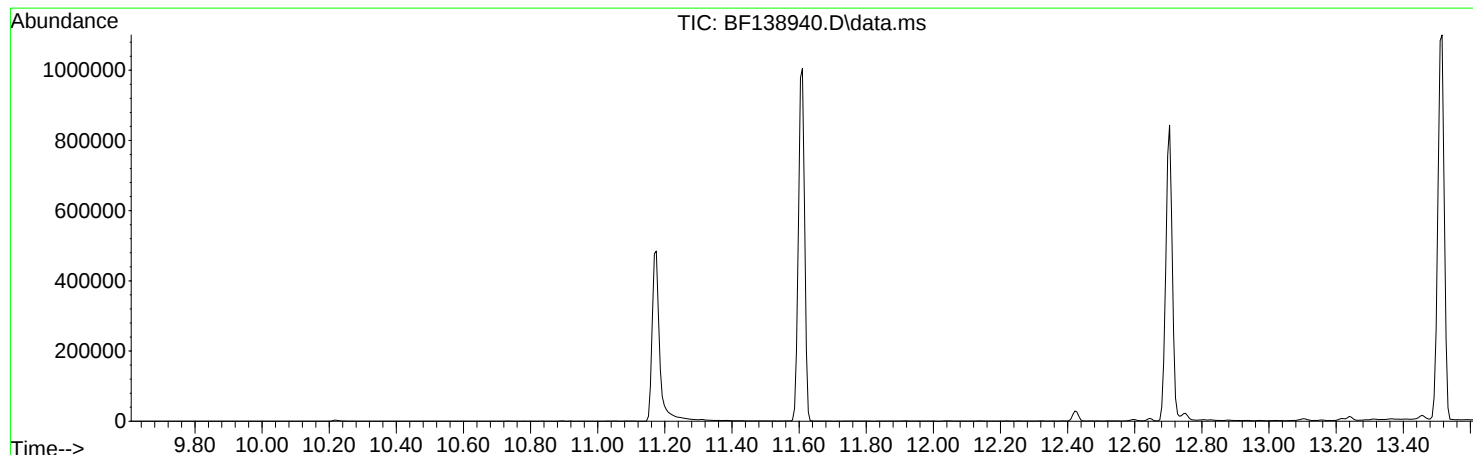

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	45232	PASS
68	69	0.00	2	2.0	758	PASS
69	198	0.00	100	40.1	38520	PASS
70	69	0.00	2	0.4	163	PASS
127	198	10	80	49.2	47331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96160	PASS
199	198	5	9	7.0	6734	PASS
275	198	10	60	26.2	25187	PASS
365	198	1	100	3.0	2930	PASS
441	198	0.01	100	13.4	12893	PASS
442	442	50	100	100.0	82949	PASS
443	442	15	24	18.2	15115	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2024	BNA_F	<u>BF138923.D</u>
Compound Name	Response	Retention Time
DDT	276627	13.516
DDD	5137	13.239
DDE	871	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6008	282635	2.13

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138940.D
Acq On : 12 Aug 2024 18:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 01:13:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

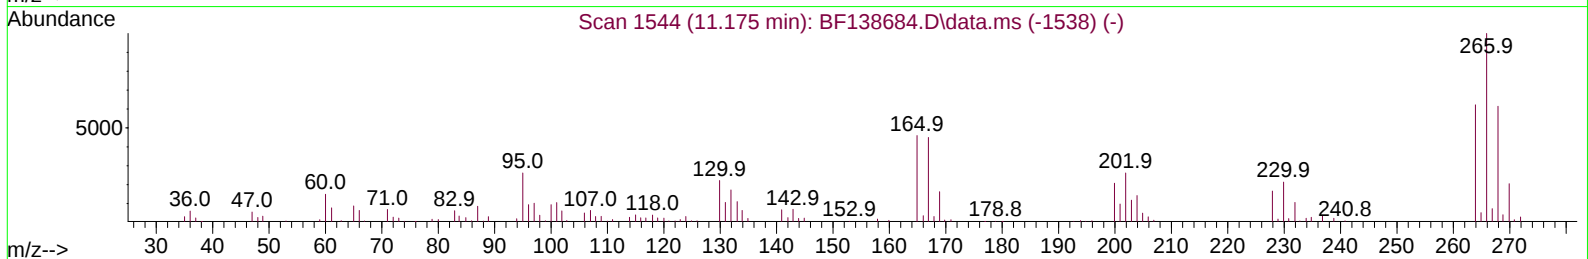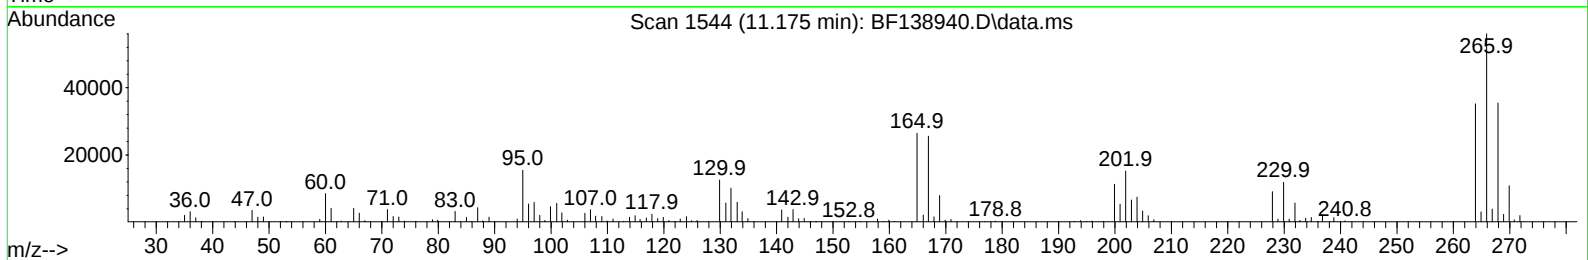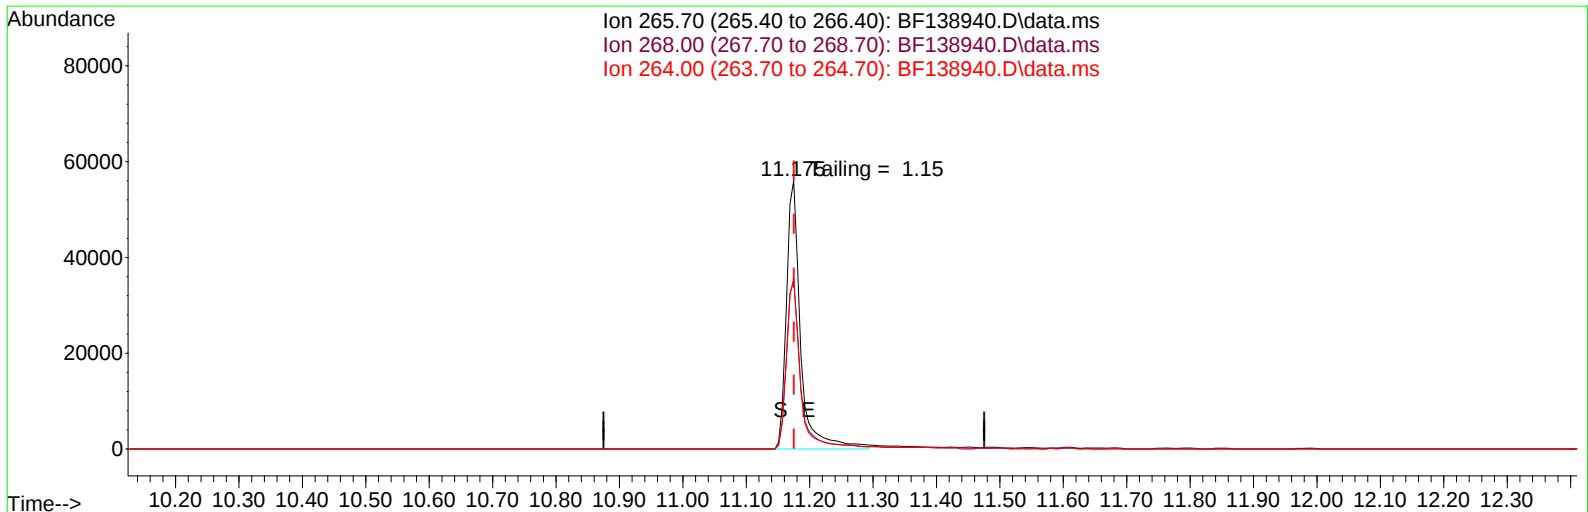

TIC: BF138940.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 153369.86 ng




response 91190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.24
264.00	62.20	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081224\
Data File : BF138940.D
Acq On : 12 Aug 2024 18:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 01:13:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

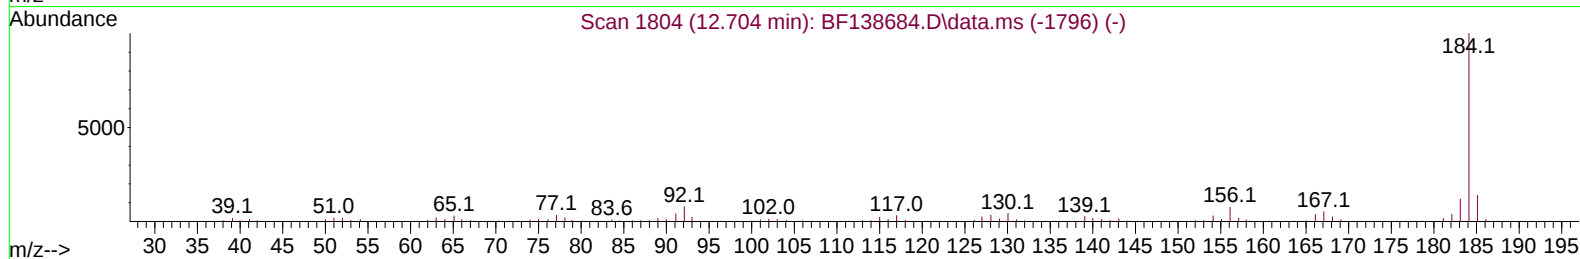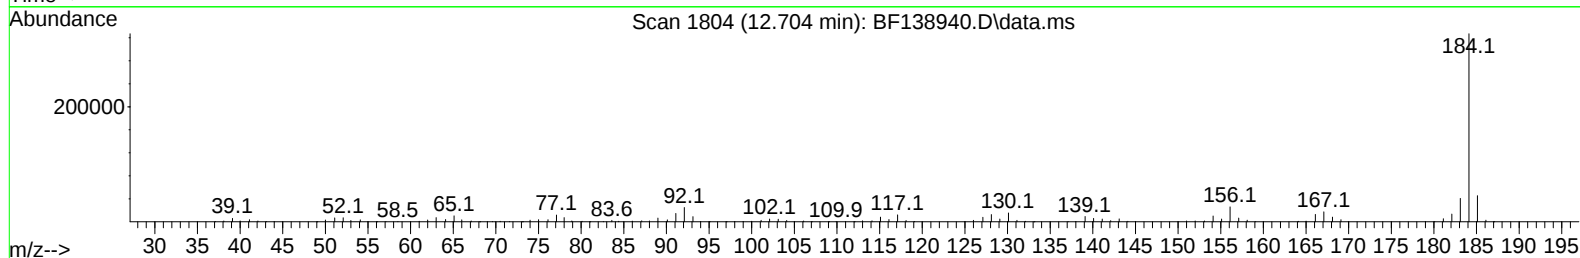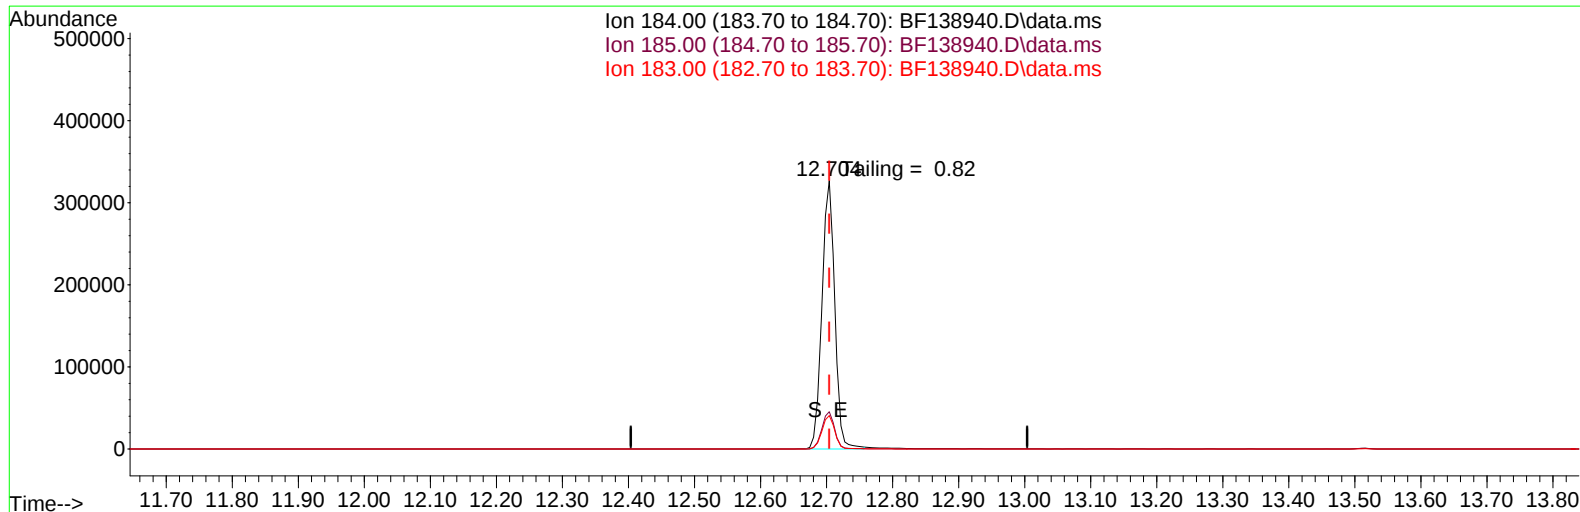

TIC: BF138940.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 445625

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.92
183.00	12.00	12.49
0.00	0.00	0.00