
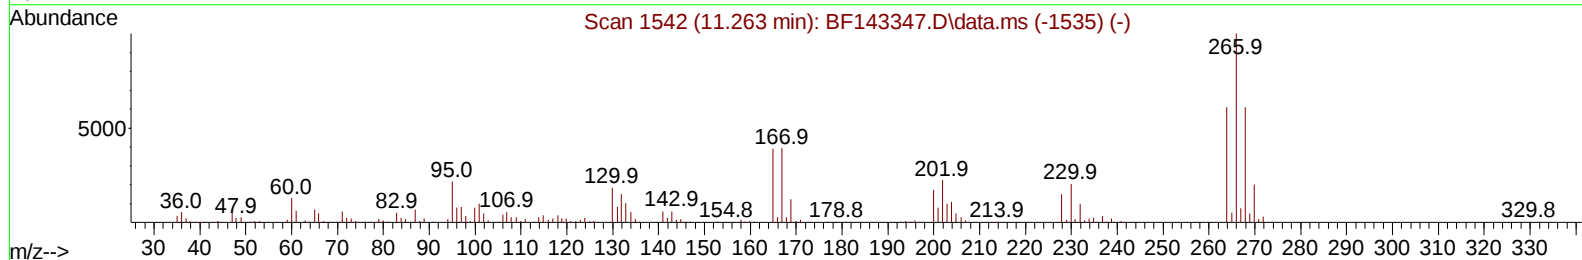
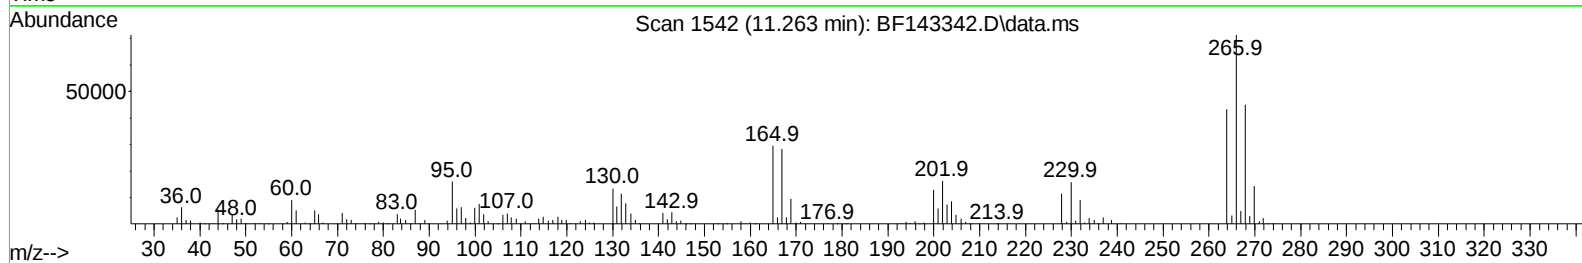


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081225\
Data File : BF143342.D
Acq On : 12 Aug 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 13:28:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

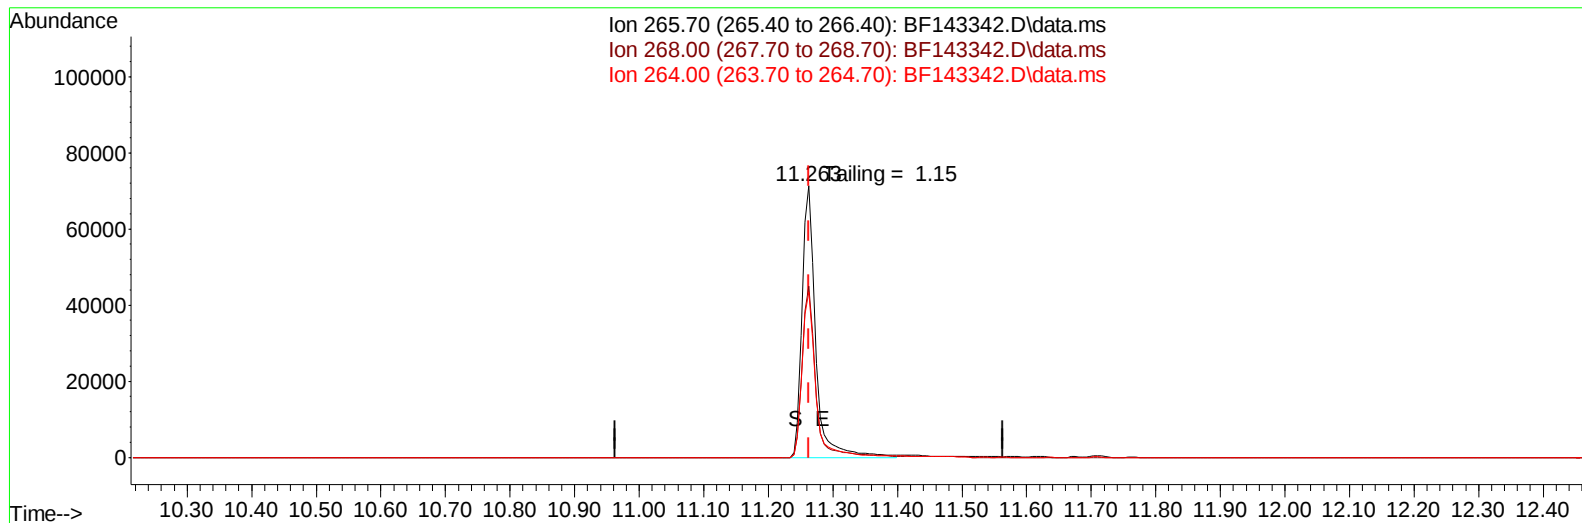

TIC: BF143342.D\data.ms

(70) Pentachlorophenol (C)




11.263min (-0.000) 127995.01 ng

response 106759

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.14
264.00	61.00	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081225\
Data File : BF143342.D
Acq On : 12 Aug 2025 08:34
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 13:28:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

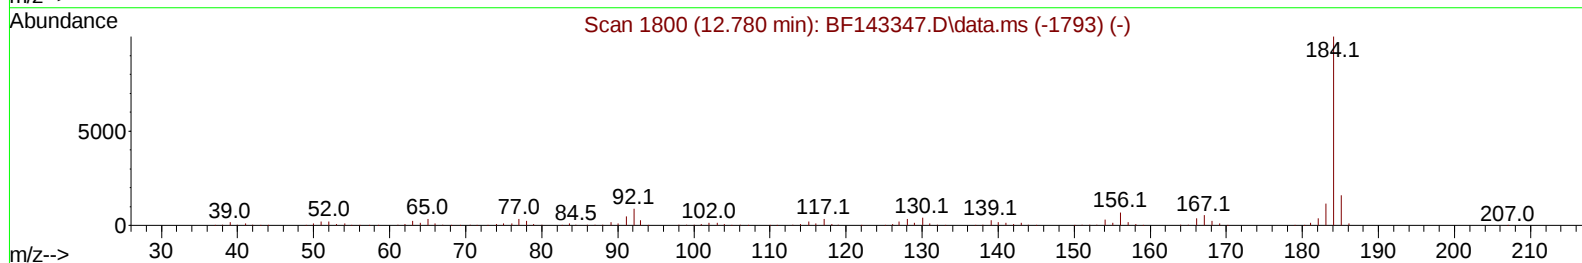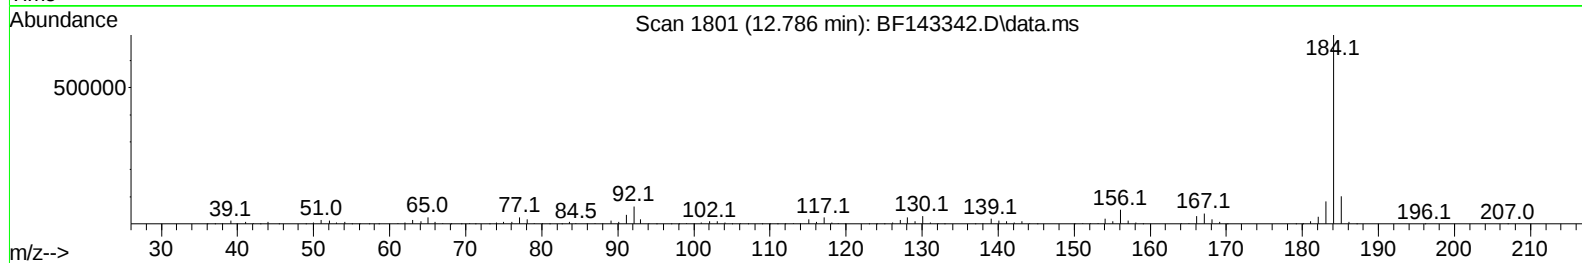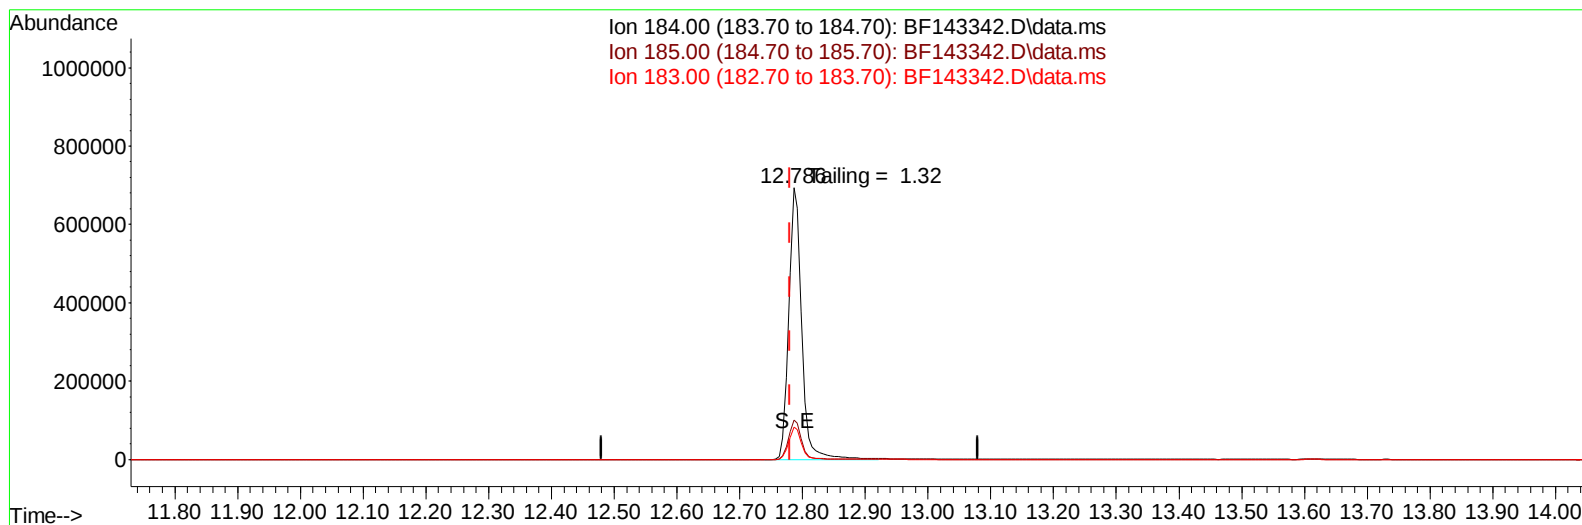

TIC: BF143342.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 1006924

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.63
183.00	11.60	11.87
0.00	0.00	0.00