


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081315\
 Data File : BF080975.D
 Acq On : 13 Aug 2015 9:10
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 08 01:33:05 2015

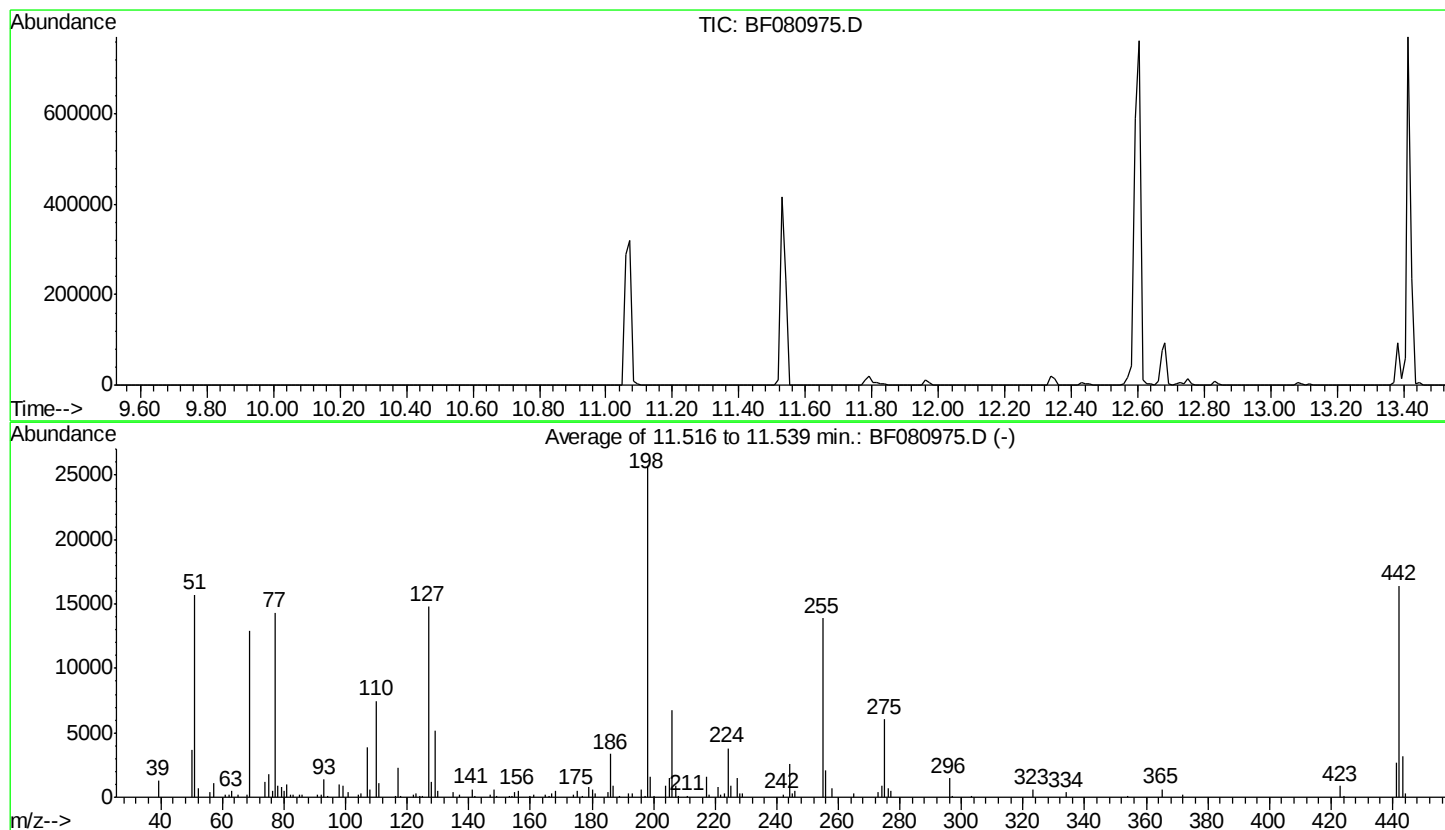

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.0	15710	PASS
68	69	0.00	2	1.3	163	PASS
69	198	0.00	100	50.3	12943	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.4	14786	PASS
197	198	0.00	2	0.5	126	PASS
198	198	100	100	100.0	25744	PASS
199	198	5	9	6.2	1594	PASS
275	198	10	60	23.4	6023	PASS
365	198	1	100	2.4	610	PASS
441	442	0.01	24	16.1	2645	PASS
442	198	50	100	63.9	16447	PASS
443	442	15	24	19.7	3232	PASS