


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081315\
 Data File : BF080994.D
 Acq On : 13 Aug 2015 23:48
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 08 01:33:05 2015

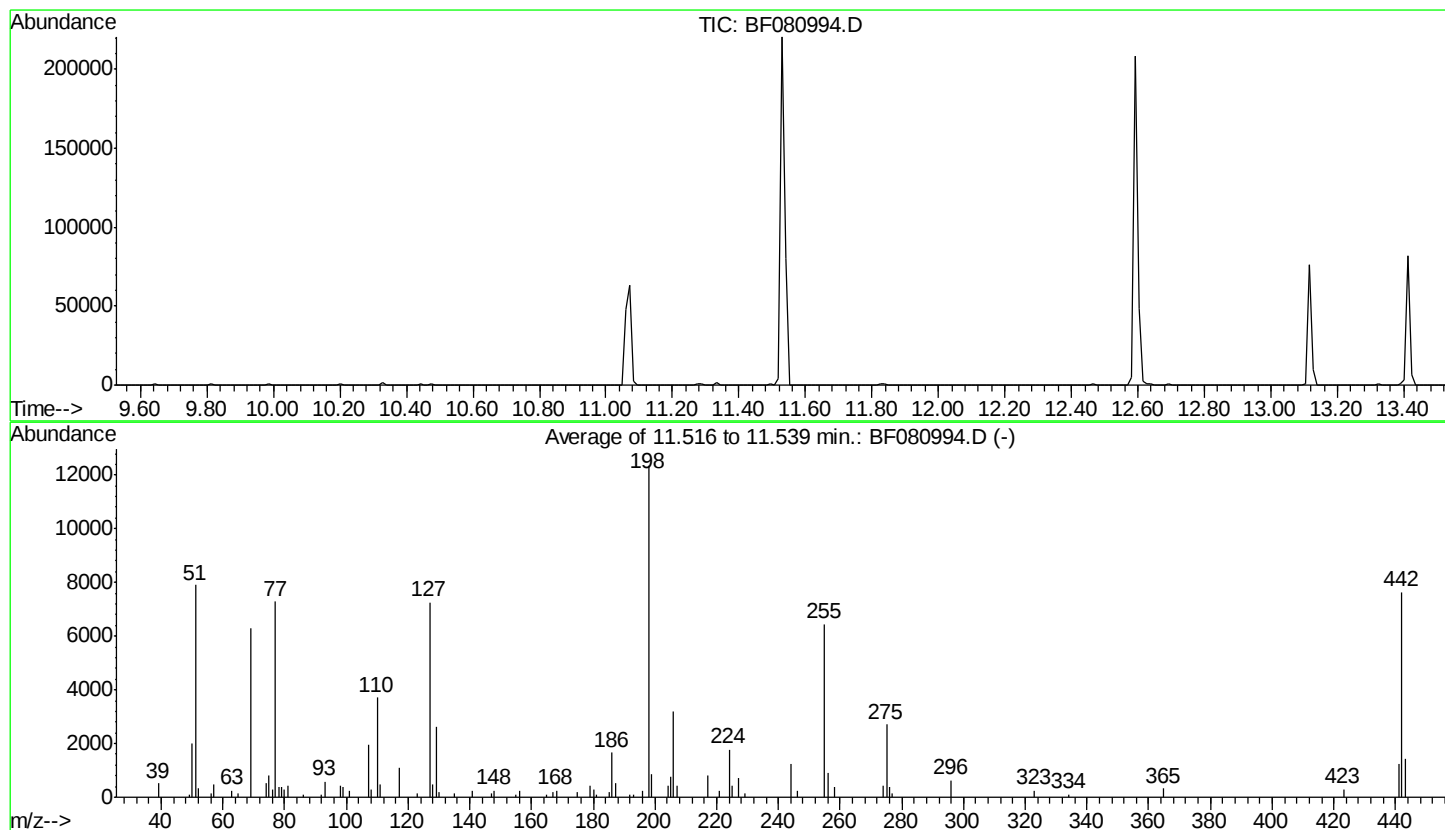

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.1	7911	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.1	6309	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.8	7265	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12349	PASS
199	198	5	9	7.1	877	PASS
275	198	10	60	21.9	2705	PASS
365	198	1	100	2.7	329	PASS
441	442	0.01	24	16.3	1246	PASS
442	198	50	100	61.8	7630	PASS
443	442	15	24	18.9	1440	PASS