

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081318\
 Data File : BF108120.D
 Acq On : 13 Aug 2018 17:05
 Operator : JU/SJ
 Sample : J4274-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HD-01-080918

Quant Time: Aug 14 01:10:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.02	152	227675	20.00	ng	0.01
21) Naphthalene-d8	8.31	136	783109	20.00	ng	0.00
38) Acenaphthene-d10	10.08	164	341871	20.00	ng	0.01
63) Phenanthrene-d10	11.58	188	593899	20.00	ng	0.02
75) Chrysene-d12	14.24	240	433441	20.00	ng	0.02
86) Perylene-d12	15.82	264	293873	20.00	ng	0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.65	112	1354589	107.72	ng	0.02
7) Phenol-d6	6.64	99	1818312	108.81	ng	0.01
23) Nitrobenzene-d5	7.58	82	1144376	81.54	ng	0.00
41) 2,4,6-Tribromophenol	10.87	330	380454	111.57	ng	0.01
44) 2-Fluorobiphenyl	9.38	172	1749600	82.16	ng	0.00
78) Terphenyl-d14	13.18	244	1432730	84.04	ng	0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.65	94	60179	3.481	ng	93
25) Isophorone	7.58	82	1144376	42.782	ng	# 64
32) Benzoic acid	8.07	122	707	6.064	ng	# 1
49) Dimethylphthalate	9.77	163	191521	8.042	ng	# 98
53) 2,4-Dinitrophenol	9.98	184	133	7.086	ng	# 1
64) 4,6-Dinitro-2-methylphenol	10.65	198	106	5.401	ng	# 1
66) 4-Bromophenyl-phenylether	10.87	248	27650	4.284	ng	# 1
74) Fluoranthene	12.80	202	66047	2.160	ng	90
77) Pyrene	13.04	202	80176	2.922	ng	98
88) Benzo(k)fluoranthene	15.34	252	32837	2.034	ng	# 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081318\
Data File : BF108120.D
Acq On : 13 Aug 2018 17:05
Operator : JU/SJ
Sample : J4274-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HD-01-080918

Quant Time: Aug 14 01:10:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

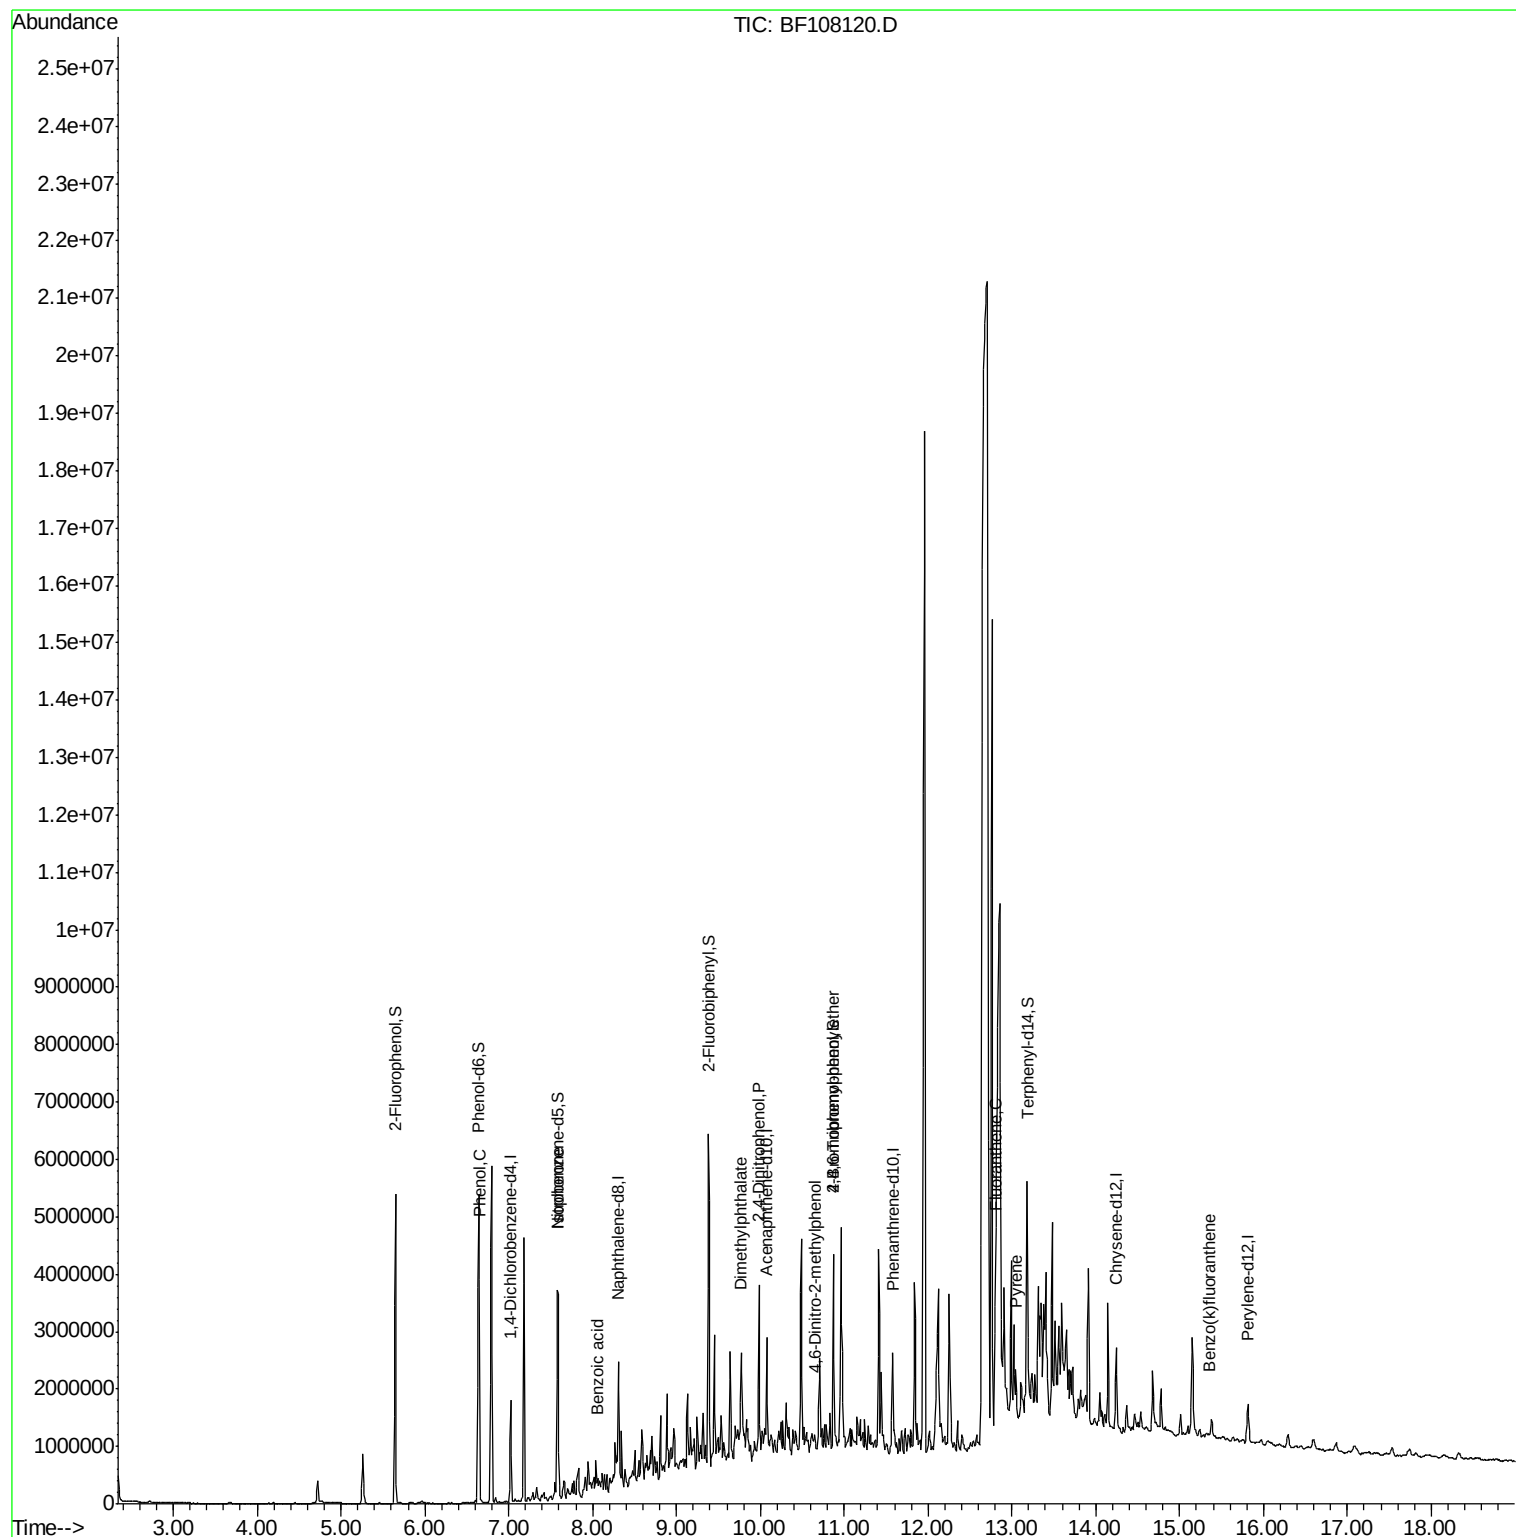




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.02 min Scan# 797
Delta R.T. 0.01 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Instrument :
BNA_F
ClientSampleId :
HD-01-080918

Tgt Ion:152 Resp: 227675
Ion Ratio Lower Upper
152 100
150 155.1 124.6 186.8
115 57.7 50.1 75.1

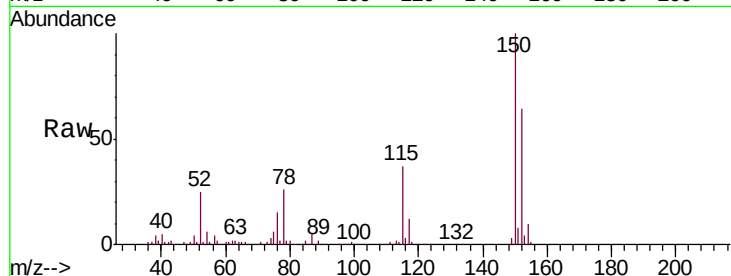


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

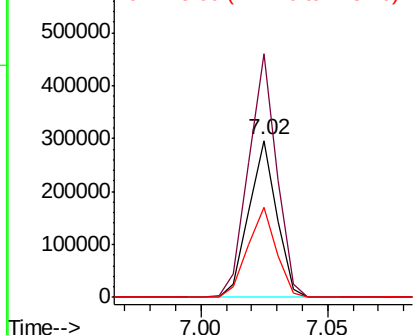



#5


2-Fluorophenol
Concen: 107.716 ng
RT: 5.65 min Scan# 563
Delta R.T. 0.02 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Tgt Ion:112 Resp: 1354589
Ion Ratio Lower Upper
112 100
64 72.2 47.9 71.9#
63 37.9 23.7 35.5#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

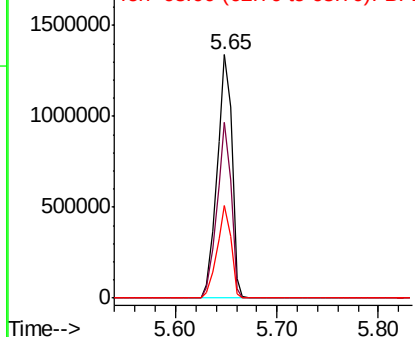

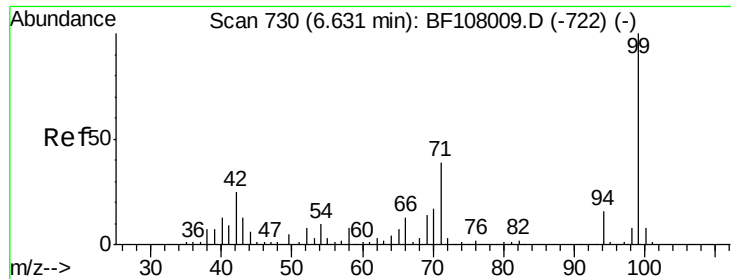

#7

Phenol-d6

Concen: 108.808 ng

RT: 6.64 min Scan# 732

Delta R.T. 0.01 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05

Instrument :


BNA_F

ClientSampleId :




HD-01-080918

Tgt Ion: 99 Resp: 1818312

Ion	Ratio	Lower	Upper
99	100		
42	24.4	14.5	21.7#
71	38.3	25.4	38.0#

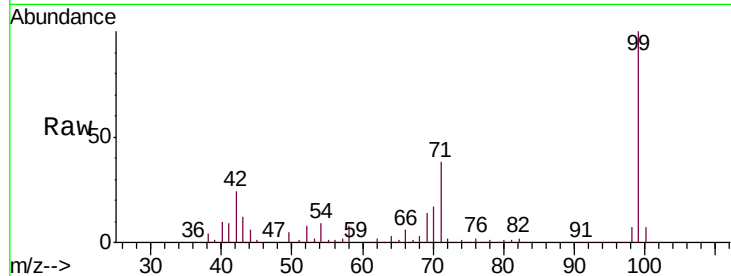

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

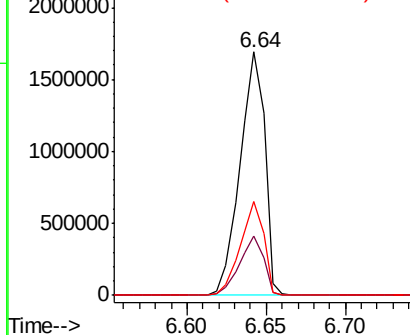

#10

Phenol

Concen: 3.481 ng

RT: 6.65 min Scan# 734


Delta R.T. 0.01 min

Lab File: BF108120.D



Acq: 13 Aug 2018 17:05


Tgt Ion: 94 Resp: 60179

Ion	Ratio	Lower	Upper
94	100		
65	30.4	7.9	47.9
66	41.1	16.2	56.2



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1




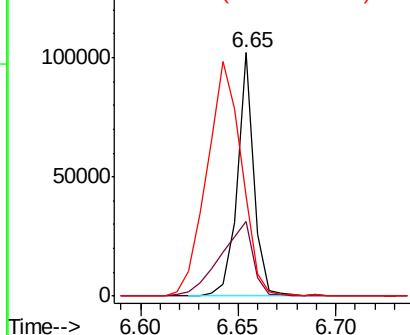




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.31 min Scan# 1015
Delta R.T. 0.01 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05




Instrument :
BNA_F
ClientSampleId :
HD-01-080918


Tgt Ion:	136	Resp:	783109
Ion	Ratio	Lower	Upper
136	100		
137	11.8	8.9	13.3
54	11.1	6.6	9.8#
68	7.2	5.0	7.4

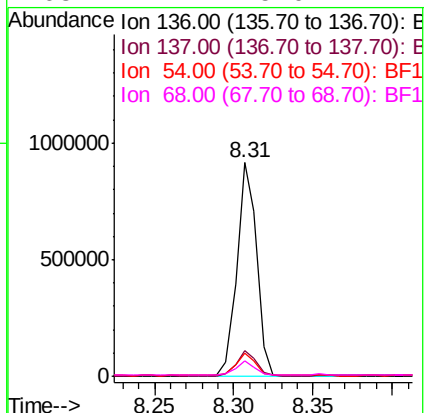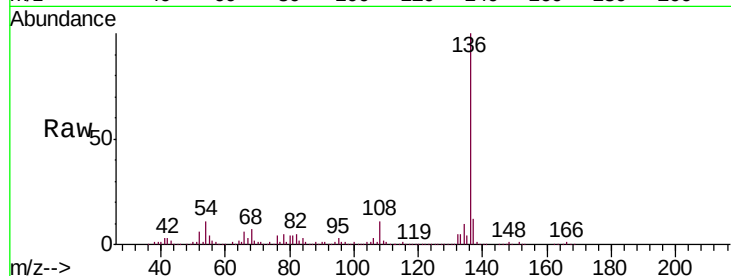

#23
Nitrobenzene-d5
Concen: 81.544 ng
RT: 7.58 min Scan# 892
Delta R.T. 0.01 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Tgt Ion:	82	Resp:	1144376
Ion	Ratio	Lower	Upper
82	100		
128	41.3	36.1	54.1
54	61.7	41.4	62.2

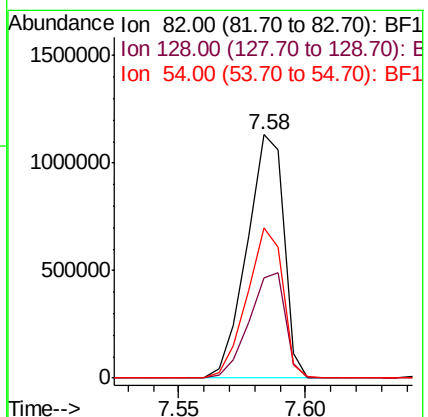

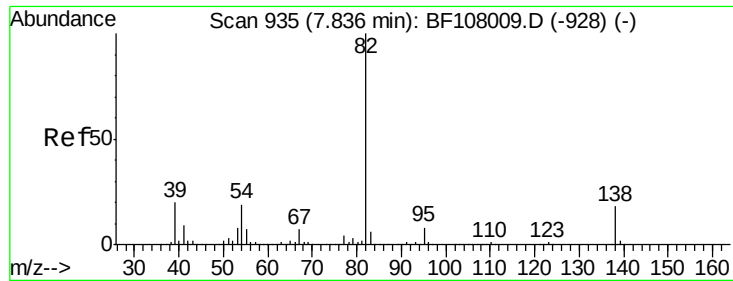

#25

Isophorone

Concen: 42.782 ng

RT: 7.58 min Scan# 892

Delta R.T. -0.25 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05

Instrument :

BNA_F

ClientSampleId :

HD-01-080918


Tgt Ion: 82 Resp: 1144376

Ion Ratio Lower Upper




82 100

95 0.3 5.2 7.8#

138 0.0 14.9 22.3#

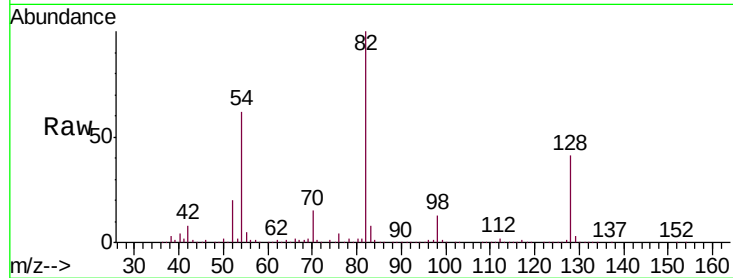

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

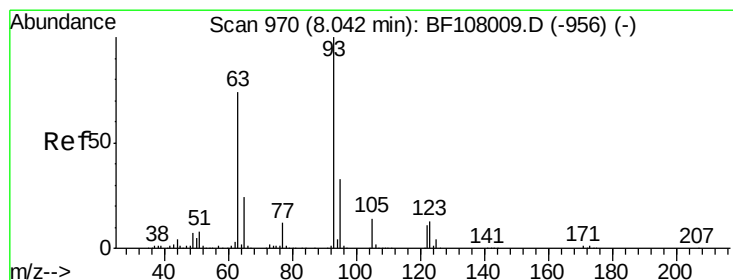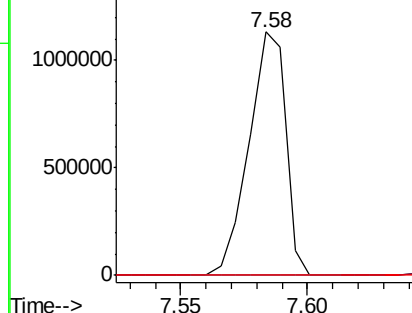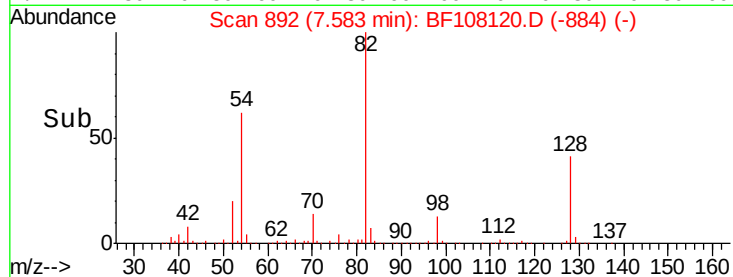

#32

Benzoic acid

Concen: 6.064 ng

RT: 8.07 min Scan# 974

Delta R.T. 0.02 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05


Tgt Ion: 122 Resp: 707

Ion Ratio Lower Upper



122 100


105 7547.2 101.1 141.1#

77 2065.6 70.7 110.7#

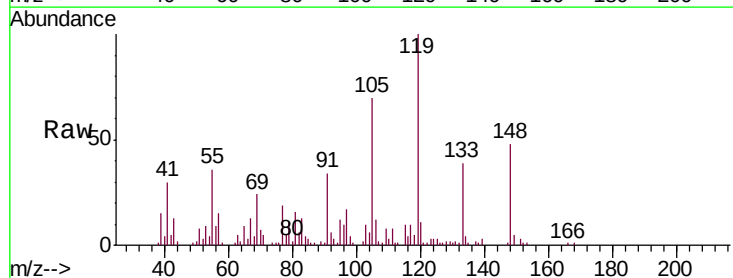

Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF1



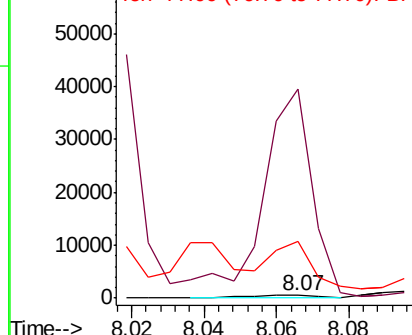
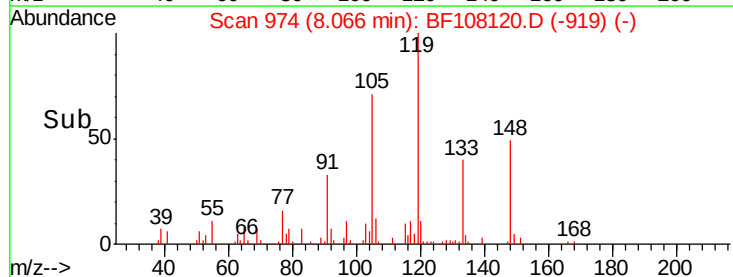


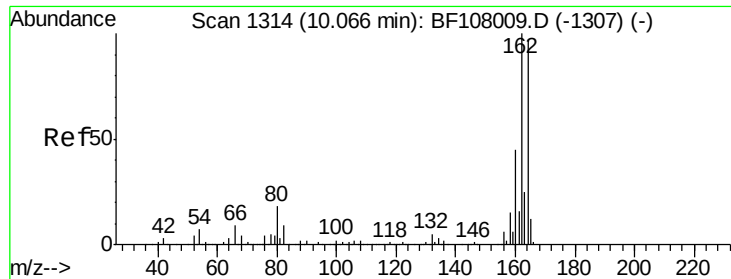

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.08 min Scan# 1316
 Delta R.T. 0.01 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05




Instrument :
 BNA_F
 ClientSampled :
 HD-01-080918


Tgt Ion:164 Resp: 341871
 Ion Ratio Lower Upper
 164 100
 162 105.0 86.1 129.1
 160 49.1 38.3 57.5

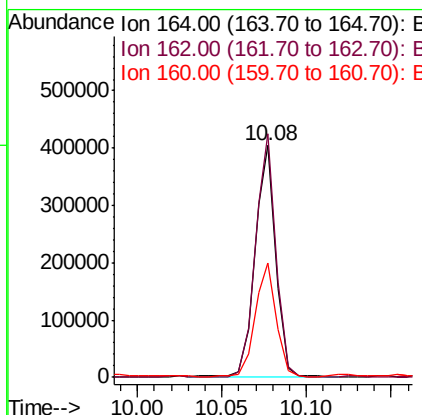

#41
 2,4,6-Tribromophenol
 Concen: 111.568 ng
 RT: 10.87 min Scan# 1451
 Delta R.T. 0.01 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05

Tgt Ion:330 Resp: 380454
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.0 115.6
 141 33.5 29.9 44.9

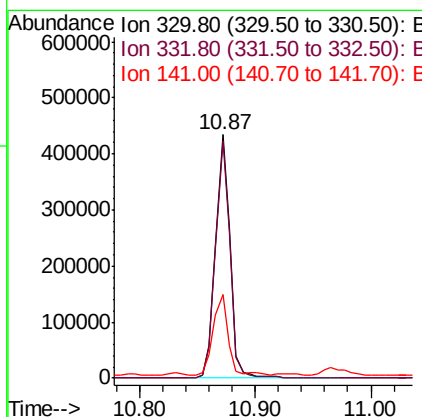







#44
2-Fluorobiphenyl
Concen: 82.163 ng
RT: 9.38 min Scan# 1198
Delta R.T. 0.01 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Instrument :
BNA_F
ClientSampleId :
HD-01-080918

Tgt Ion:172 Resp: 1749600
Ion Ratio Lower Upper
172 100
171 38.1 29.7 44.5
170 25.5 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


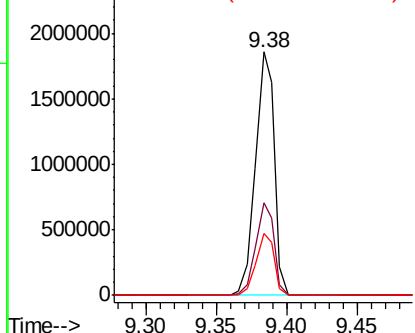



#49
Dimethylphthalate
Concen: 8.042 ng
RT: 9.77 min Scan# 1264
Delta R.T. -0.01 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Tgt Ion:163 Resp: 191521
Ion Ratio Lower Upper
163 100
194 5.5 2.7 4.1#
164 10.5 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E




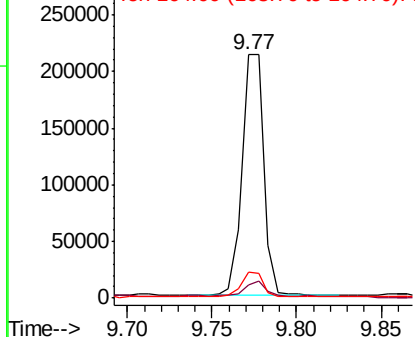


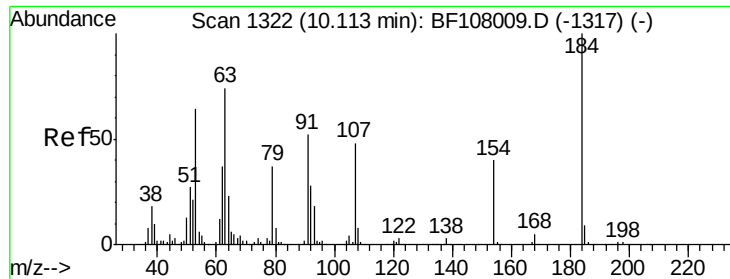

#53
 2,4-Dinitrophenol
 Concen: 7.086 ng
 RT: 9.98 min Scan# 1300
 Delta R.T. -0.13 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05




Instrument :
 BNA_F
 ClientSampleId :
 HD-01-080918


Tgt Ion:184 Resp: 133
 Ion Ratio Lower Upper
 184 100
 63 498.7 54.2 81.2#
 154 1263.0 184.0 276.0#

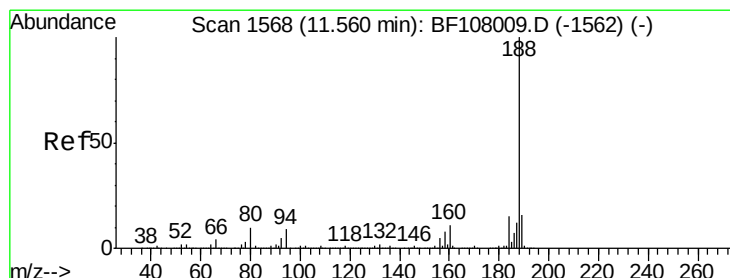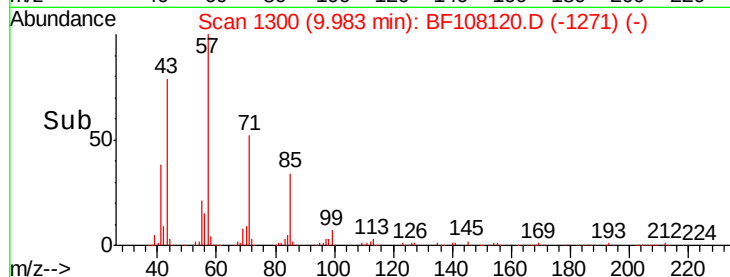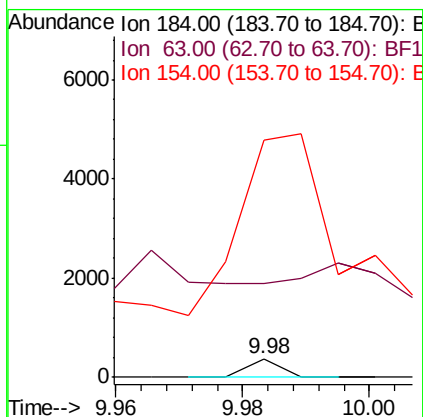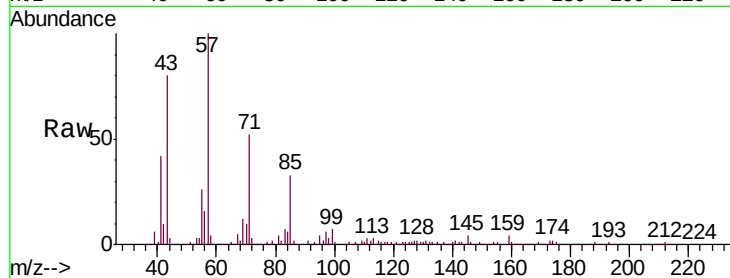

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.58 min Scan# 1571
 Delta R.T. 0.02 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05

Tgt Ion:188 Resp: 593899
 Ion Ratio Lower Upper
 188 100
 94 8.3 8.5 12.7#
 80 9.1 9.2 13.8#


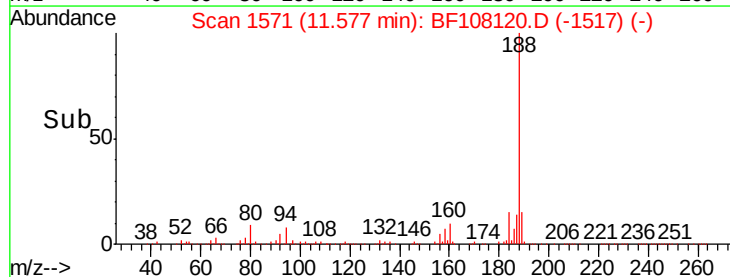
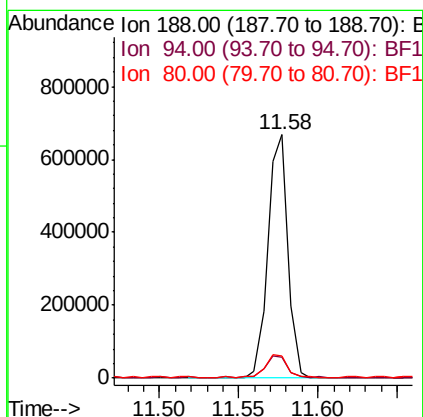
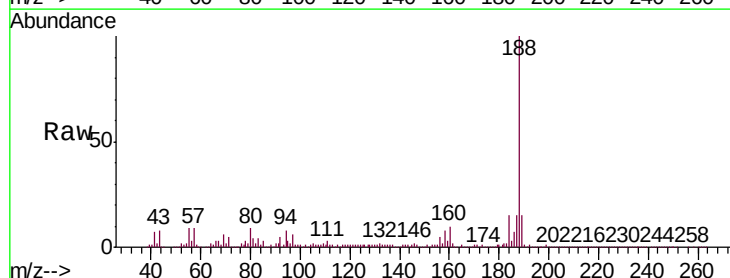




#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.401 ng
 RT: 10.65 min Scan# 1413
 Delta R.T. -0.01 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05




Instrument :
 BNA_F
 ClientSampleId :
 HD-01-080918


Tgt Ion:198 Resp: 106
 Ion Ratio Lower Upper
 198 100
 51 1163.1 37.7 77.7#
 105 5063.8 36.3 76.3#

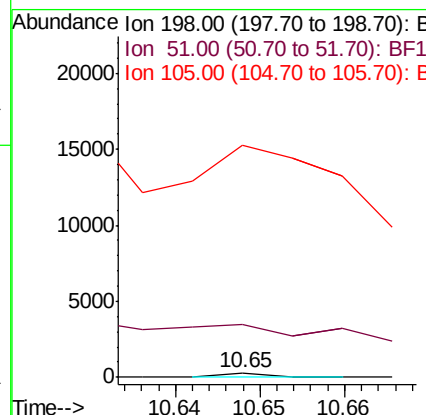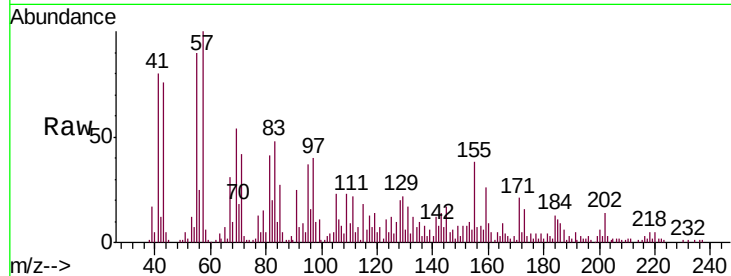

#66
 4-Bromophenyl-phenylether
 Concen: 4.284 ng
 RT: 10.87 min Scan# 1451
 Delta R.T. -0.23 min
 Lab File: BF108120.D
 Acq: 13 Aug 2018 17:05

Tgt Ion:248 Resp: 27650
 Ion Ratio Lower Upper
 248 100
 250 189.1 76.9 115.3#
 141 457.2 74.4 111.6#

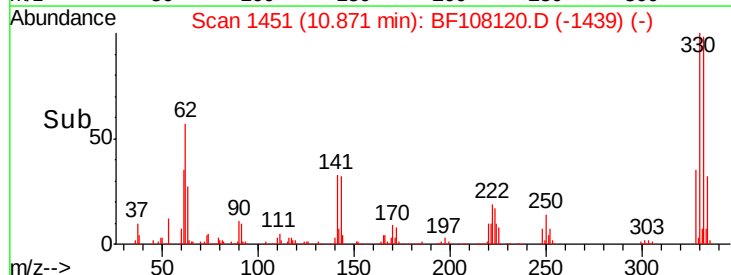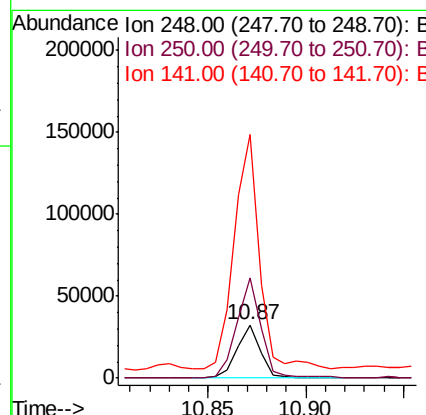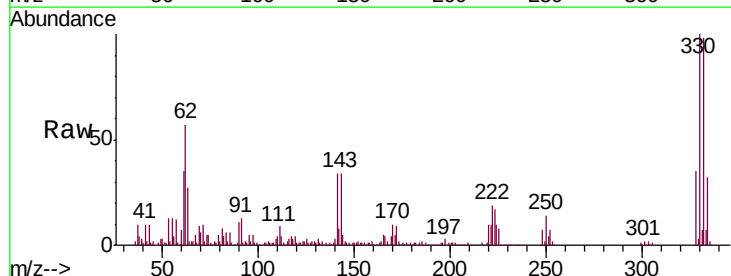



#74

Fluoranthene

Concen: 2.160 ng

RT: 12.80 min Scan# 1779

Delta R.T. 0.02 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05

Instrument :

BNA_F

ClientSampleId :

HD-01-080918


Tgt Ion:202 Resp: 66047

Ion Ratio Lower Upper

202 100

101 19.6 0.0 34.1




203 21.7 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

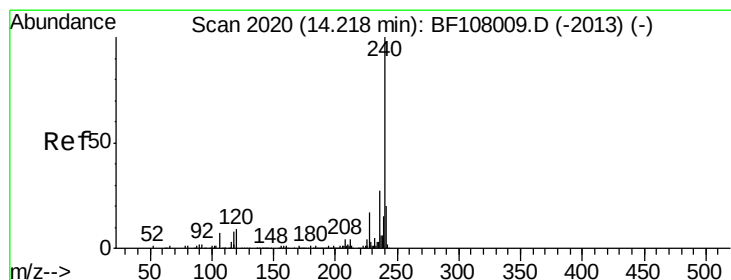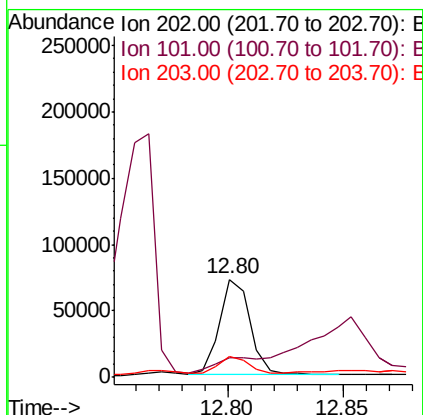

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.24 min Scan# 2024

Delta R.T. 0.02 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05


Tgt Ion:240 Resp: 433441

Ion Ratio Lower Upper

240 100

120 11.3 9.5 14.3



236 26.4 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

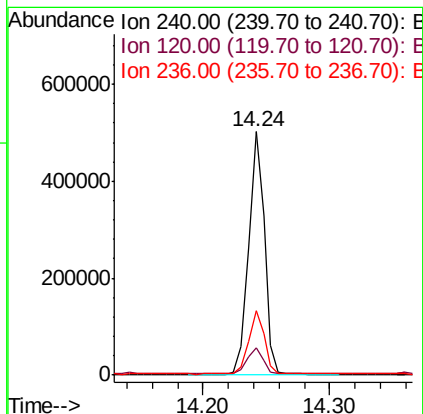

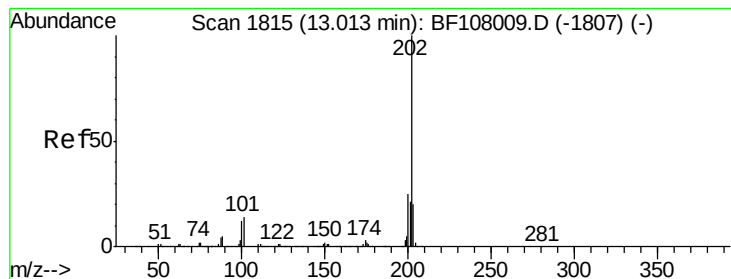

#77

Pyrene

Concen: 2.922 ng

RT: 13.04 min Scan# 1820

Delta R.T. 0.03 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05

Instrument :

BNA_F

ClientSampleId :

HD-01-080918


Tgt Ion: 202 Resp: 80176

Ion Ratio Lower Upper

202 100

200 22.3 17.4 26.2




203 19.4 14.3 21.5



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

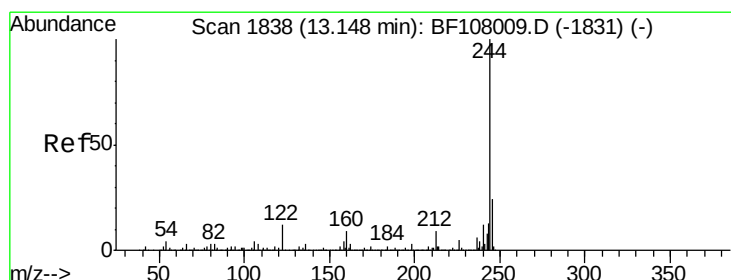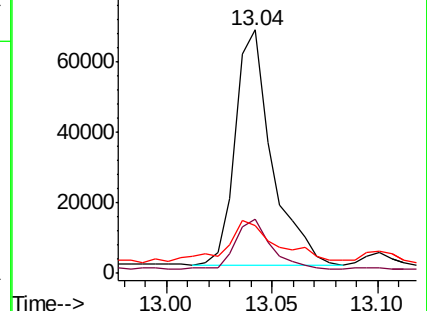

#78

Terphenyl-d14

Concen: 84.044 ng

RT: 13.18 min Scan# 1844

Delta R.T. 0.04 min

Lab File: BF108120.D

Acq: 13 Aug 2018 17:05


Tgt Ion: 244 Resp: 1432730

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 9.1 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



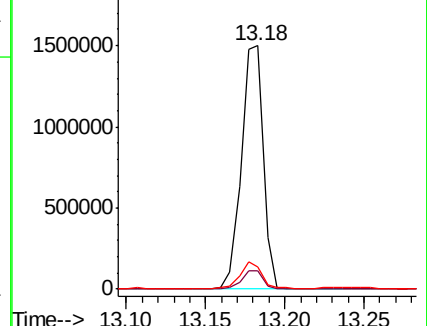



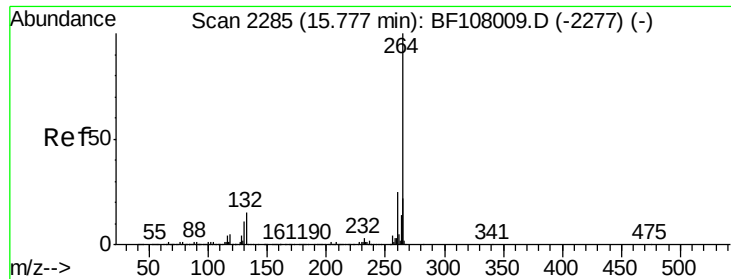

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.82 min Scan# 2292
Delta R.T. 0.04 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Instrument :
BNA_F
ClientSampleId :
HD-01-080918

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.2	28.8
265	21.5	17.5	26.3

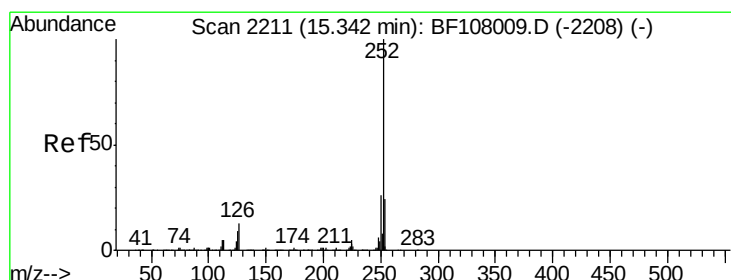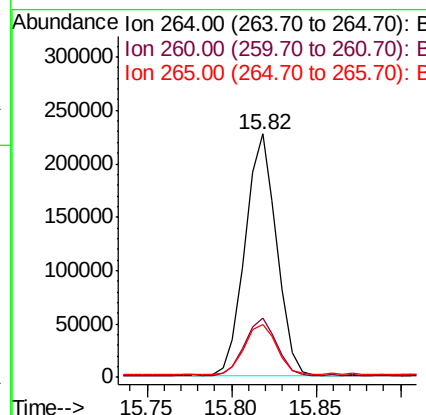

#88
Benzo(k)fluoranthene
Concen: 2.034 ng
RT: 15.34 min Scan# 2211
Delta R.T. -0.00 min
Lab File: BF108120.D
Acq: 13 Aug 2018 17:05

Tgt Ion	Ratio	Lower	Upper
252	100		
253	62.9	17.9	26.9#
125	45.0	10.2	15.2#

