

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081318\
 Data File : BF108121.D
 Acq On : 13 Aug 2018 17:32
 Operator : JU/SJ
 Sample : J4282-03RE 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-080918-BRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.249	491	495	500	rVB	231256	232022	3.91%	0.568%
2	5.643	558	562	565	rBV	1326456	1226305	20.69%	3.000%
3	6.631	727	730	734	rBV	1517231	1324211	22.34%	3.240%
4	6.790	753	757	760	rBV	1602016	1298649	21.91%	3.177%
5	7.025	793	797	800	rBV	1847404	1448797	24.44%	3.544%
6	7.178	820	823	827	rBV	1171740	950871	16.04%	2.326%
7	7.578	888	891	895	rBV	901543	794197	13.40%	1.943%
8	8.307	1011	1015	1019	rBV	2155733	1805551	30.46%	4.417%
9	8.884	1108	1113	1118	rBV2	88928	94471	1.59%	0.231%
10	9.384	1194	1198	1201	rBV	1472065	1243090	20.97%	3.041%
11	9.448	1206	1209	1213	rVV	153660	122873	2.07%	0.301%
12	9.636	1239	1241	1247	rBV2	87271	88145	1.49%	0.216%
13	9.772	1259	1264	1269	rVB2	171455	161876	2.73%	0.396%
14	9.984	1296	1300	1304	rVB	211919	166553	2.81%	0.407%
15	10.078	1312	1316	1319	rBV	1877271	1740295	29.36%	4.257%
16	10.107	1319	1321	1324	rVB	98667	71421	1.21%	0.175%
17	10.278	1346	1350	1353	rBV2	71595	68638	1.16%	0.168%
18	10.483	1380	1385	1388	rBV	261118	216330	3.65%	0.529%
19	10.625	1406	1409	1412	rVB	126771	104277	1.76%	0.255%
20	10.707	1418	1423	1425	rBV3	92350	112160	1.89%	0.274%
21	10.866	1446	1450	1454	rBV	797605	692999	11.69%	1.695%
22	10.960	1463	1466	1475	rVB	257032	298009	5.03%	0.729%
23	11.413	1540	1543	1545	rBV	199304	163783	2.76%	0.401%
24	11.572	1567	1570	1573	rBV	1856155	1754127	29.60%	4.291%
25	11.595	1573	1574	1578	rVB	745426	549581	9.27%	1.344%
26	11.648	1580	1583	1586	rVB	220489	169417	2.86%	0.414%
27	11.842	1613	1616	1618	rBV	145546	125306	2.11%	0.307%
28	11.942	1629	1633	1637	rVB	3500827	2789571	47.07%	6.824%
29	12.078	1653	1656	1658	rBV	123729	111589	1.88%	0.273%
30	12.107	1658	1661	1664	rVB	127564	116564	1.97%	0.285%
31	12.154	1665	1669	1672	rBV	70932	75643	1.28%	0.185%
32	12.195	1672	1676	1678	rBV2	168373	196466	3.31%	0.481%
33	12.248	1682	1685	1690	rBV	144473	141503	2.39%	0.346%
34	12.636	1747	1751	1753	rBV	5834645	5848880	98.68%	14.308%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081318\
Data File : BF108121.D
Acq On : 13 Aug 2018 17:32
Operator : JU/SJ
Sample : J4282-03RE 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-080918-BRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.660	1753	1755	1762	rVB	6878233	5926969	100.00%	14.500%
36	12.742	1765	1769	1772	rVB	1325202	1172058	19.77%	2.867%
37	12.795	1775	1778	1781	rBV	1074503	931005	15.71%	2.278%
38	12.977	1806	1809	1812	rVB	265367	229572	3.87%	0.562%
39	13.030	1815	1818	1823	rVB	964975	902837	15.23%	2.209%
40	13.160	1836	1840	1843	rBV	1285710	1085785	18.32%	2.656%
41	13.183	1843	1844	1847	rVB	97127	77708	1.31%	0.190%
42	13.307	1862	1865	1867	rBV2	170088	171522	2.89%	0.420%
43	13.342	1867	1871	1875	rVV3	185107	367362	6.20%	0.899%
44	13.424	1883	1885	1888	rVB	116734	88841	1.50%	0.217%
45	13.466	1889	1892	1895	rVV3	207319	196096	3.31%	0.480%
46	13.907	1962	1967	1970	rVB3	241754	346988	5.85%	0.849%
47	14.236	2018	2023	2025	rBV2	1597744	1793038	30.25%	4.386%
48	14.260	2025	2027	2032	rVB	377017	328162	5.54%	0.803%
49	15.813	2287	2291	2296	rBV	720298	954893	16.11%	2.336%


Sum of corrected areas: 40877006

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081318\
Data File : BF108121.D
Acq On : 13 Aug 2018 17:32
Operator : JU/SJ
Sample : J4282-03RE 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-080918-BRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

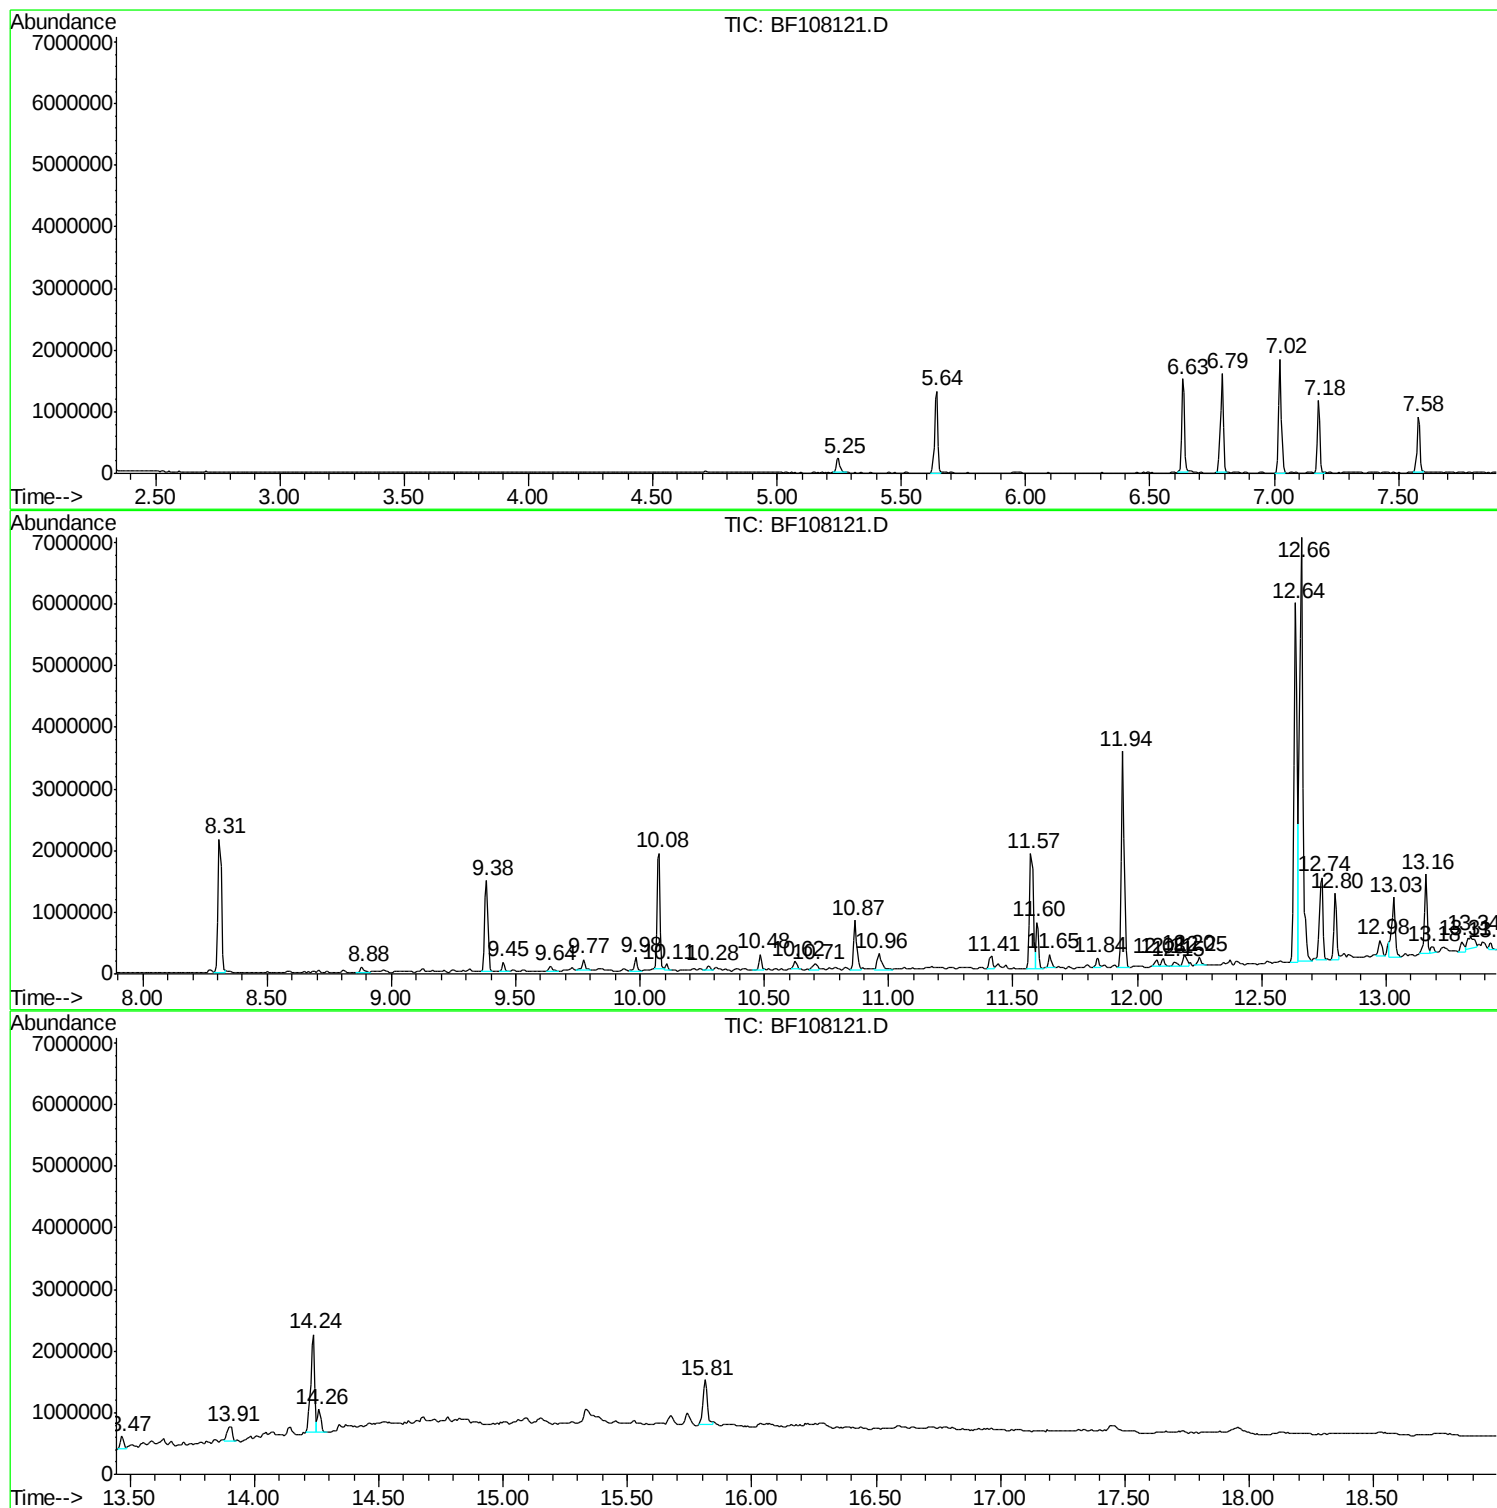

DbaaaPathh::ZZ\SS00SSRVNPE000001BBNAFNDATAAB0003338\
 DbaaaFile::BBE003221DD
 Aeqq00n ::133Aagg20038 177322
 Oppaaaor ::JUUSJ
 Sample ::J4282200BRE5X
 Misc ::
 ASSVaal ::14 SampleMMultiplicier:11

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-080918-BRE

QqaantMebbdd::ZZ\SS00SSRVNPE000001BBNAFMEH00SS82Z00BB000038MM
 QqaantFile ::ASBPBNASSANDABBSF00R55P000NTCAIBRATION

TICCLibbaay ::CC\DATAABASSEN0\$T11LL
 TICInteggaionPaaaecess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
