


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081318\
 Data File : BF108108.D
 Acq On : 13 Aug 2018 11:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

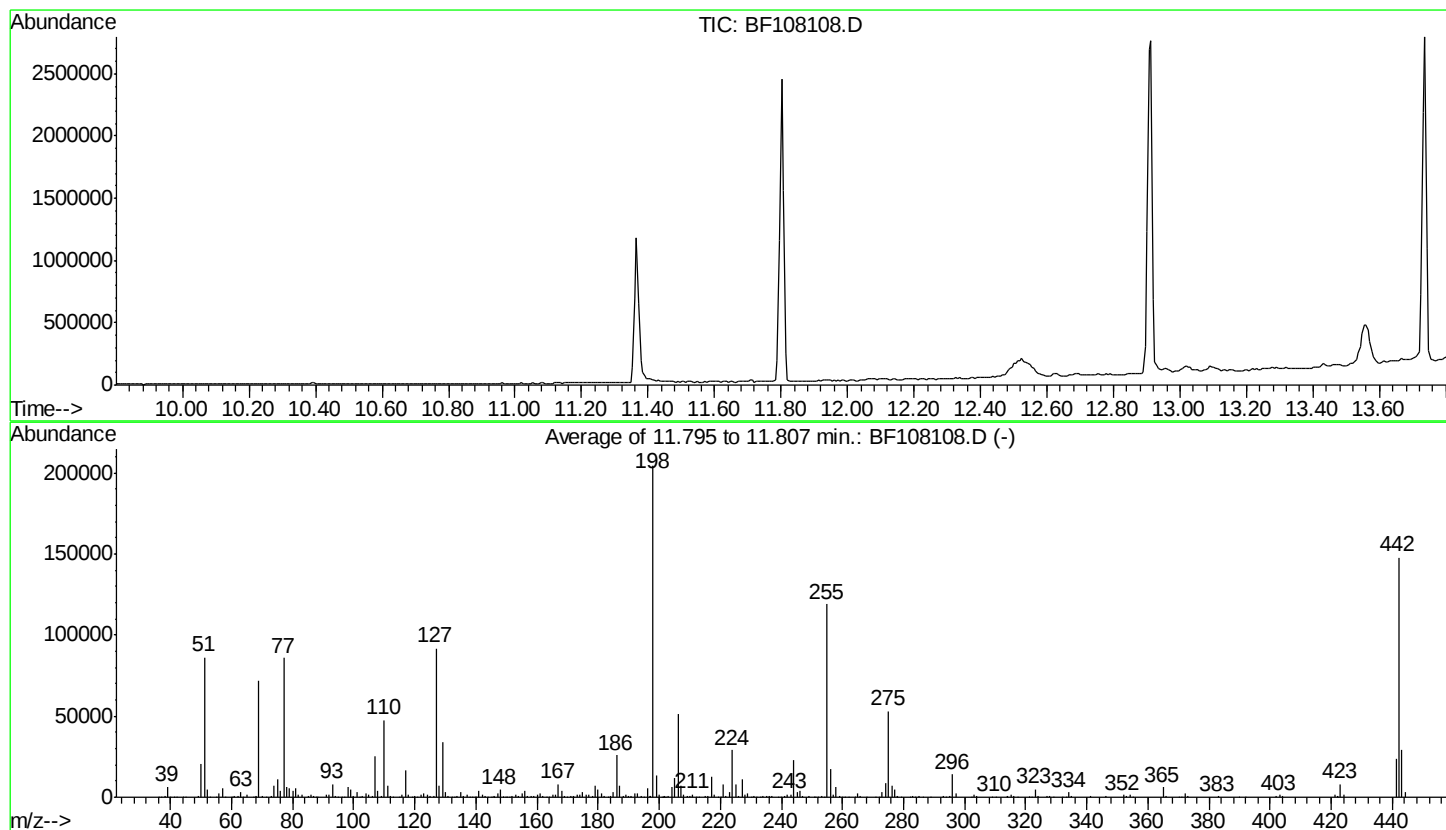

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	86416	PASS
68	69	0.00	2	1.1	823	PASS
69	198	0.00	100	35.1	71681	PASS
70	69	0.00	2	0.7	521	PASS
127	198	10	80	44.9	91770	PASS
197	198	0.00	2	0.5	1104	PASS
198	198	100	100	100.0	204416	PASS
199	198	5	9	6.7	13793	PASS
275	198	10	60	26.0	53125	PASS
365	198	1	100	3.1	6284	PASS
441	198	0.01	100	11.7	24008	PASS
442	198	50	100	72.4	147957	PASS
443	442	15	24	19.5	28854	PASS