
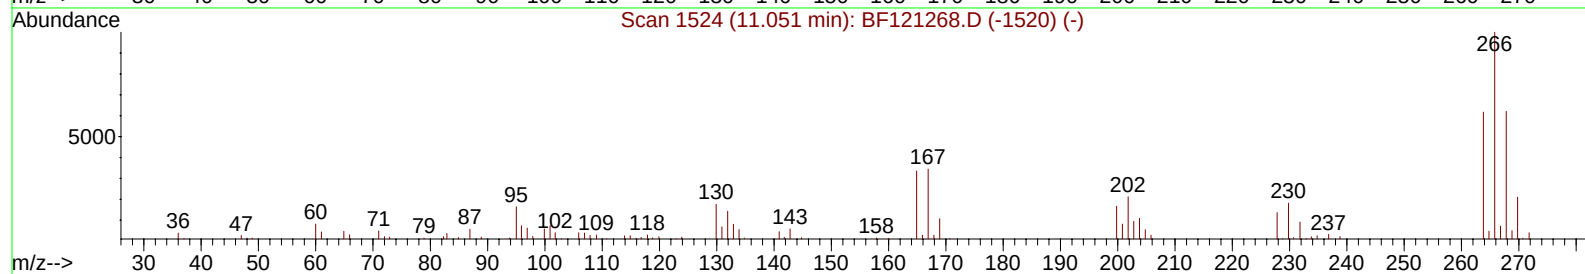
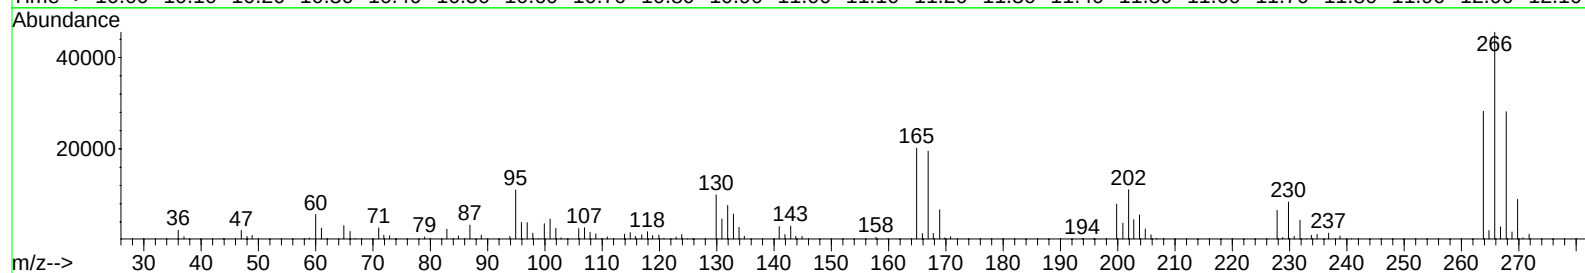


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081320\  
 Data File : BF121264.D  
 Acq On : 13 Aug 2020 10:30  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 18:09:19 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Aug 13 15:23:26 2020  
 Response via : Initial Calibration

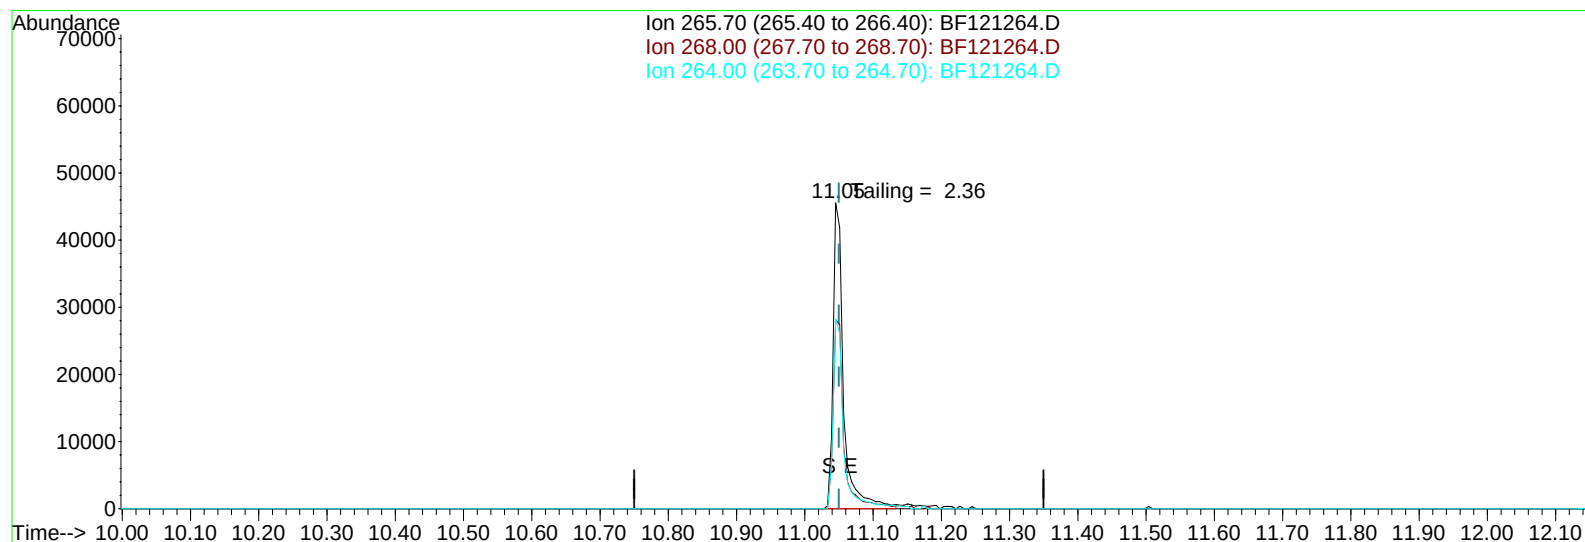

TIC: BF121264.D

(70) Pentachlorophenol (C)




11.045min (-0.005) 57394.28ng

response 48713

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.70 | 61.75 |
| 264.00 | 63.30 | 62.05 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081320\  
 Data File : BF121264.D  
 Acq On : 13 Aug 2020 10:30  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 18:09:19 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Aug 13 15:23:26 2020  
 Response via : Initial Calibration

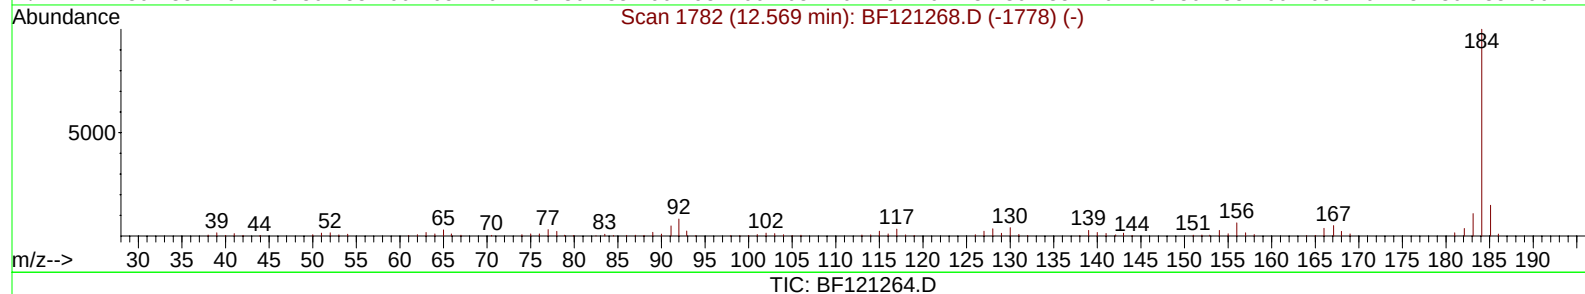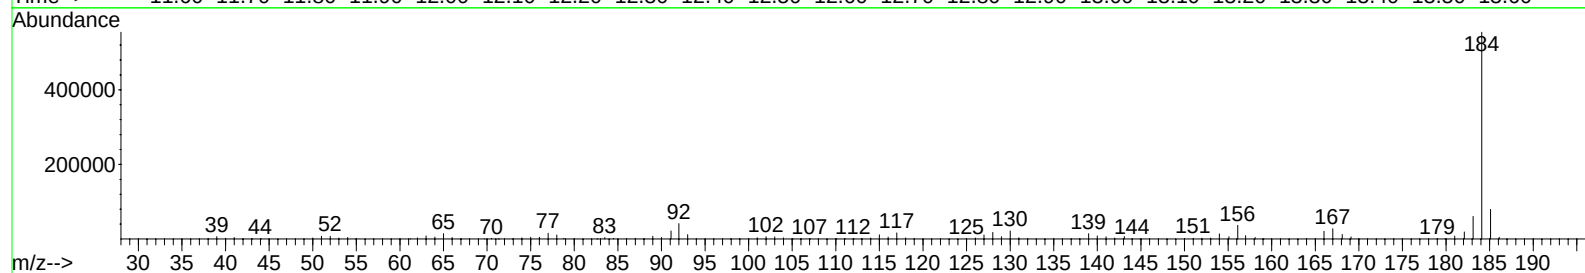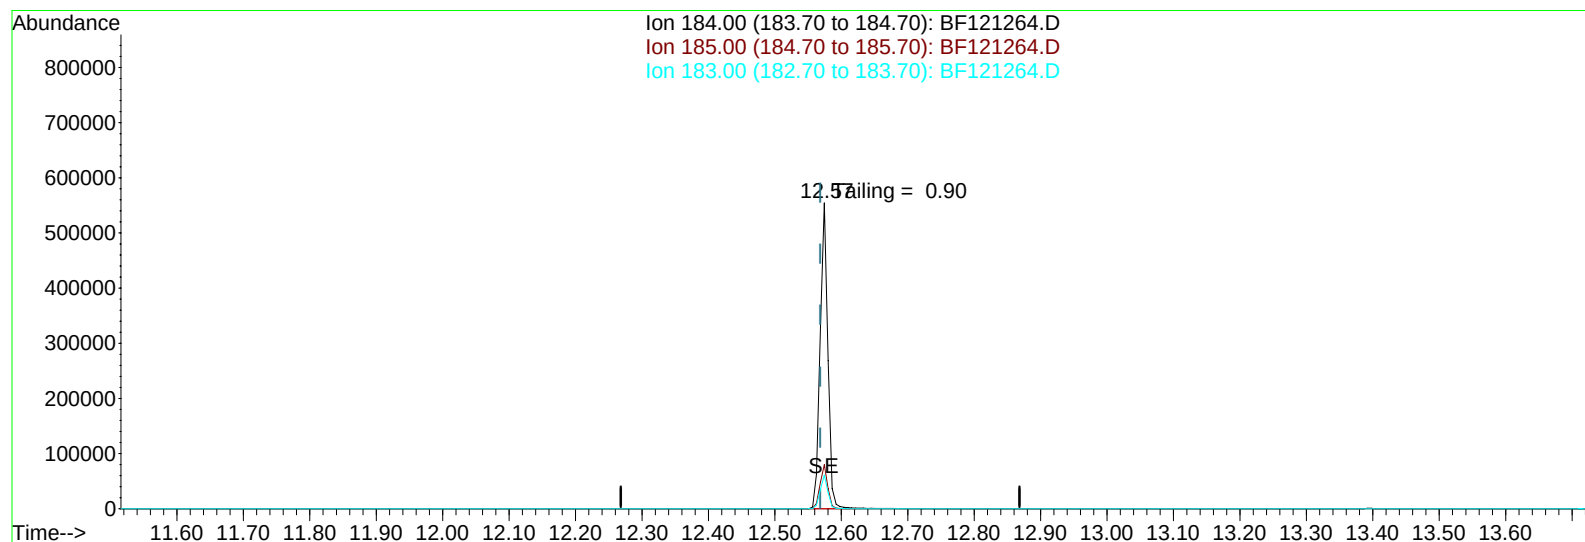

(77) Benzidine

12.574min (+0.006) 0.00ng

response 453218

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.80 | 14.41 |
| 183.00 | 10.40 | 10.99 |
| 0.00   | 0.00  | 0.00  |